

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
 Data File : BN033391.D
 Acq On : 14 Aug 2024 21:11
 Operator : MA/JU
 Sample : P3481-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0AE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN033391.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	25	29	36	rVB	56799	75781	1.11%	0.092%
2	3.405	68	71	84	rBV	148784	217871	3.18%	0.266%
3	3.540	90	94	110	rBV	567038	859039	12.56%	1.048%
4	3.864	145	149	155	rBV	17121	22953	0.34%	0.028%
5	4.505	254	258	259	rBV3	6774	8235	0.12%	0.010%
6	4.746	293	299	303	rBV6	7297	11710	0.17%	0.014%
7	4.958	331	335	344	rBV	6540	13972	0.20%	0.017%
8	5.699	454	461	468	rVB3	9930	19672	0.29%	0.024%
9	6.575	606	610	615	rBV3	10140	14939	0.22%	0.018%
10	6.746	632	639	648	rBV	1146147	1797263	26.27%	2.192%
11	6.869	656	660	662	rBV2	11314	15642	0.23%	0.019%
12	6.916	662	668	676	rVB	973254	1430462	20.91%	1.745%
13	7.105	693	700	708	rBV	1197376	1803045	26.35%	2.199%
14	7.181	708	713	724	rVB	178834	272731	3.99%	0.333%
15	7.569	771	779	787	rBV	1482046	2264507	33.10%	2.762%
16	7.646	787	792	797	rBV4	12566	19723	0.29%	0.024%
17	7.869	826	830	835	rBV6	7733	12114	0.18%	0.015%
18	8.269	890	898	907	rBV	1503555	2351170	34.36%	2.868%
19	8.710	965	973	982	rBV	1095661	1779536	26.01%	2.170%
20	8.840	991	995	999	rVB6	7249	12846	0.19%	0.016%
21	8.893	999	1004	1008	rBV6	9276	15243	0.22%	0.019%
22	9.193	1051	1055	1060	rVB7	7141	11719	0.17%	0.014%
23	9.287	1065	1071	1077	rBV	57942	88061	1.29%	0.107%
24	9.422	1084	1094	1104	rBV	828505	1328586	19.42%	1.620%
25	9.663	1130	1135	1142	rBV7	9769	17800	0.26%	0.022%
26	9.958	1178	1185	1194	rBV	1482385	2360823	34.51%	2.879%
27	10.134	1211	1215	1219	rVB4	9038	14265	0.21%	0.017%
28	10.334	1240	1249	1257	rBV	2186938	3572822	52.22%	4.357%
29	10.469	1264	1272	1281	rBV	929207	1493407	21.83%	1.821%
30	10.699	1306	1311	1315	rBV7	4413	9499	0.14%	0.012%
31	10.816	1327	1331	1336	rVB8	4267	7277	0.11%	0.009%
32	10.893	1339	1344	1353	rBV	46319	69581	1.02%	0.085%
33	11.081	1369	1376	1383	rBV	333718	548237	8.01%	0.669%
34	11.140	1383	1386	1390	rVB4	12383	18119	0.26%	0.022%
35	11.852	1501	1507	1510	rBV5	6140	9534	0.14%	0.012%
36	11.928	1515	1520	1526	rVB2	32721	55882	0.82%	0.068%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
 Data File : BN033391.D
 Acq On : 14 Aug 2024 21:11
 Operator : MA/JU
 Sample : P3481-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0AE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
 Title : SVOA CALIBRATION

37	12.204	1565	1567	1577	rVB4	6183	9378	0.14%	0.011%
38	12.569	1625	1629	1635	rBV5	9885	14291	0.21%	0.017%
39	12.828	1668	1673	1676	rBV2	11475	14201	0.21%	0.017%
40	13.199	1731	1736	1739	rVB7	5307	9443	0.14%	0.012%

41	13.428	1770	1775	1782	rBV5	17279	25817	0.38%	0.031%
42	13.628	1803	1809	1816	rBV	2533501	3445013	50.35%	4.202%
43	13.734	1824	1827	1831	rVB6	5416	7797	0.11%	0.010%
44	13.898	1847	1855	1861	rBV	2900036	4332628	63.33%	5.284%
45	14.210	1900	1908	1915	rBV	3334365	4894571	71.54%	5.970%

46	14.410	1932	1942	1946	rBV	948142	1381714	20.20%	1.685%
47	14.446	1946	1948	1949	rVV	187434	188036	2.75%	0.229%
48	14.463	1949	1951	1961	rVB	214627	256539	3.75%	0.313%
49	14.569	1966	1969	1974	rVB6	7755	12459	0.18%	0.015%
50	14.634	1976	1980	1982	rBV5	9223	12946	0.19%	0.016%

51	14.740	1994	1998	2001	rBV3	14050	18349	0.27%	0.022%
52	15.051	2047	2051	2057	rVB3	14000	20272	0.30%	0.025%
53	15.110	2057	2061	2065	rBV5	6879	8658	0.13%	0.011%
54	15.210	2071	2078	2091	rBV	3563323	5232973	76.48%	6.382%
55	15.322	2091	2097	2103	rBV	619157	854967	12.50%	1.043%

56	15.445	2114	2118	2123	rVB2	21702	29975	0.44%	0.037%
57	15.522	2128	2131	2136	rVB6	6969	9533	0.14%	0.012%
58	15.598	2141	2144	2151	rVV9	5384	8889	0.13%	0.011%
59	15.792	2170	2177	2183	rBV3	51685	79995	1.17%	0.098%
60	15.910	2194	2197	2202	rVB2	11887	15801	0.23%	0.019%

61	15.969	2204	2207	2209	rVV4	11449	13736	0.20%	0.017%
62	15.998	2209	2212	2220	rVB5	20000	36274	0.53%	0.044%
63	16.128	2231	2234	2239	rVV6	11615	16699	0.24%	0.020%
64	16.392	2275	2279	2283	rBV3	26255	35417	0.52%	0.043%
65	16.822	2348	2352	2359	rVB3	20776	36691	0.54%	0.045%

66	16.957	2365	2375	2382	rBV	4202916	5817518	85.03%	7.095%
67	17.057	2385	2392	2404	rVV	3988153	5606822	81.95%	6.838%
68	17.163	2407	2410	2416	rVB7	26441	38741	0.57%	0.047%
69	17.345	2436	2441	2450	rBV	107338	177373	2.59%	0.216%
70	17.675	2493	2497	2503	rVB2	79546	103594	1.51%	0.126%

71	17.757	2508	2511	2515	rBV6	26458	42395	0.62%	0.052%
72	17.892	2529	2534	2541	rBV	490563	675051	9.87%	0.823%
73	18.857	2695	2698	2702	rVB3	46166	56040	0.82%	0.068%
74	18.922	2705	2709	2714	rVB	60155	82143	1.20%	0.100%
75	18.992	2717	2721	2724	rBV	67384	98806	1.44%	0.121%

76	19.181	2749	2753	2759	rBV	161223	263342	3.85%	0.321%
----	--------	------	------	------	-----	--------	--------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
Data File : BN033391.D
Acq On : 14 Aug 2024 21:11
Operator : MA/JU
Sample : P3481-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AE5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
Title : SVOA CALIBRATION

77	19.357	2777	2783	2789	rBV	4989139	6841858	100.00%	8.344%
78	19.416	2790	2793	2798	rVB	411500	553674	8.09%	0.675%
79	20.416	2959	2963	2969	rBV	270071	313842	4.59%	0.383%
80	20.922	3045	3049	3055	rBV2	309569	429257	6.27%	0.524%
81	21.192	3089	3095	3105	rVB	4230966	6087673	88.98%	7.425%
82	22.769	3359	3363	3370	rVB2	99477	163681	2.39%	0.200%
83	23.827	3535	3543	3559	rVB	2429543	5590168	81.71%	6.818%
84	24.021	3567	3576	3588	rVB	2331692	5403744	78.98%	6.591%




Sum of corrected areas: 81992850

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
Data File : BN033391.D
Acq On : 14 Aug 2024 21:11
Operator : MA/JU
Sample : P3481-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AE5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

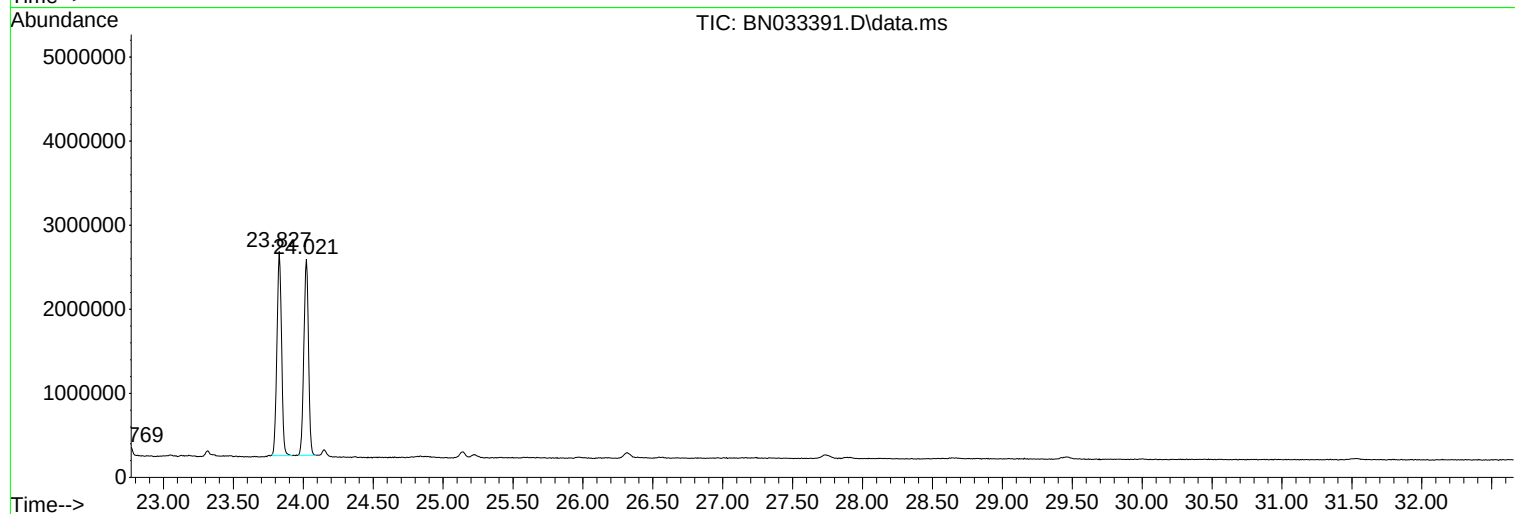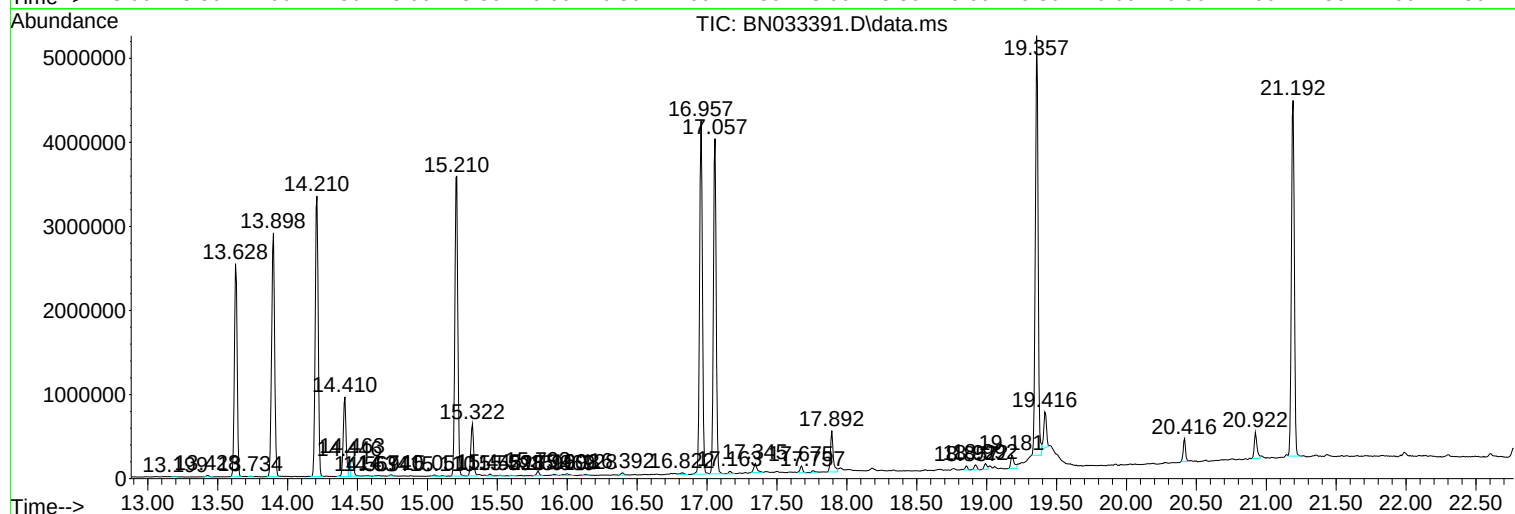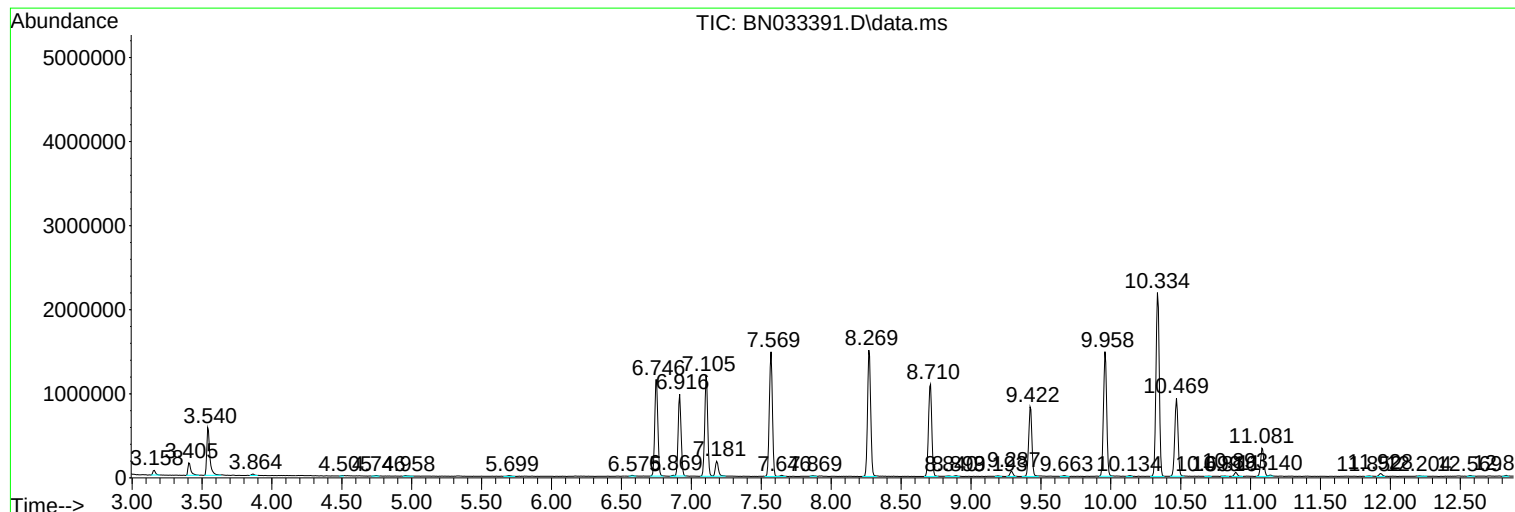

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
Data File : BN033391.D
Acq On : 14 Aug 2024 21:11
Operator : MA/JU
Sample : P3481-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AE5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
Data File : BN033391.D
Acq On : 14 Aug 2024 21:11
Operator : MA/JU
Sample : P3481-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AE5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc