

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081518\
 Data File : BN002340.D
 Acq On : 15 Aug 2018 18:17
 Operator : JU/SJ
 Sample : PB112090BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK90

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.852	652	657	670	rBV	393423	664377	16.58%	1.713%
2	7.016	679	685	699	rBV	344357	561307	14.01%	1.447%
3	7.210	713	718	734	rVB	419127	696995	17.39%	1.797%
4	7.675	791	797	810	rVB	560369	932921	23.28%	2.405%
5	8.381	911	917	933	rVB	526675	875143	21.84%	2.256%
6	8.822	986	992	1005	rBV	446863	774262	19.32%	1.996%
7	9.540	1108	1114	1124	rBV	355678	604640	15.09%	1.559%
8	10.075	1199	1205	1222	rBV	481644	864333	21.57%	2.228%
9	10.446	1261	1268	1279	rBV	847101	1467344	36.61%	3.783%
10	10.587	1286	1292	1305	rBV	536898	1000112	24.95%	2.578%
11	13.722	1819	1825	1835	rBV	1322432	1828596	45.63%	4.714%
12	13.998	1865	1872	1885	rBV	1382891	2043385	50.99%	5.268%
13	14.310	1918	1925	1933	rBV2	1373797	2116919	52.82%	5.457%
14	14.522	1956	1961	1981	rBV	436973	770832	19.23%	1.987%
15	15.304	2088	2094	2102	rBV	1822017	2631797	65.67%	6.784%
16	15.439	2111	2117	2128	rBV	496477	759216	18.94%	1.957%
17	17.057	2386	2392	2402	rBV	1918998	2625565	65.51%	6.768%
18	17.157	2403	2409	2421	rVV	2074365	2980181	74.36%	7.682%
19	19.457	2794	2800	2811	rBV	2611379	3512207	87.63%	9.054%
20	21.257	3100	3106	3121	rBV	2643480	3337628	83.28%	8.604%
21	22.815	3368	3371	3377	rVB2	39254	58384	1.46%	0.151%
22	23.339	3453	3460	3473	rBV2	2133381	4007785	100.00%	10.331%
23	23.480	3477	3484	3496	rVB	1788210	3460340	86.34%	8.920%
24	24.010	3569	3574	3581	rBV3	57892	102564	2.56%	0.264%
25	24.745	3694	3699	3705	rVB3	58302	115434	2.88%	0.298%


Sum of corrected areas: 38792267

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081518\
Data File : BN002340.D
Acq On : 15 Aug 2018 18:17
Operator : JU/SJ
Sample : PB112090BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK90

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

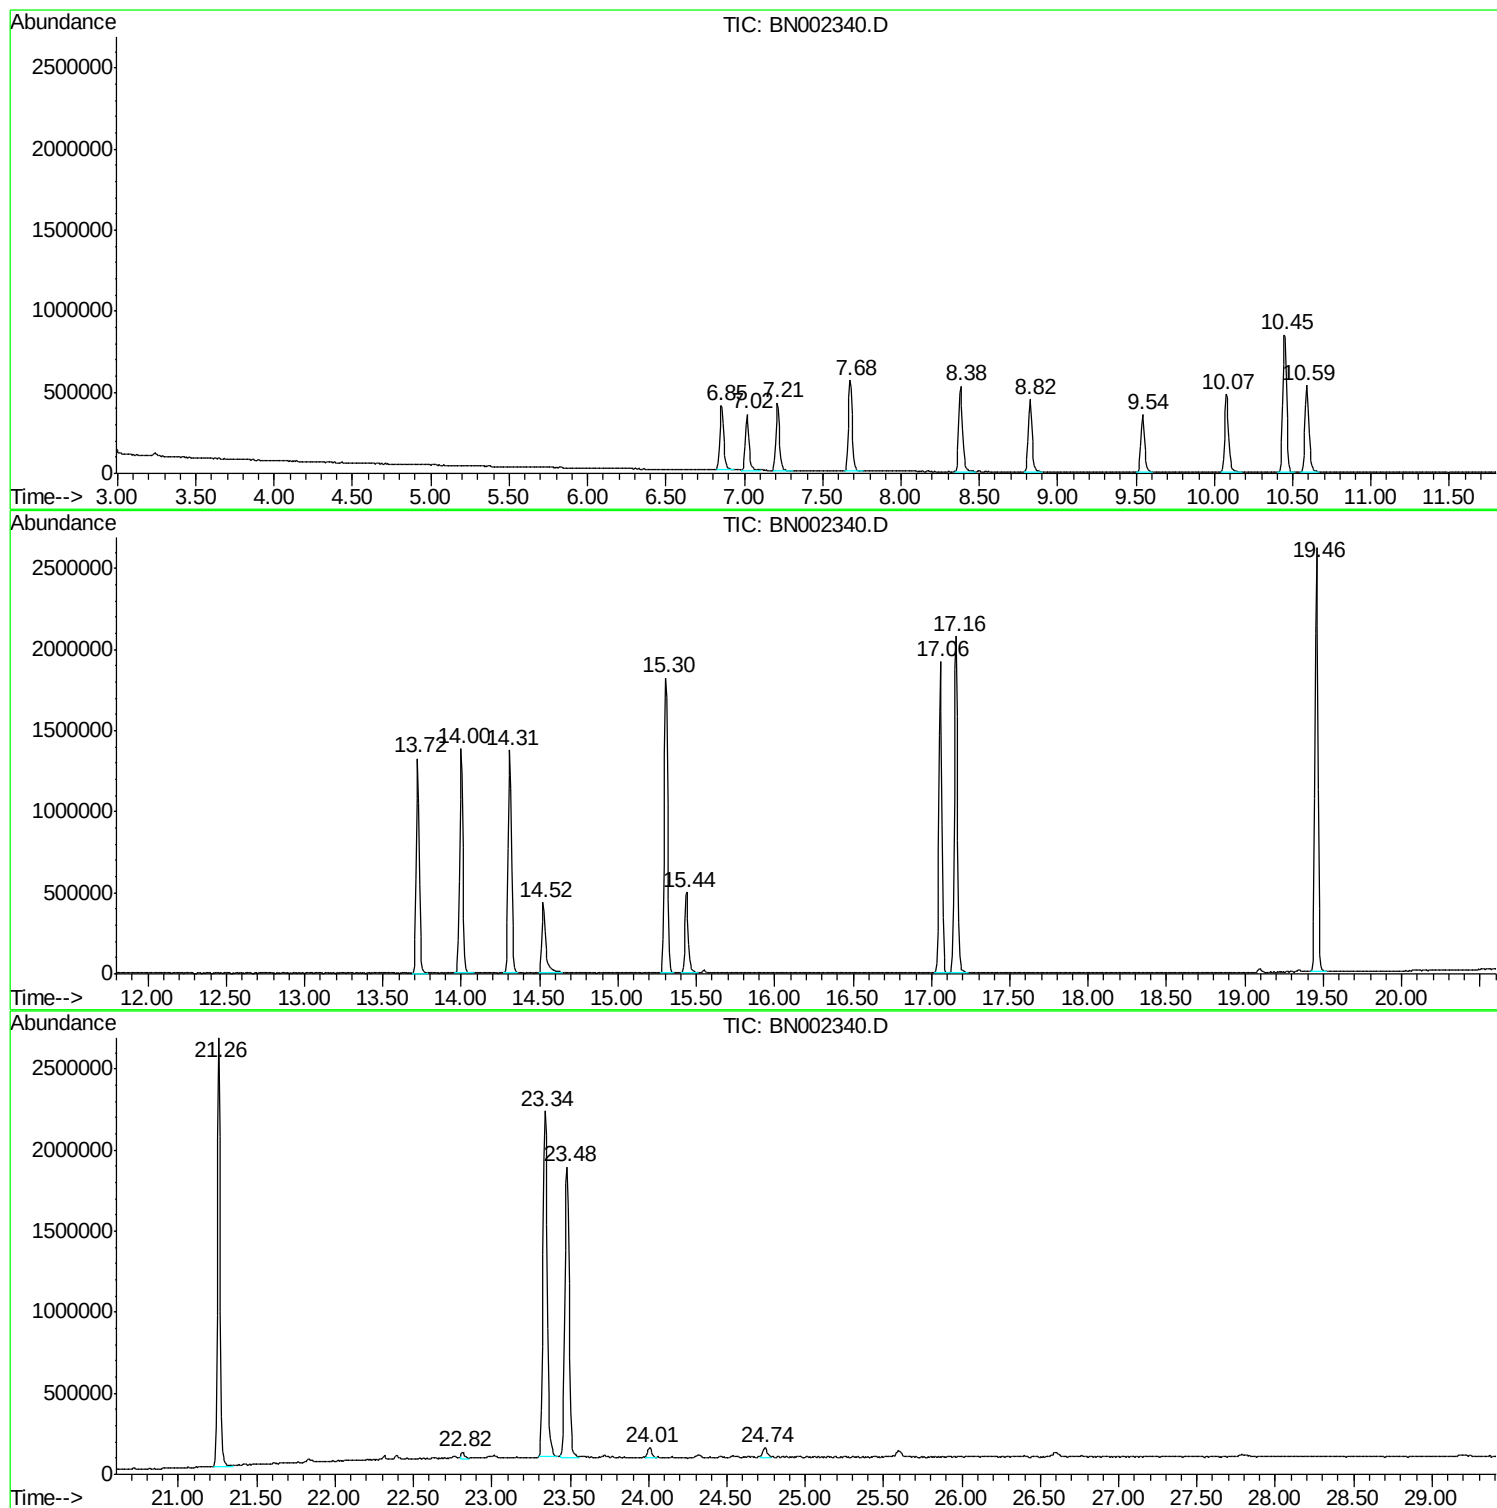

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081518\
Data File : BN002340.D
Acq On : 15 Aug 2018 18:17
Operator : JU/SJ
Sample : PB112090BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK90

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081518\
Data File : BN002340.D
Acq On : 15 Aug 2018 18:17
Operator : JU/SJ
Sample : PB112090BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK90

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc