

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081523\
 Data File : BN026902.D
 Acq On : 15 Aug 2023 15:40
 Operator : MA/JU
 Sample : PB154811BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK811

Quant Time: Aug 16 00:54:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 00:50:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	10472	0.400	ng/ul	0.00
4) Naphthalene-d8	10.938	136	34373	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.735	164	20437	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.481	188	45540	0.400	ng/ul	0.00
17) Chrysene-d12	21.659	240	33907	0.400	ng/ul	0.00
23) Perylene-d12	24.211	264	41592	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.443	96	62835	5.054	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.511	152	14585	0.288	ng/ul	0.00
18) Fluoranthene-d10	19.497	212	36172	0.338	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.725	166	5453	0.061	ng/ul#	13
20) Pyrene	19.864	202	5309	0.035	ng/ul#	1
26) Benzo(a)pyrene	24.047	252	12842	0.090	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081523\
Data File : BN026902.D
Acq On : 15 Aug 2023 15:40
Operator : MA/JU
Sample : PB154811BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK811

Quant Time: Aug 16 00:54:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 00:50:05 2023
Response via : Initial Calibration




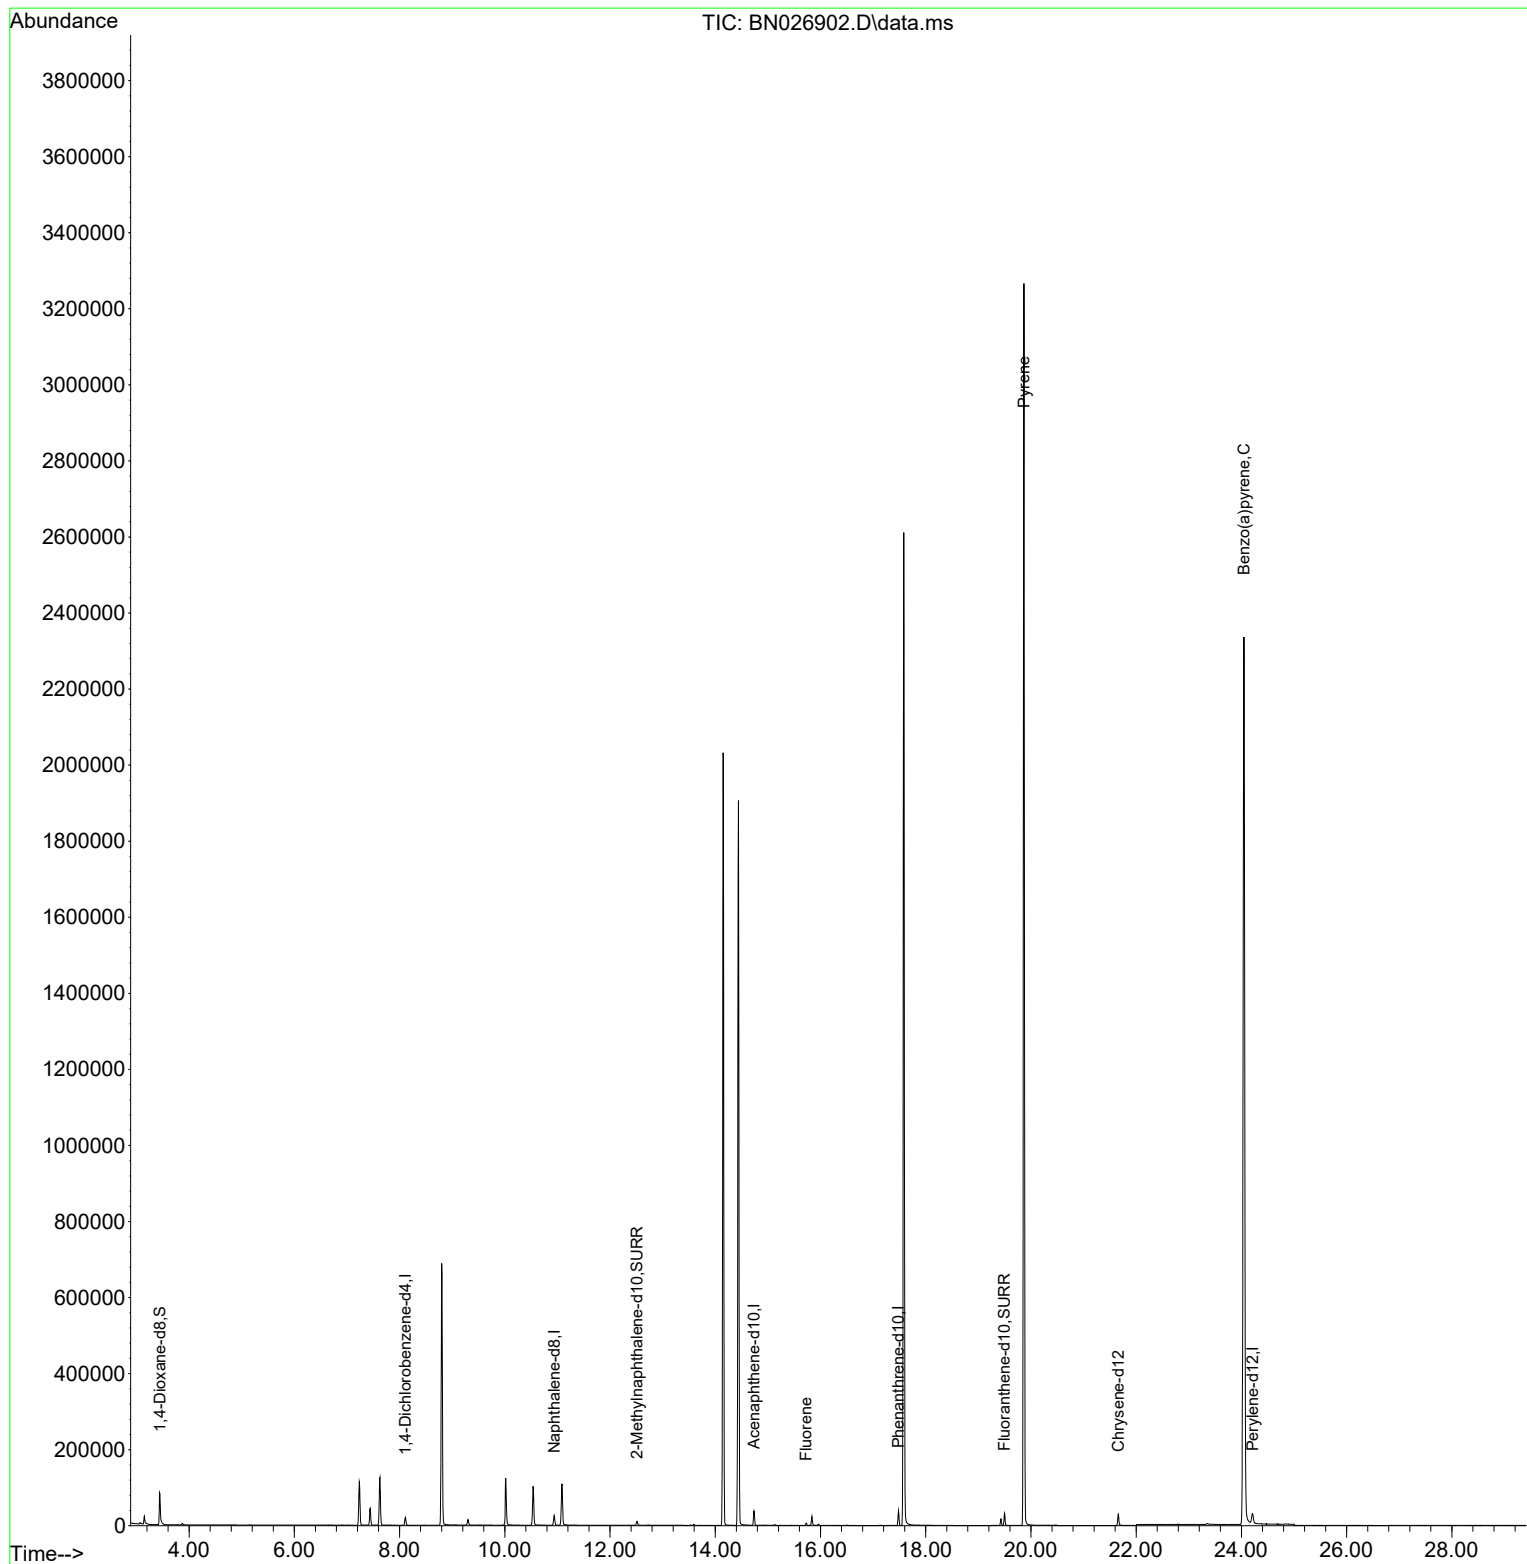


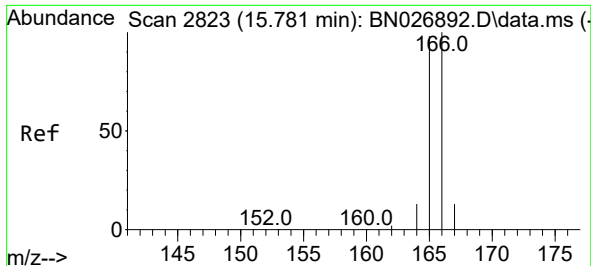

#12
Fluorene
Concen: 0.061 ng/ul
RT: 15.725 min Scan# 2811
Delta R.T. -0.055 min
Lab File: BN026902.D
Acq: 15 Aug 2023 15:40




Instrument :
BNA_N
ClientSampleId :
SBLK811


Tgt Ion:166 Resp: 5453
Ion Ratio Lower Upper
166 100
165 6.1 79.1 118.7#
167 31.8 11.4 17.0#

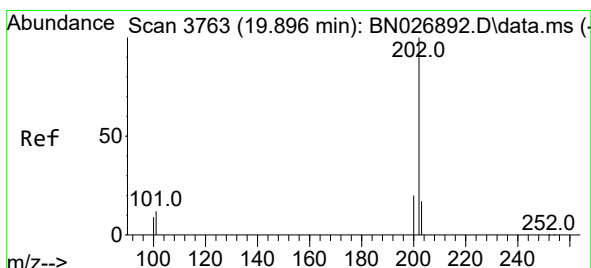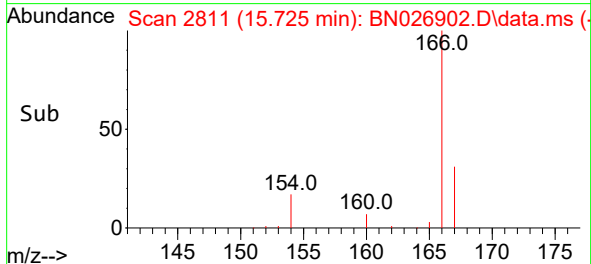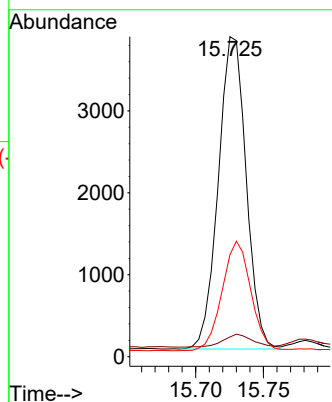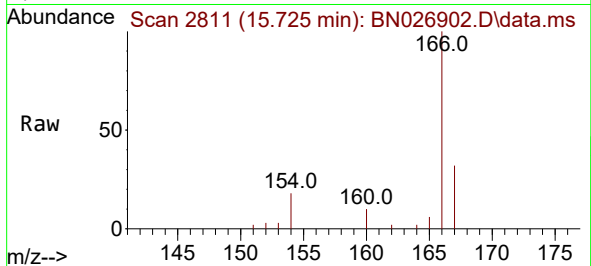

#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.864 min Scan# 3756
Delta R.T. -0.032 min
Lab File: BN026902.D
Acq: 15 Aug 2023 15:40


Tgt Ion:202 Resp: 5309
Ion Ratio Lower Upper
202 100
101 152.3 10.7 16.1#
100 1167.4 8.5 12.7#

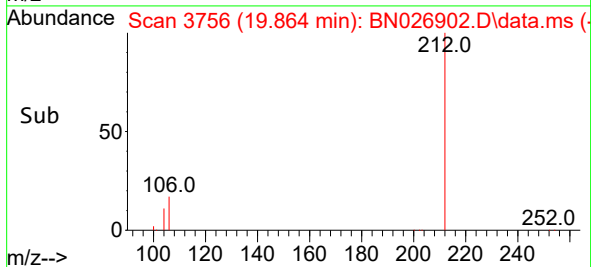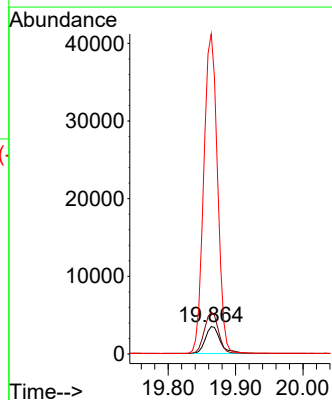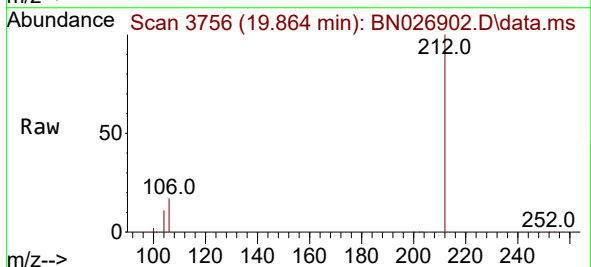

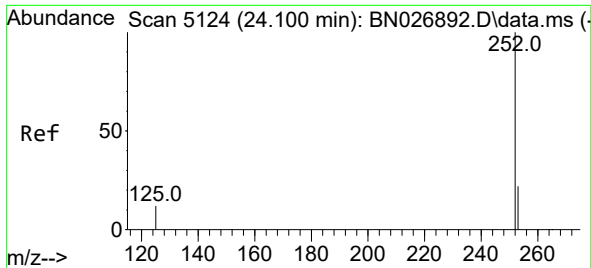

#26
Benzo(a)pyrene
Concen: 0.090 ng/ul
RT: 24.047 min Scan# 51
Delta R.T. -0.053 min
Lab File: BN026902.D
Acq: 15 Aug 2023 15:40

Instrument :
BNA_N
ClientSampleId :
SBLK811

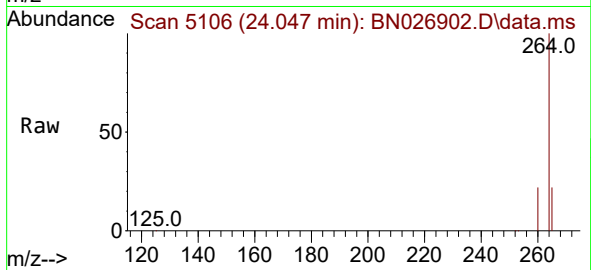

Tgt Ion:252 Resp: 12842
Ion Ratio Lower Upper
252 100
253 34.7 19.0 28.6#
125 37.8 11.4 17.0#

