

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081523\
 Data File : BN026911.D
 Acq On : 15 Aug 2023 21:54
 Operator : MA/JU
 Sample : PB154774BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK774

Quant Time: Aug 16 00:55:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 00:50:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	15154	0.400	ng/ul	0.00
4) Naphthalene-d8	10.938	136	51299	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.735	164	30195	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.481	188	66697	0.400	ng/ul	0.00
17) Chrysene-d12	21.653	240	62683	0.400	ng/ul	0.00
23) Perylene-d12	24.199	264	68790	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.444	96	60475	3.361	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.511	152	15882	0.210	ng/ul	0.00
18) Fluoranthene-d10	19.496	212	39079	0.197	ng/ul	0.00
Target Compounds						
					Qvalue	
26) Benzo(a)pyrene	24.041	252	12003	0.051	ng/ul#	26


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081523\
Data File : BN026911.D
Acq On : 15 Aug 2023 21:54
Operator : MA/JU
Sample : PB154774BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK774


Quant Time: Aug 16 00:55:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 00:50:05 2023
Response via : Initial Calibration

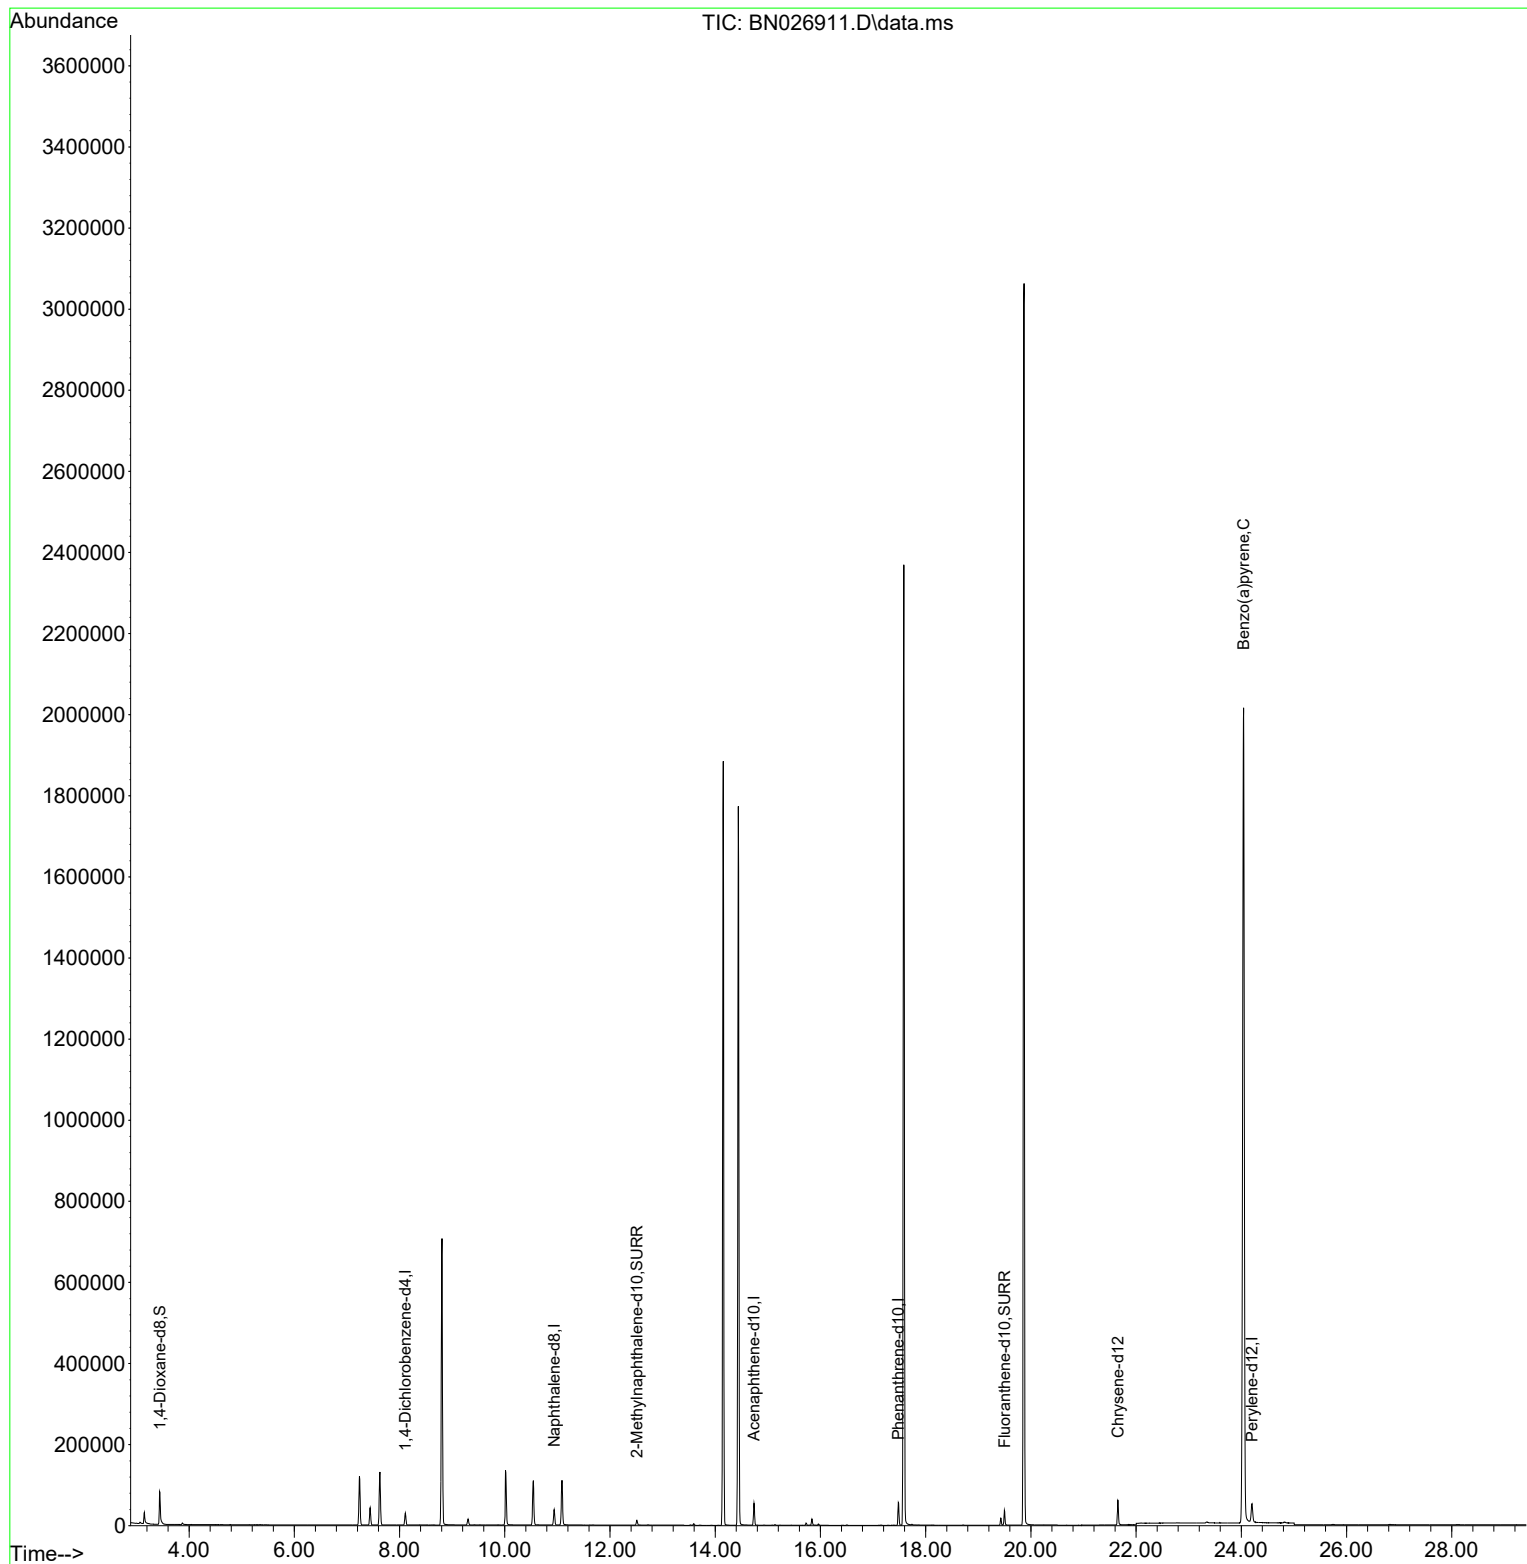

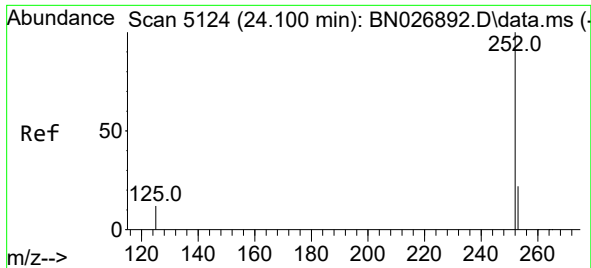

#26
Benzo(a)pyrene
Concen: 0.051 ng/ul
RT: 24.041 min Scan# 51
Delta R.T. -0.059 min
Lab File: BN026911.D
Acq: 15 Aug 2023 21:54

Instrument :
BNA_N
ClientSampleId :
SBLK774

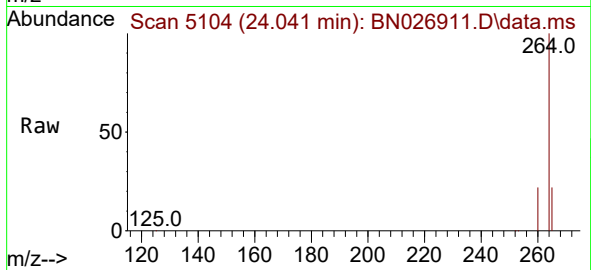

Tgt Ion:252 Resp: 12003
Ion Ratio Lower Upper
252 100
253 43.8 19.0 28.6#
125 67.3 11.4 17.0#

