




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081523\
 Data File : BN026899.D
 Acq On : 15 Aug 2023 13:49
 Operator : MA/JU
 Sample : 03967-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A48A0

Manual IntegrationsAPPROVED

Quant Time: Aug 16 00:53:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 00:50:05 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/16/2023
 Supervised By :Sohil Jodhani 08/16/2023

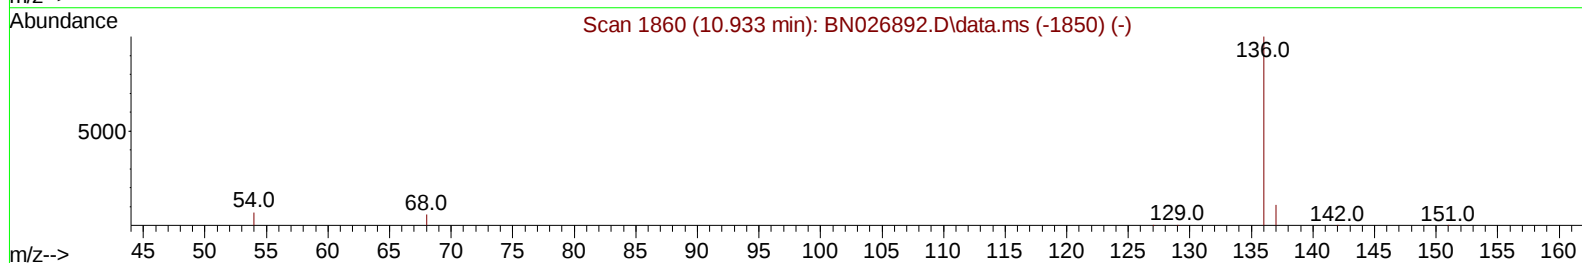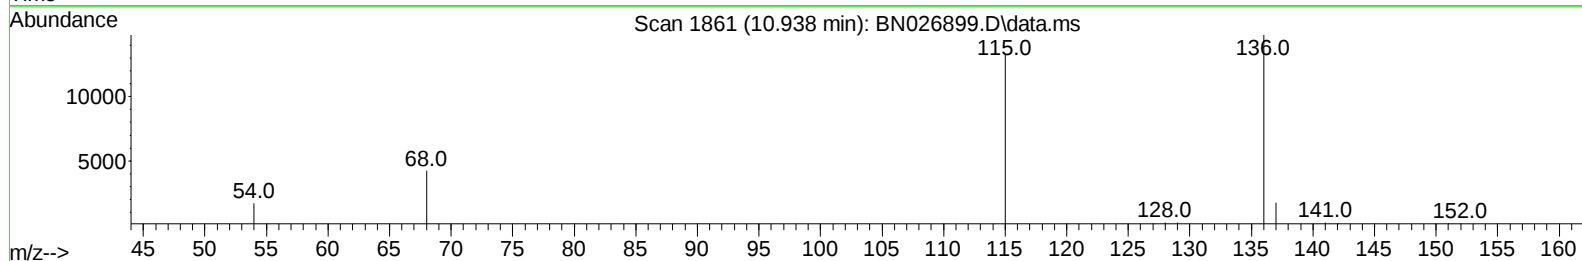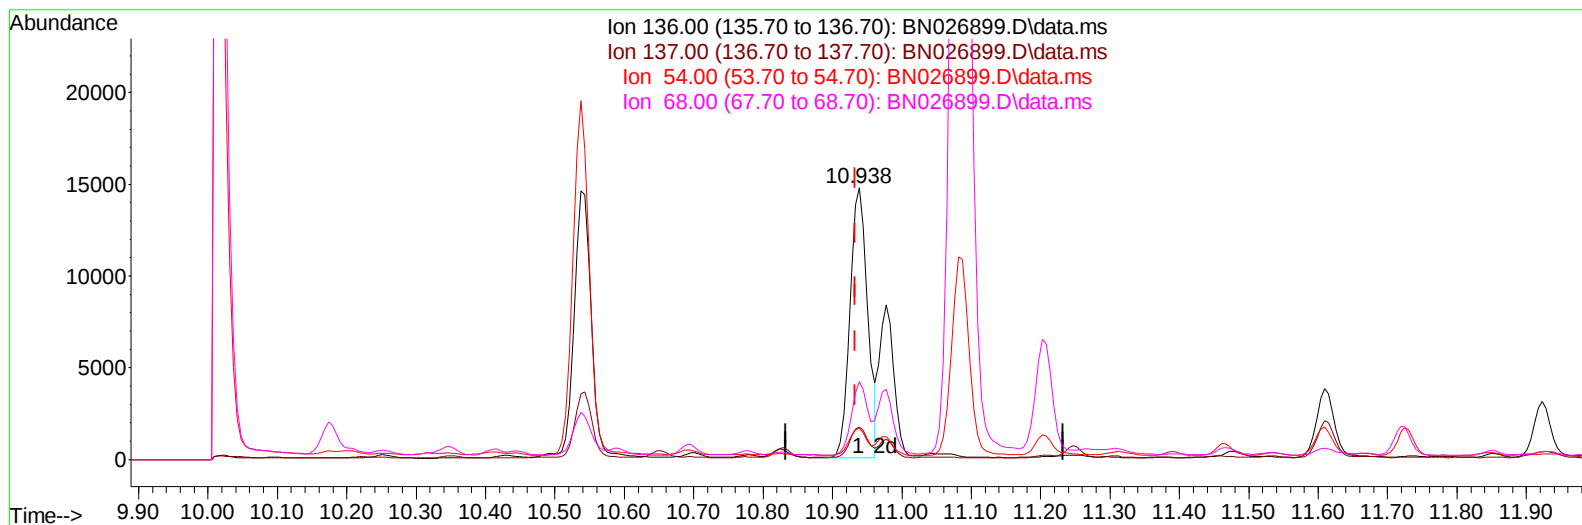

TIC: BN026899.D\data.ms

(4) Naphthalene-d8 (I)

10.938min (+ 0.006) 0.40 ng/u1

response 25765

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	11.50	11.92
54.00	7.50	11.44#
68.00	6.80	28.55#




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081523\
 Data File : BN026899.D
 Acq On : 15 Aug 2023 13:49
 Operator : MA/JU
 Sample : 03967-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A48A0

Manual IntegrationsAPPROVED

Quant Time: Aug 16 00:53:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 00:50:05 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/16/2023
 Supervised By :Sohil Jodhani 08/16/2023

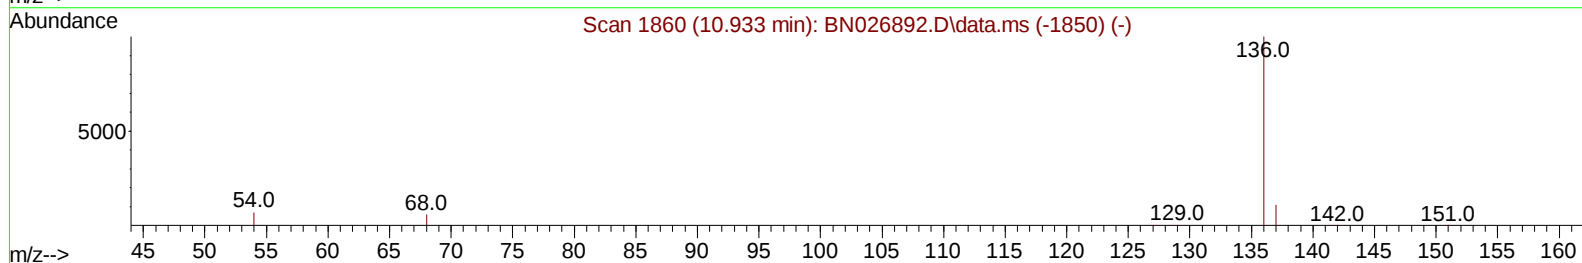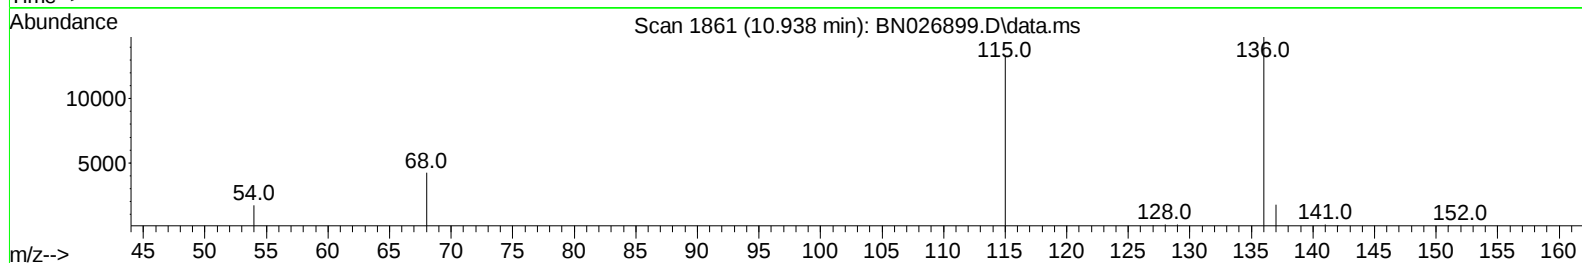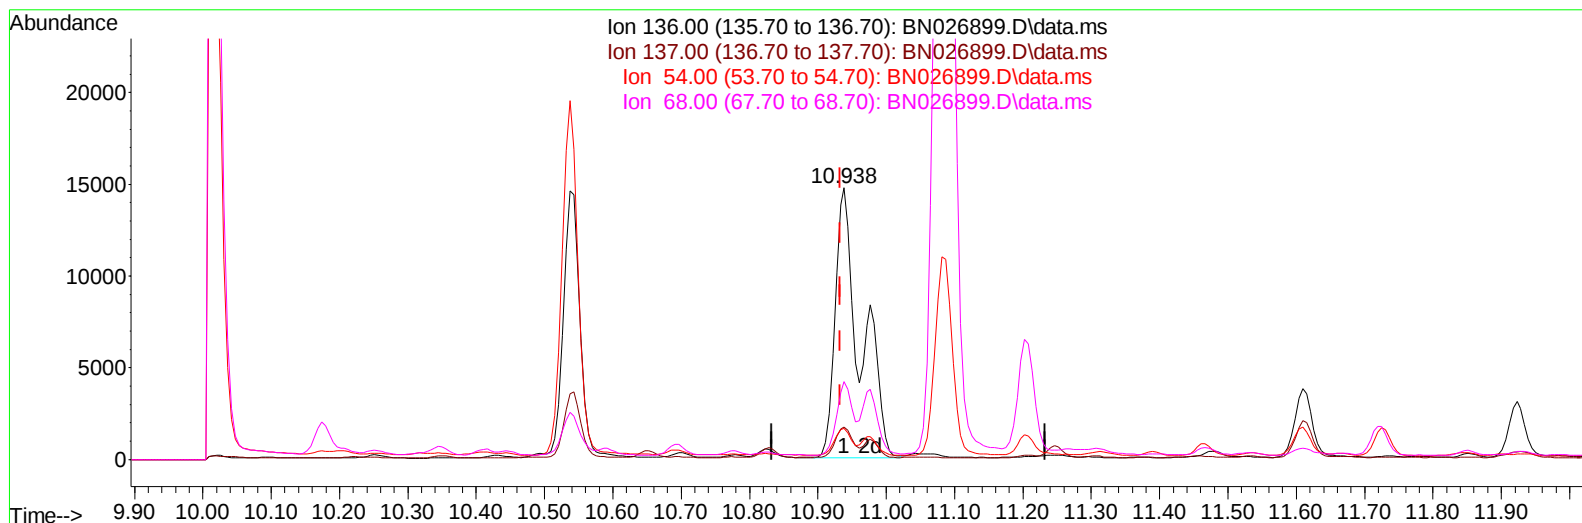

TIC: BN026899.D\data.ms

(4) Naphthalene-d8 (I)

10.938min (+ 0.006) 0.40 ng/ul m

response 38243

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	11.50	11.92
54.00	7.50	11.44#
68.00	6.80	28.55#

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081523\
 Data File : BN026899.D
 Acq On : 15 Aug 2023 13:49
 Operator : MA/JU
 Sample : 03967-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A48A0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/16/2023
 Supervised By :Sohil Jodhani 08/16/2023

Quant Time: Aug 16 00:53:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 00:50:05 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.110	152		7308	0.400	ng/ul	0.00
4) Naphthalene-d8	10.938	136		38243m	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.735	164		15046	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.481	188		32999	0.400	ng/ul	0.00
17) Chrysene-d12	21.661	240		26070	0.400	ng/ul	0.00
23) Perylene-d12	24.214	264		31206	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.439	96		17448	2.011	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.511	152		13124	0.233	ng/ul	0.00
18) Fluoranthene-d10	19.496	212		35456	0.431	ng/ul	0.00
Target Compounds							Qvalue
5) Naphthalene	10.988	128		2750	0.025	ng/ul#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081523\
Data File : BN026899.D
Acq On : 15 Aug 2023 13:49
Operator : MA/JU
Sample : 03967-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A48A0

Manual IntegrationsAPPROVED

Quant Time: Aug 16 00:53:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 00:50:05 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/16/2023
Supervised By :Sohil Jodhani 08/16/2023

