




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081523\
Data File : BN026900.D
Acq On : 15 Aug 2023 14:26
Operator : MA/JU
Sample : 03968-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A48B1

Manual IntegrationsAPPROVED

Quant Time: Aug 16 00:53:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 00:50:05 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/16/2023
Supervised By :Sohil Jodhani 08/16/2023

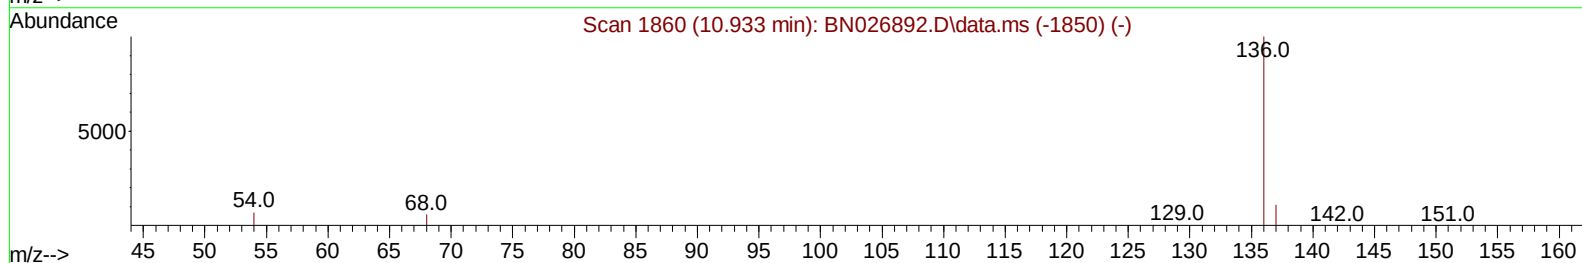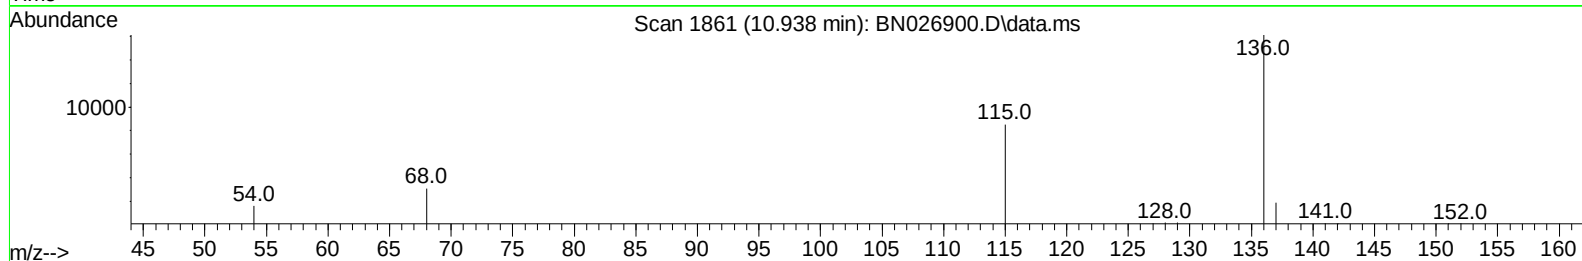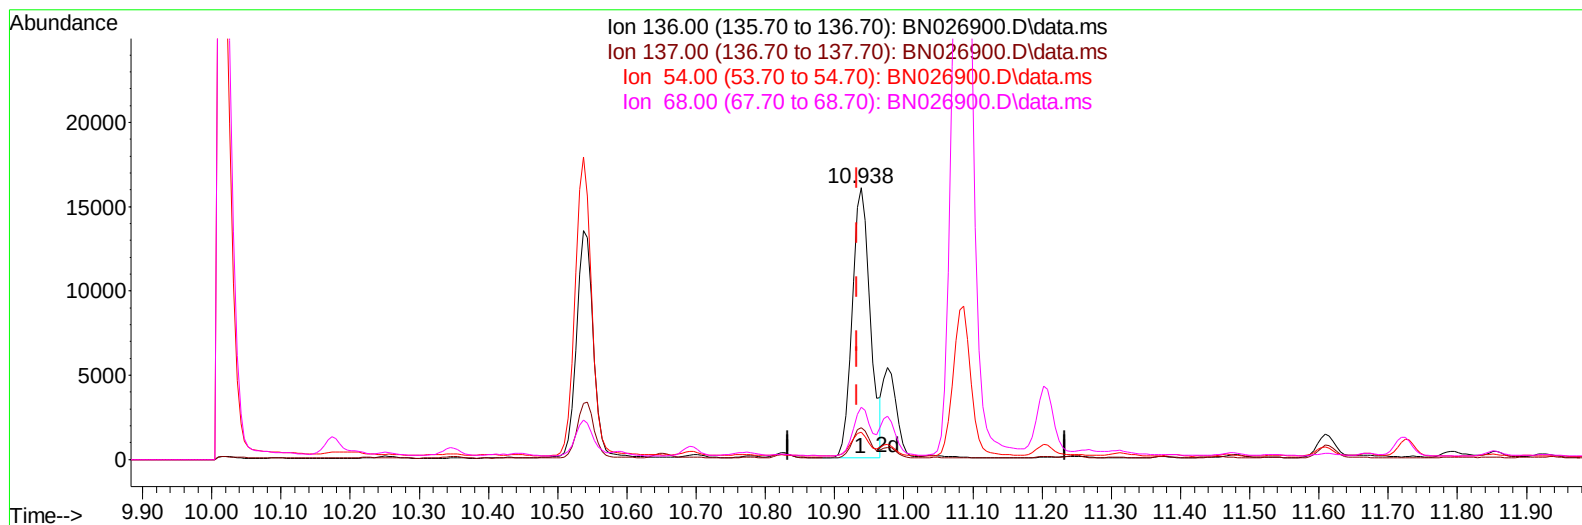

TIC: BN026900.D\data.ms

(4) Naphthalene-d8 (I)

10.938min (+ 0.006) 0.40 ng/ul

response 28884

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	11.50	11.72
54.00	7.50	9.93#
68.00	6.80	19.26#




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081523\
Data File : BN026900.D
Acq On : 15 Aug 2023 14:26
Operator : MA/JU
Sample : 03968-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A48B1

Manual IntegrationsAPPROVED

Quant Time: Aug 16 00:53:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 00:50:05 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/16/2023
Supervised By :Sohil Jodhani 08/16/2023

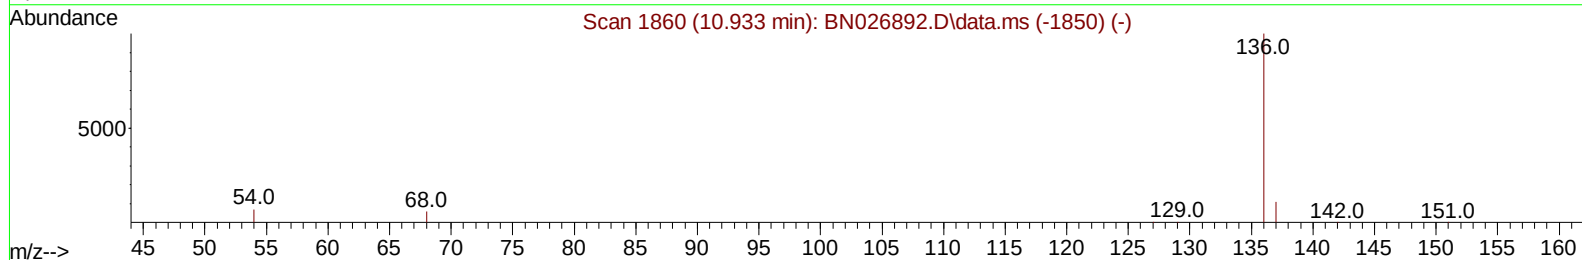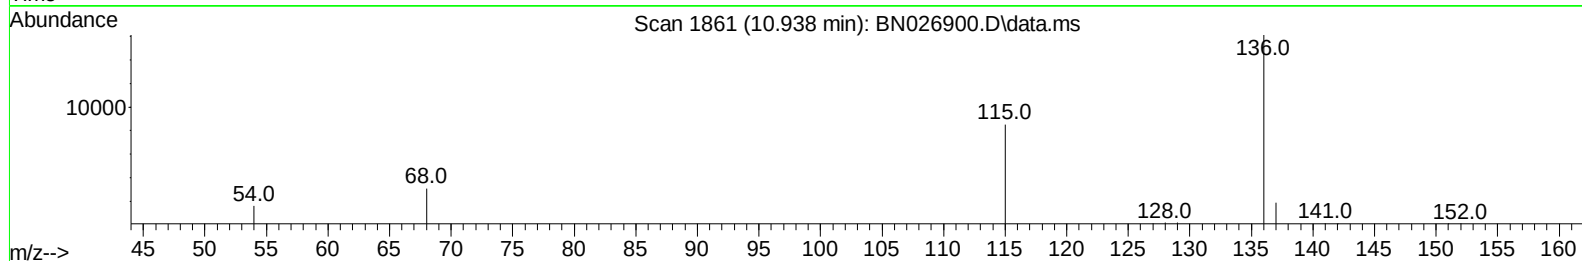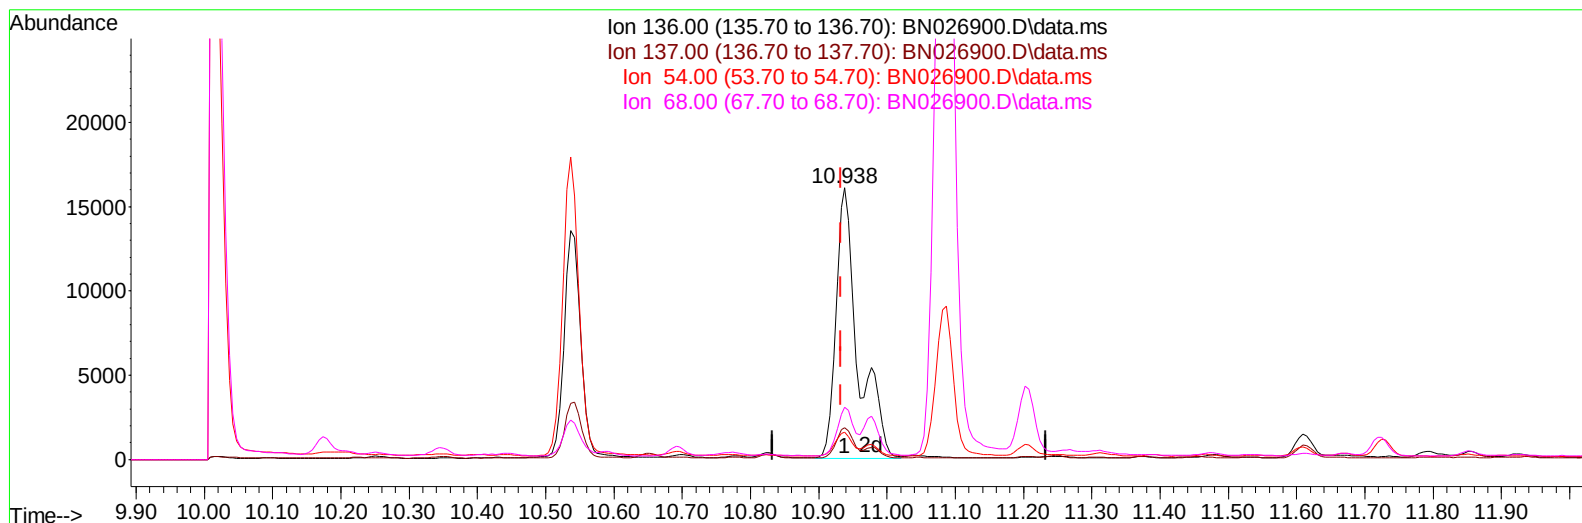

TIC: BN026900.D\data.ms

(4) Naphthalene-d8 (I)

10.938min (+ 0.006) 0.40 ng/ul m

response 36216

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	11.50	11.72
54.00	7.50	9.93#
68.00	6.80	19.26#

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081523\
 Data File : BN026900.D
 Acq On : 15 Aug 2023 14:26
 Operator : MA/JU
 Sample : 03968-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A48B1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/16/2023
 Supervised By :Sohil Jodhani 08/16/2023

Quant Time: Aug 16 00:53:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 00:50:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	7945	0.400	ng/ul	0.00
4) Naphthalene-d8	10.938	136	36216m	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.735	164	16493	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.481	188	36109	0.400	ng/ul	0.00
17) Chrysene-d12	21.656	240	28579	0.400	ng/ul	0.00
23) Perylene-d12	24.205	264	33754	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.439	96	19676	2.086	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.511	152	11298	0.212	ng/ul	0.00
18) Fluoranthene-d10	19.497	212	31637	0.351	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081523\
Data File : BN026900.D
Acq On : 15 Aug 2023 14:26
Operator : MA/JU
Sample : 03968-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A48B1

Manual IntegrationsAPPROVED

Quant Time: Aug 16 00:53:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 00:50:05 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/16/2023
Supervised By :Sohil Jodhani 08/16/2023

