

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081523\
 Data File : BN026897.D
 Acq On : 15 Aug 2023 12:35
 Operator : MA/JU
 Sample : 03965-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4880

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/16/2023
 Supervised By :Sohil Jodhani 08/16/2023

Quant Time: Aug 16 01:03:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 00:50:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.109	152	5992	0.400	ng/ul	0.00
4) Naphthalene-d8	10.938	136	32302m	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.735	164	12234	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.481	188	26174	0.400	ng/ul	0.00
17) Chrysene-d12	21.659	240	19723	0.400	ng/ul	0.00
23) Perylene-d12	24.205	264	23800	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.439	96	15204	2.137	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.511	152	12088	0.254	ng/ul	0.00
18) Fluoranthene-d10	19.496	212	32272	0.518	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.987	128	3950	0.043	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081523\
Data File : BN026897.D
Acq On : 15 Aug 2023 12:35
Operator : MA/JU
Sample : 03965-04
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A4880

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/16/2023
Supervised By :Sohil Jodhani 08/16/2023


Quant Time: Aug 16 01:03:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 00:50:05 2023
Response via : Initial Calibration

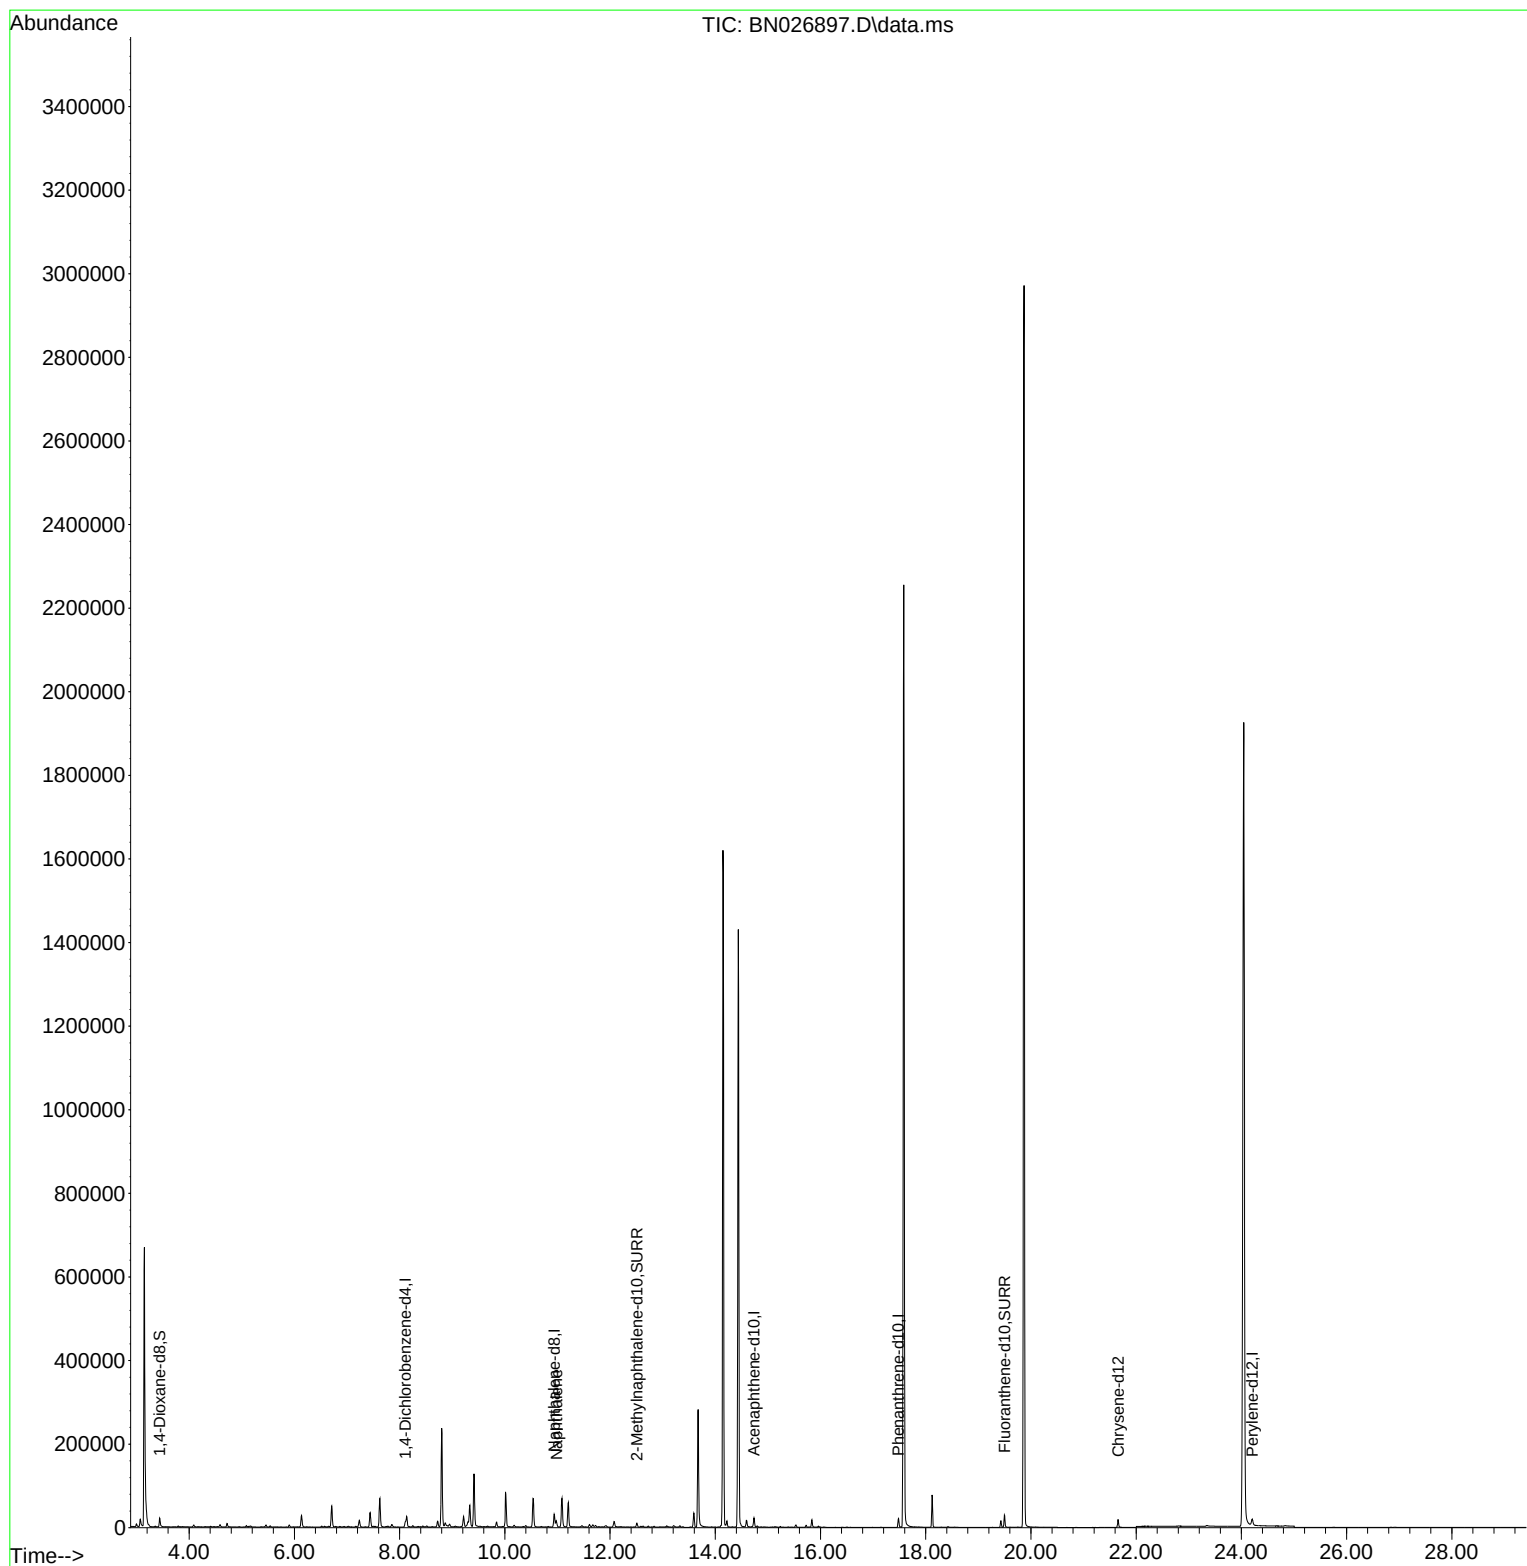

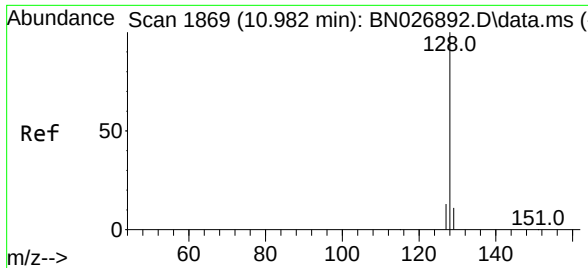

#5
 Naphthalene
 Concen: 0.043 ng/ul
 RT: 10.987 min Scan# 1869
 Delta R.T. 0.005 min
 Lab File: BN026897.D
 Acq: 15 Aug 2023 12:35

Instrument :
 BNA_N
 ClientSampleId :
 A4880

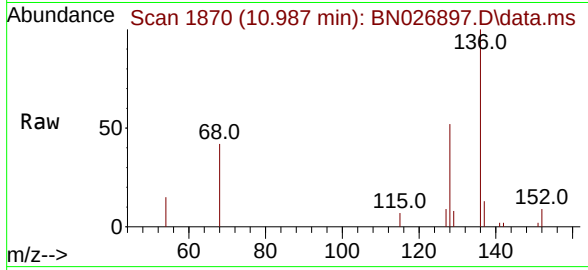

Tgt Ion:	128	Resp:	3950
Ion	Ratio	Lower	Upper
128	100		
129	16.3	9.2	13.8
127	16.6	10.5	15.7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/16/2023
 Supervised By :Sohil Jodhani 08/16/2023

