

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081523\
 Data File : BN026899.D
 Acq On : 15 Aug 2023 13:49
 Operator : MA/JU
 Sample : 03967-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A48A0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/16/2023
 Supervised By :Sohil Jodhani 08/16/2023

Quant Time: Aug 16 00:53:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 00:50:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	7308	0.400	ng/ul	0.00
4) Naphthalene-d8	10.938	136	38243m	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.735	164	15046	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.481	188	32999	0.400	ng/ul	0.00
17) Chrysene-d12	21.661	240	26070	0.400	ng/ul	0.00
23) Perylene-d12	24.214	264	31206	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.439	96	17448	2.011	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.511	152	13124	0.233	ng/ul	0.00
18) Fluoranthene-d10	19.496	212	35456	0.431	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.988	128	2750	0.025	ng/ul#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081523\
Data File : BN026899.D
Acq On : 15 Aug 2023 13:49
Operator : MA/JU
Sample : 03967-07
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A48A0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/16/2023
Supervised By :Sohil Jodhani 08/16/2023


Quant Time: Aug 16 00:53:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 00:50:05 2023
Response via : Initial Calibration

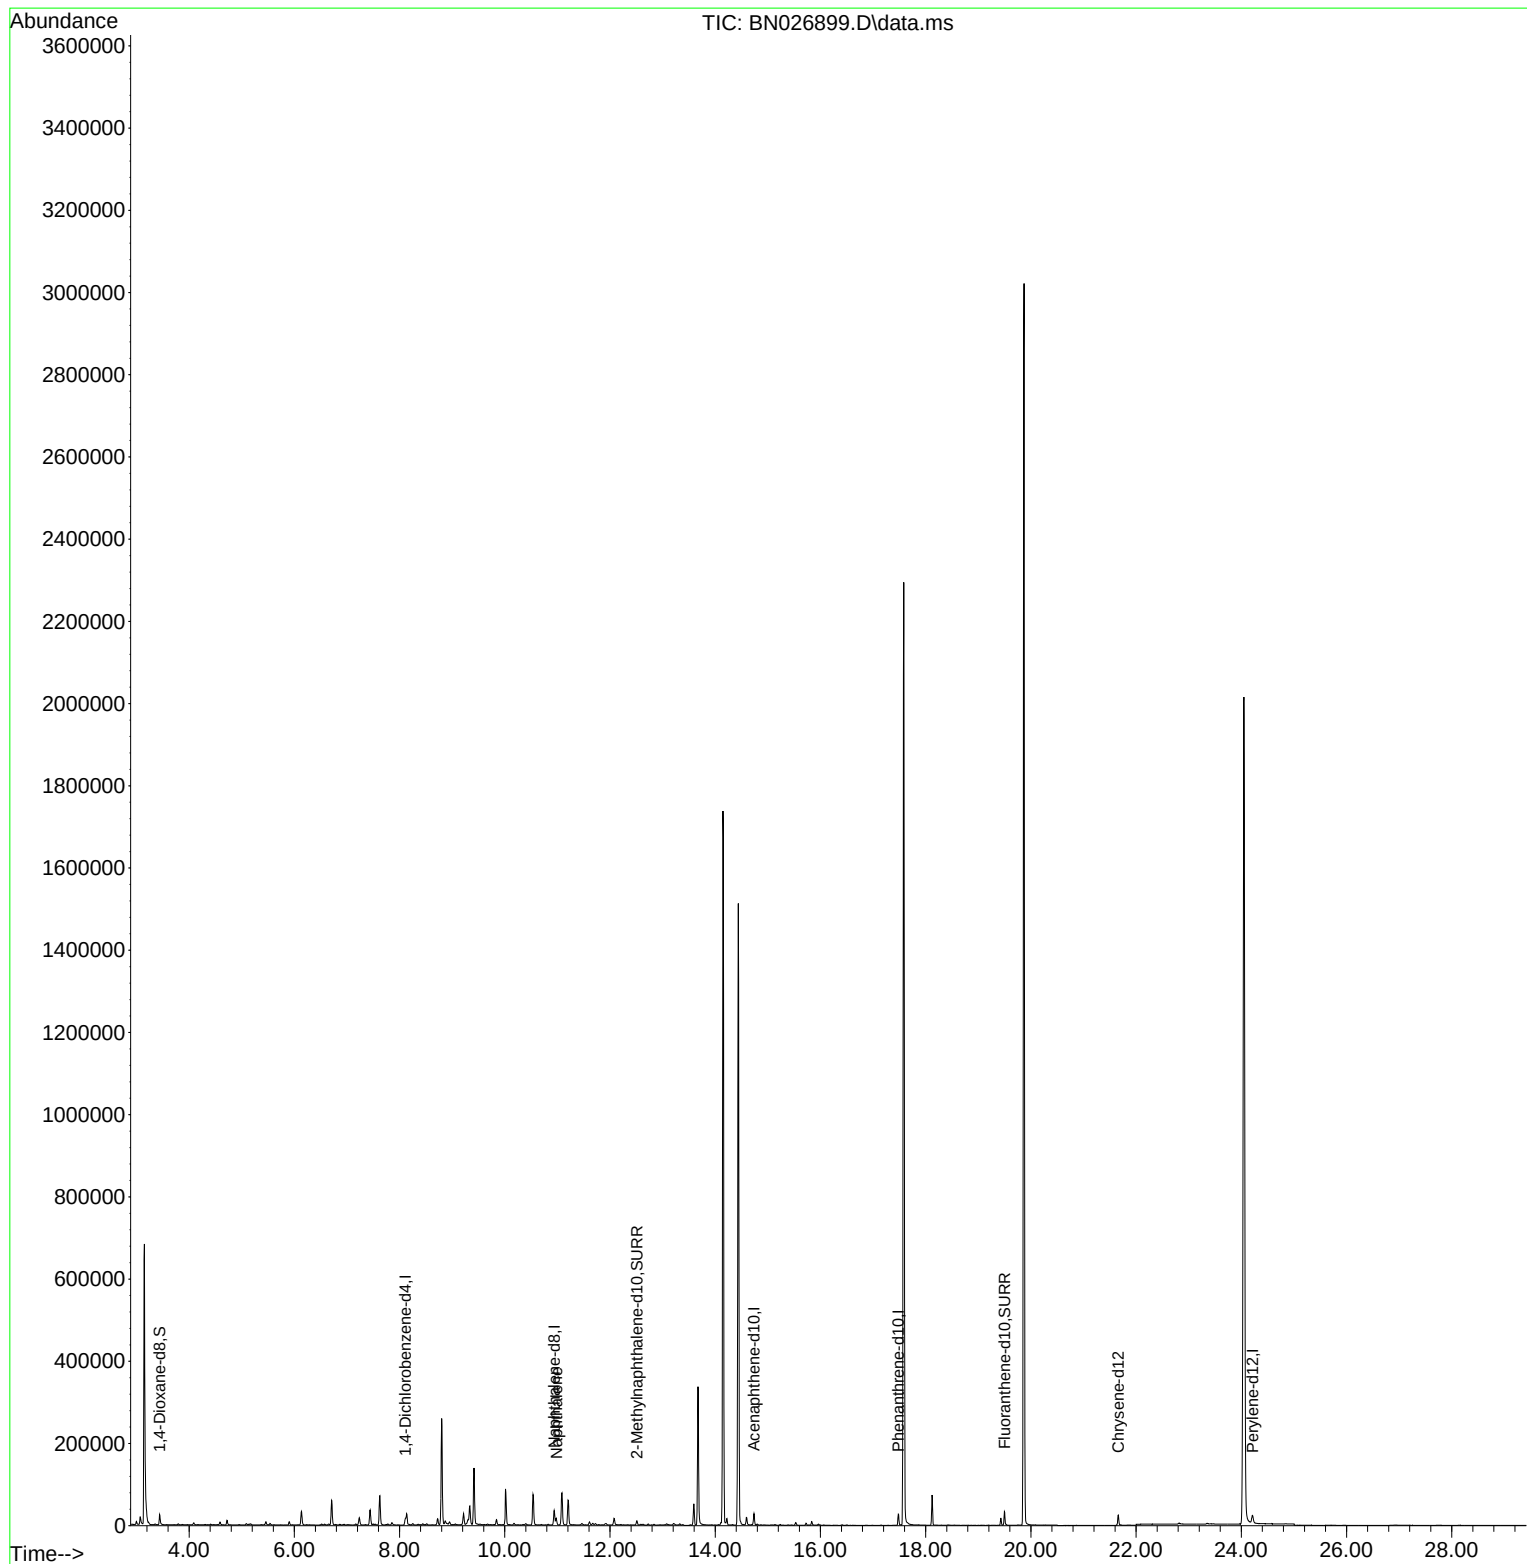

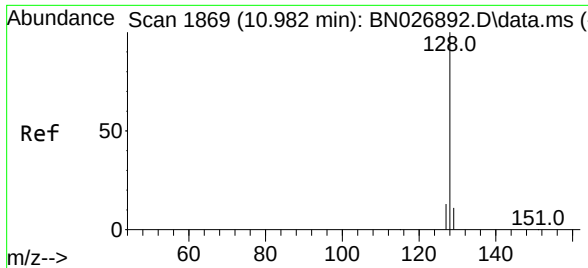

#5
Naphthalene
Concen: 0.025 ng/ul
RT: 10.988 min Scan# 1869
Delta R.T. 0.006 min
Lab File: BN026899.D
Acq: 15 Aug 2023 13:49

Instrument :
BNA_N
ClientSampleId :
A48A0

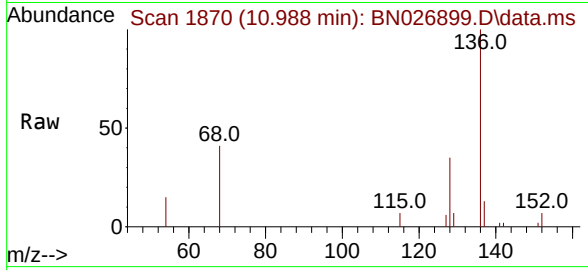

Tgt Ion:128 Resp: 2750

Ion	Ratio	Lower	Upper
128	100		
129	18.9	9.2	13.8
127	18.1	10.5	15.7

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/16/2023
Supervised By :Sohil Jodhani 08/16/2023

