

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081619\
 Data File : BN007232.D
 Acq On : 16 Aug 2019 20:37
 Operator : HP/JU
 Sample : K4336-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 KY038PS037-190812

Quant Time: Aug 17 02:16:35 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN081019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 13 12:12:02 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	7306	0.40	ng	-0.02
6) Naphthalene-d8	10.17	136	27581	0.40	ng	-0.01
12) Acenaphthene-d10	14.07	164	16515	0.40	ng	-0.01
18) Phenanthrene-d10	16.81	188	39232	0.40	ng	-0.01
26) Chrysene-d12	21.03	240	39080	0.40	ng	-0.02
32) Perylene-d12	23.15	264	40997	0.40	ng	-0.02
System Monitoring Compounds						
3) 2-Fluorophenol	5.05	112	3486	0.20	ng	0.00
4) Phenol-d6	6.61	99	2711	0.12	ng	0.00
7) Nitrobenzene-d5	8.55	82	8284	0.37	ng	-0.01
10) 2-Methylnaphthalene-d10	11.78	152	17825	0.35	ng	-0.01
13) 2,4,6-Tribromophenol	15.56	330	3306	0.37	ng	-0.01
14) 2-Fluorobiphenyl	12.71	172	1331	0.06	ng	0.00
24) Fluoranthene-d10	18.86	212	46815	0.34	ng	-0.02
28) Terphenyl-d14	19.48	244	40443	0.38	ng	-0.02
Target Compounds						
15) Acenaphthylene	13.78	152	3815	0.044	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081619\
Data File : BN007232.D
Acq On : 16 Aug 2019 20:37
Operator : HP/JU
Sample : K4336-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
KY038PS037-190812

Quant Time: Aug 17 02:16:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN081019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 13 12:12:02 2019
Response via : Initial Calibration

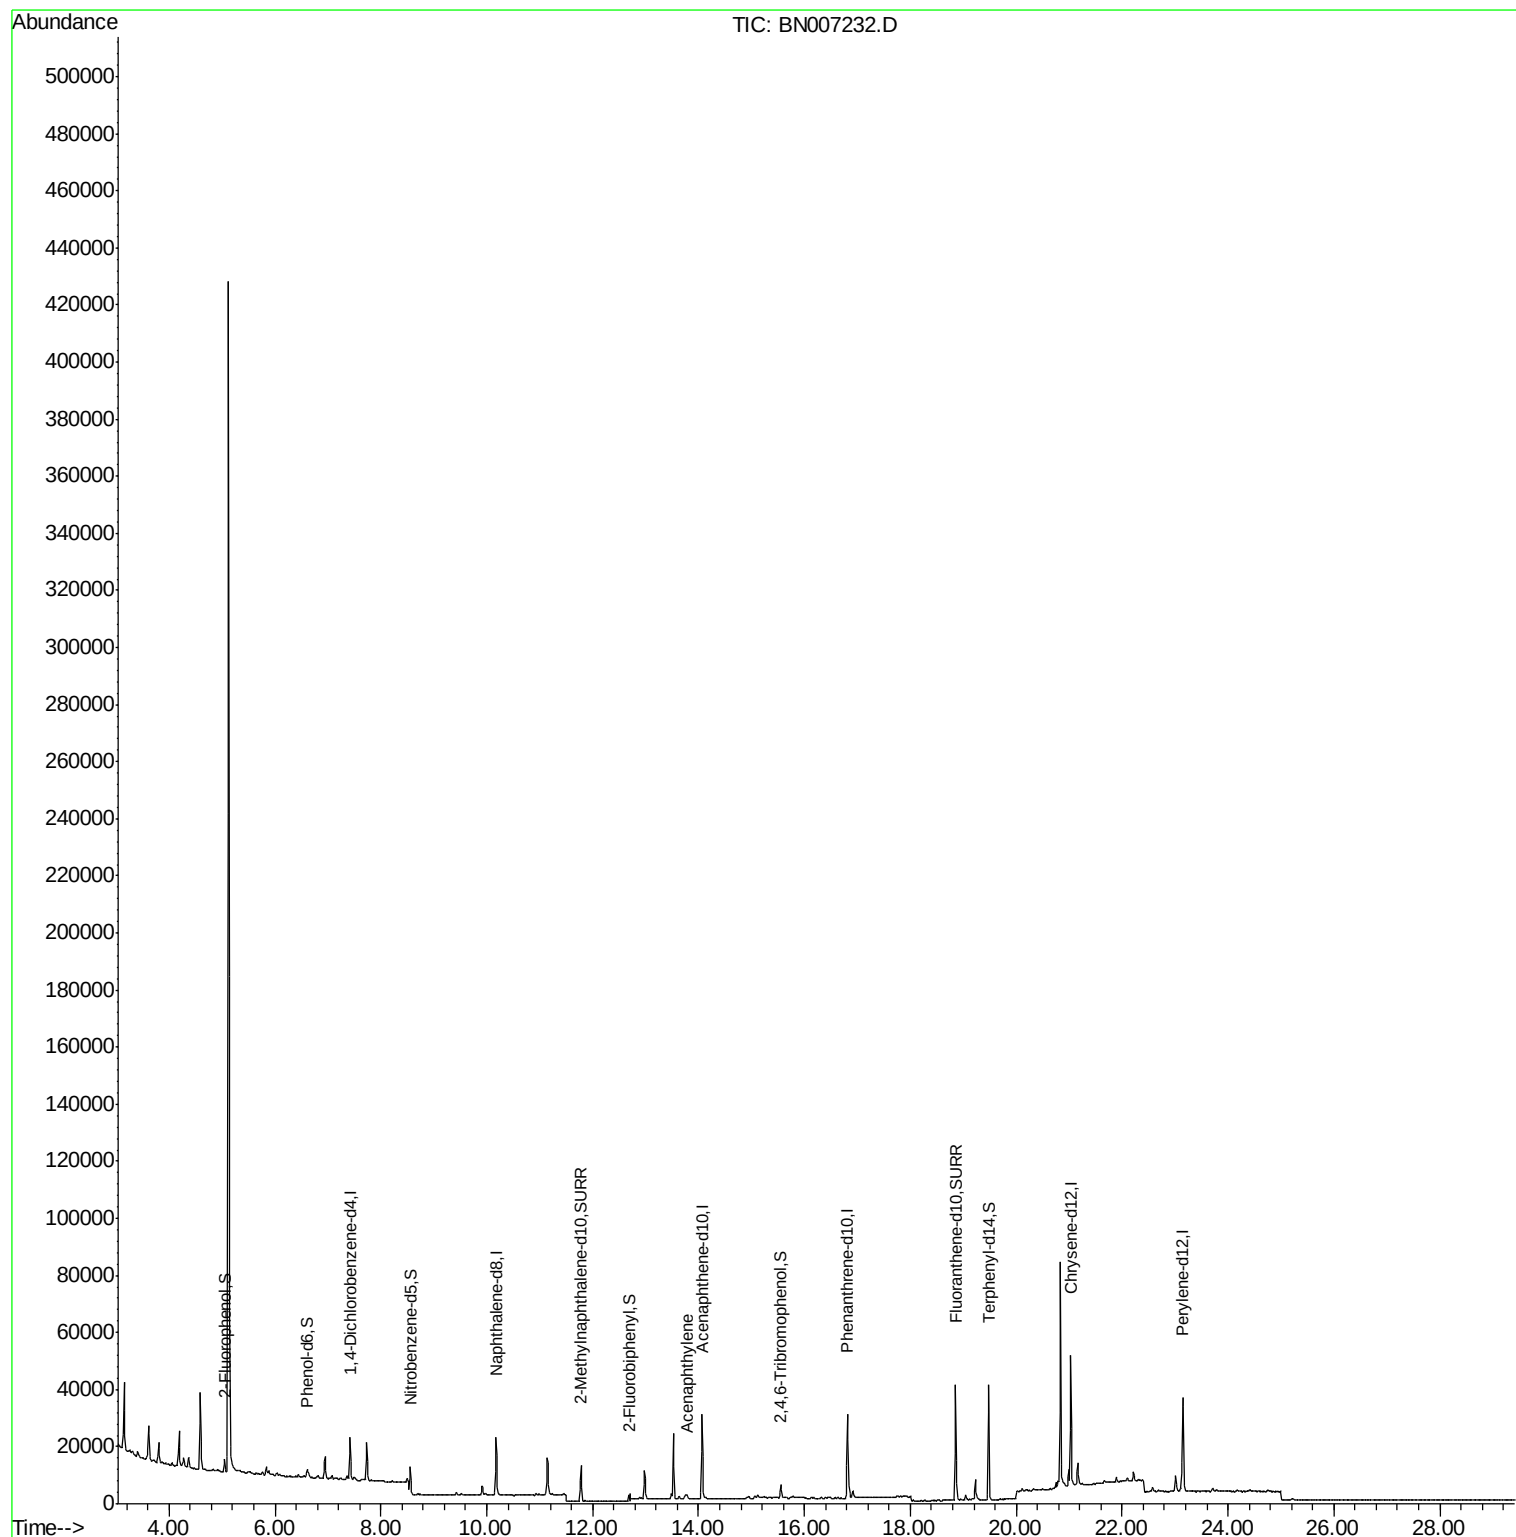

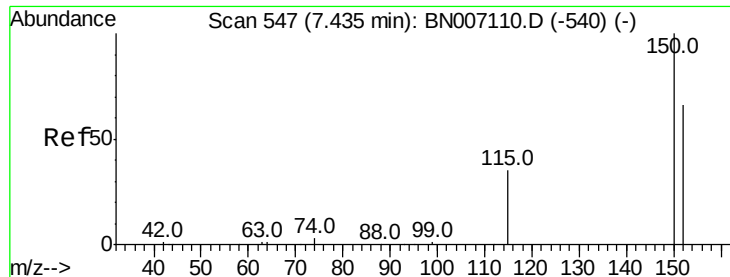


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.42 min Scan# 545
Delta R.T. -0.02 min
Lab File: BN007232.D
Acq: 16 Aug 2019 20:37

Instrument :
BNA_N
ClientSampleId :
KY038PS037-190812

Tot Ion:152 Resp: 7306
Ion Ratio Lower Upper
152 100
150 155.5 121.7 182.5
115 60.1 46.2 69.4

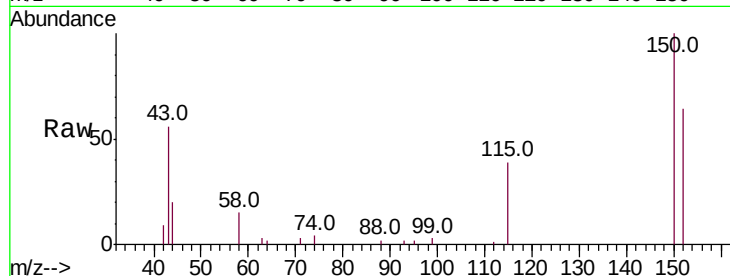


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

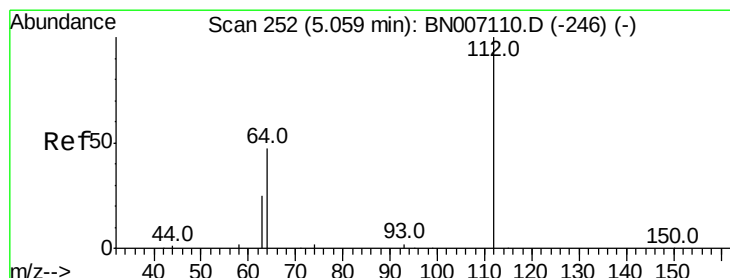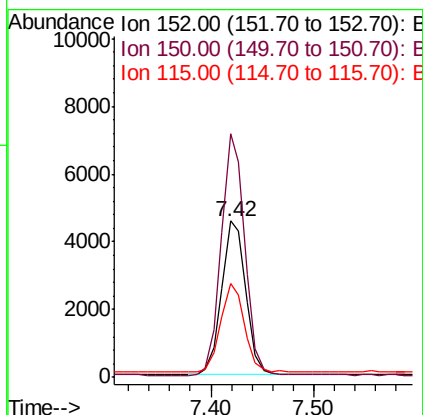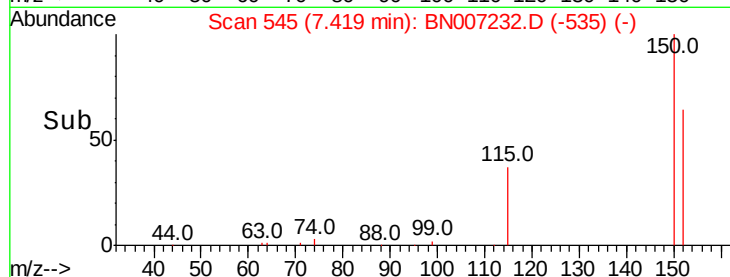



#3


2-Fluorophenol
Concen: 0.199 ng
RT: 5.05 min Scan# 251
Delta R.T. -0.01 min
Lab File: BN007232.D
Acq: 16 Aug 2019 20:37

Tgt Ion:112 Resp: 3486
Ion Ratio Lower Upper
112 100
64 51.2 42.6 63.8
63 27.6 22.2 33.2

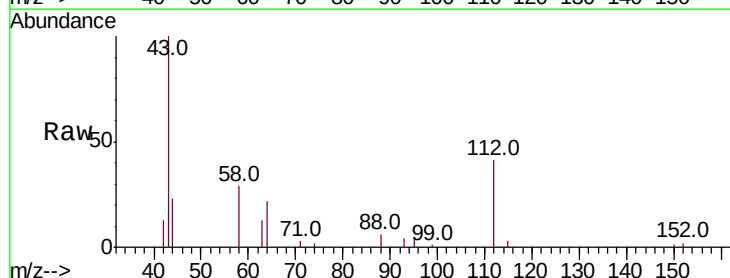

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

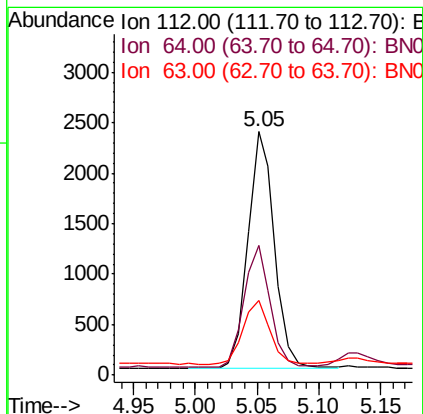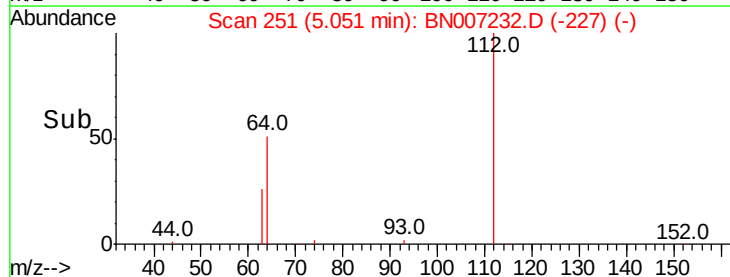



#4

Phenol-d6

Concen: 0.125 ng

RT: 6.61 min Scan# 445

Delta R.T. -0.00 min

Lab File: BN007232.D

Acq: 16 Aug 2019 20:37

Instrument :

BNA_N

ClientSampleId :

KY038PS037-190812


Tot Ion: 99 Resp: 2711

Ion Ratio Lower Upper

99 100

42 27.3 15.8 23.6#




71 38.2 27.0 40.4

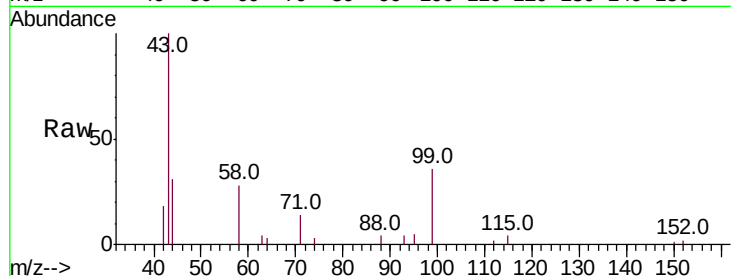

Abundance Ion 99.00 (98.70 to 99.70): BN007232.D (-433) (-)

Ion 42.00 (41.70 to 42.70): BN007232.D (-433) (-)

Ion 71.00 (70.70 to 71.70): BN007232.D (-433) (-)

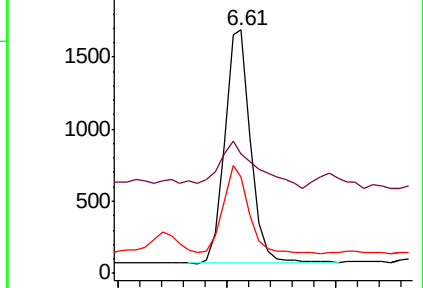

#6

Naphthalene-d8

Concen: 0.400 ng

RT: 10.17 min Scan# 812

Delta R.T. -0.01 min

Lab File: BN007232.D

Acq: 16 Aug 2019 20:37

Tgt Ion: 136 Resp: 27581


Ion Ratio Lower Upper

136 100

137 11.3 9.4 14.0

54 7.0 6.6 9.8

68 6.5 6.0 9.0






Abundance Ion 136.00 (135.70 to 136.70): BN007232.D (-797) (-)

Ion 137.00 (136.70 to 137.70): BN007232.D (-797) (-)

Ion 54.00 (53.70 to 54.70): BN007232.D (-797) (-)

Ion 68.00 (67.70 to 68.70): BN007232.D (-797) (-)

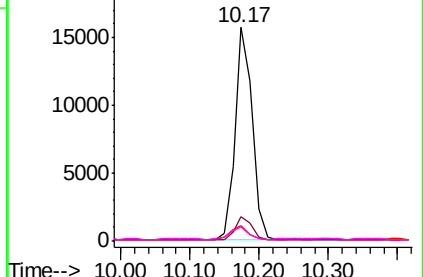



#7

Nitrobenzene-d5

Concen: 0.372 ng

RT: 8.55 min Scan# 684

Delta R.T. -0.01 min

Lab File: BN007232.D

Acq: 16 Aug 2019 20:37

Instrument :

BNA_N

ClientSampleId :

KY038PS037-190812


Tot Ion: 82 Resp: 8284

Ion Ratio Lower Upper

82 100

128 46.4 34.6 51.8




54 44.0 36.2 54.4



Abundance Ion 82.00 (81.70 to 82.70): BN007232.D (-679) (-)

Ion 128.00 (127.70 to 128.70): BN007232.D (-679) (-)

Ion 54.00 (53.70 to 54.70): BN007232.D (-679) (-)

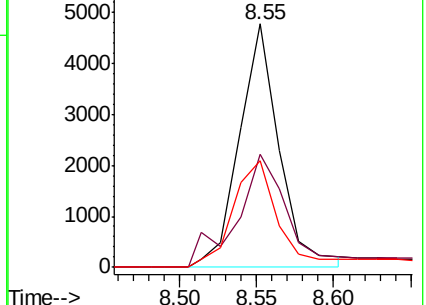

#10

2-Methylnaphthalene-d10

Concen: 0.347 ng

RT: 11.78 min Scan# 979

Delta R.T. -0.01 min

Lab File: BN007232.D


Acq: 16 Aug 2019 20:37

Tgt Ion: 152 Resp: 17825

Ion Ratio Lower Upper



152 100


151 19.8 15.5 23.3



Abundance Ion 152.00 (151.70 to 152.70): BN007232.D (-937) (-)

Ion 151.00 (150.70 to 151.70): BN007232.D (-937) (-)

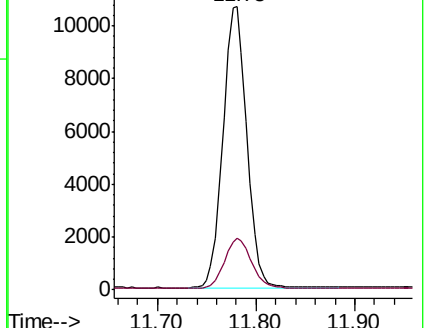

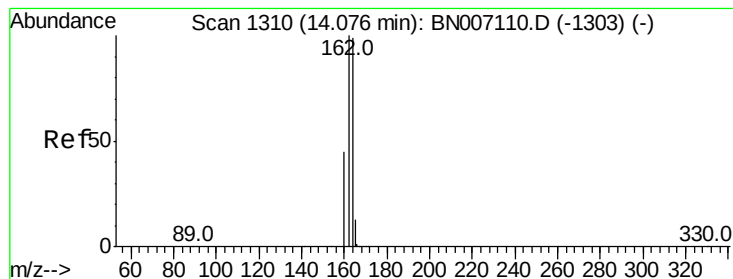

#12

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.07 min Scan# 1309

Delta R.T. -0.01 min

Lab File: BN007232.D

Acq: 16 Aug 2019 20:37

Instrument :

BNA_N

ClientSampleId :

KY038PS037-190812


Tot Ion:164 Resp: 16515

Ion Ratio Lower Upper

164 100

162 102.6 82.2 123.4




160 46.9 38.3 57.5

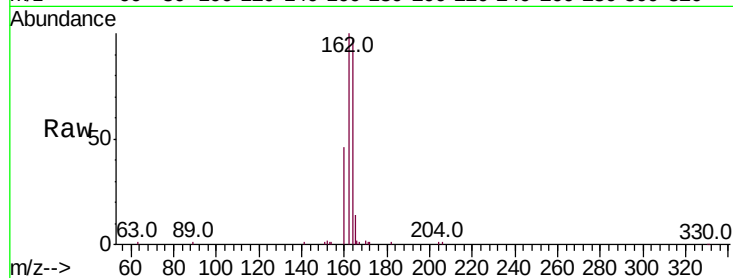

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

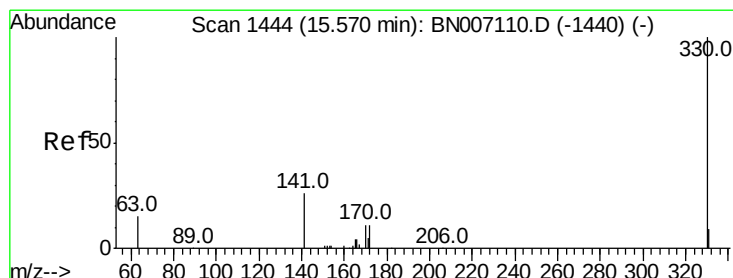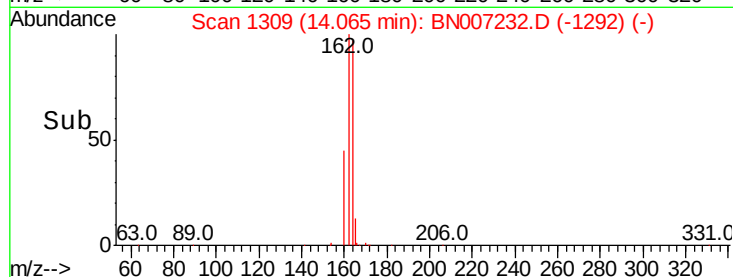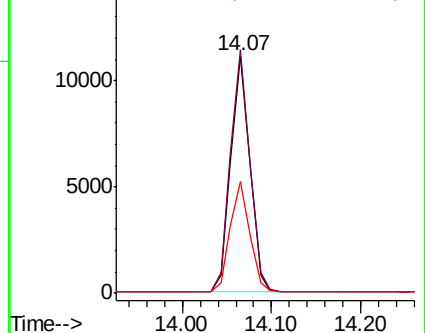

#13

2,4,6-Tribromophenol

Concen: 0.372 ng

RT: 15.56 min Scan# 1443

Delta R.T. -0.01 min

Lab File: BN007232.D

Acq: 16 Aug 2019 20:37


Tgt Ion:330 Resp: 3306

Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0



141 40.2 33.6 50.4

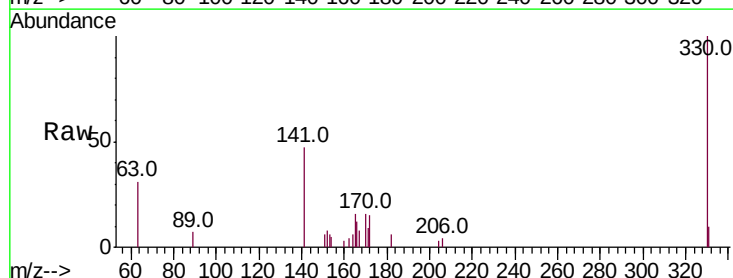


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

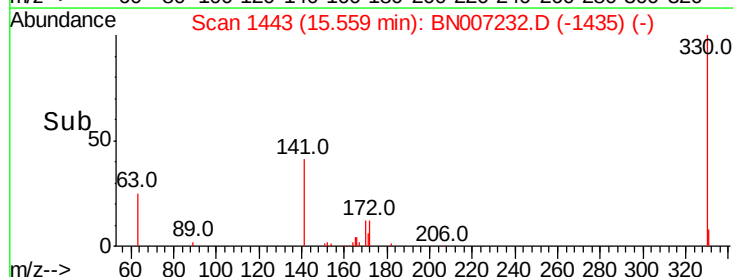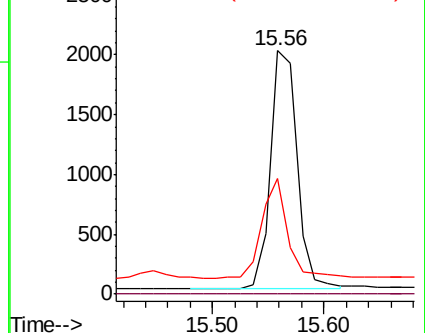

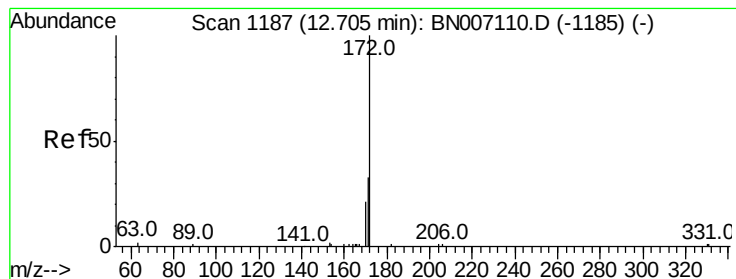

#14

2-Fluorobiphenyl

Concen: 0.055 ng

RT: 12.71 min Scan# 1187

Delta R.T. -0.00 min

Lab File: BN007232.D

Acq: 16 Aug 2019 20:37

Instrument :

BNA_N

ClientSampleId :

KY038PS037-190812


Tot Ion:172 Resp: 1331

Ion Ratio Lower Upper

172 100

171 33.1 26.3 39.5




170 22.5 17.0 25.4

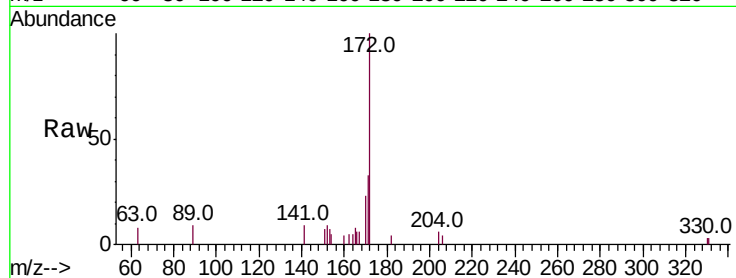

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

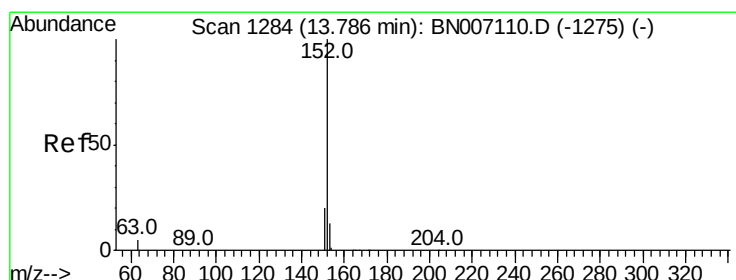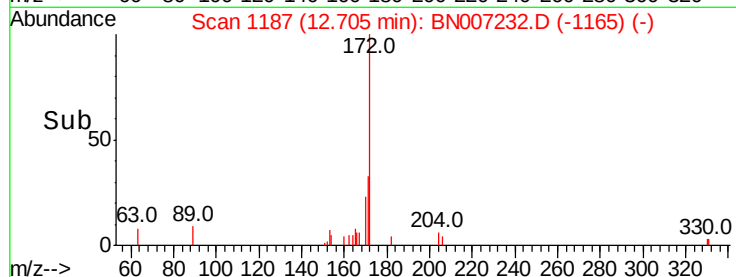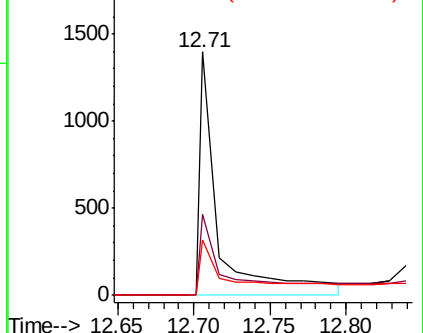

#15

Acenaphthylene

Concen: 0.044 ng

RT: 13.78 min Scan# 1283

Delta R.T. -0.01 min

Lab File: BN007232.D

Acq: 16 Aug 2019 20:37


Tgt Ion:152 Resp: 3815

Ion Ratio Lower Upper

152 100

151 19.8 15.8 23.6



153 13.0 10.4 15.6

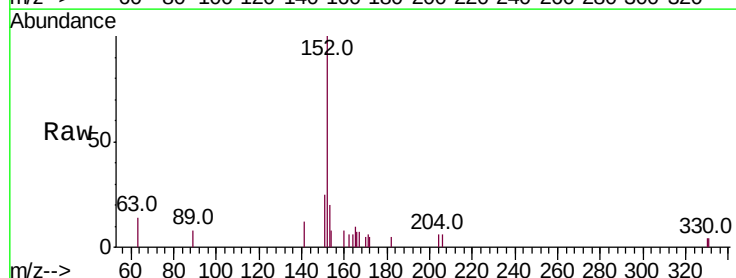


Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

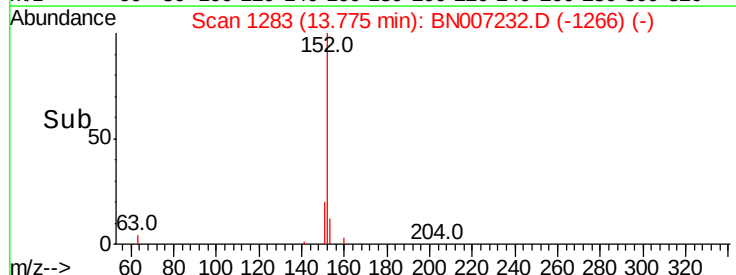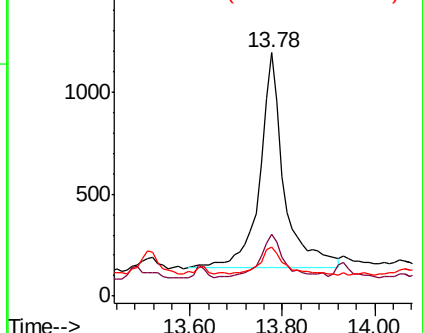



#18

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.81 min Scan# 1559

Delta R.T. -0.01 min

Lab File: BN007232.D

Acq: 16 Aug 2019 20:37

Instrument :

BNA_N

ClientSampleId :

KY038PS037-190812


Tot Ion:188 Resp: 39232

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 9.3 7.8 11.6

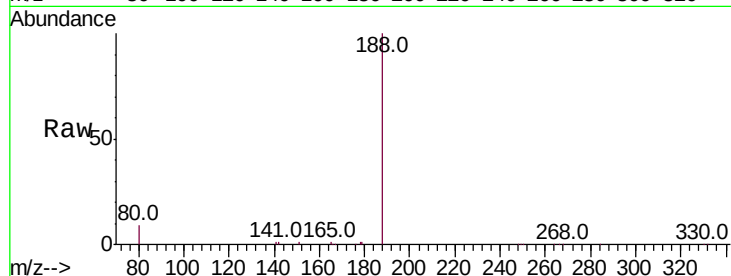

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

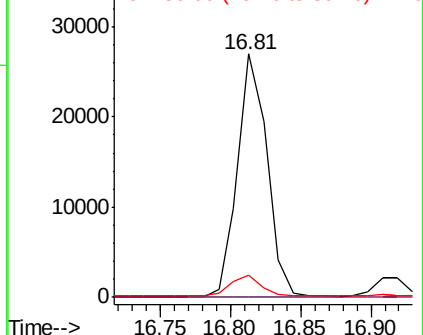

#24

Fluoranthene-d10

Concen: 0.336 ng

RT: 18.86 min Scan# 1842

Delta R.T. -0.02 min

Lab File: BN007232.D

Acq: 16 Aug 2019 20:37


Tgt Ion:212 Resp: 46815

Ion Ratio Lower Upper

212 100

106 10.5 8.2 12.2



104 5.9 4.5 6.7




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

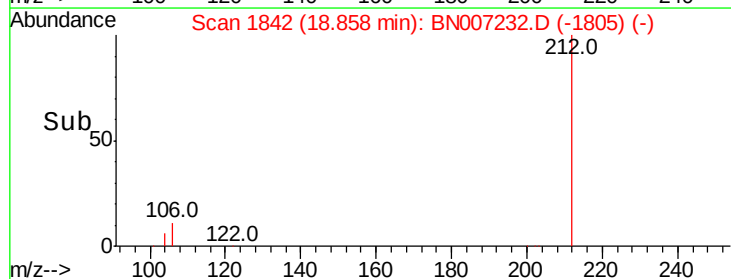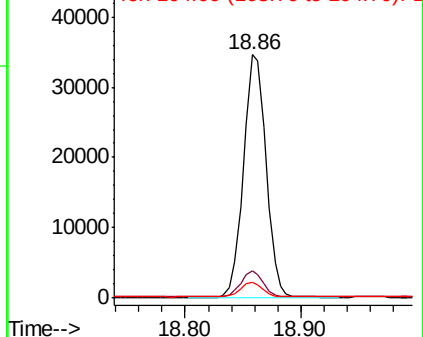



#26

Chrysene-d12

Concen: 0.400 ng

RT: 21.03 min Scan# 2170

Delta R.T. -0.02 min

Lab File: BN007232.D

Acq: 16 Aug 2019 20:37

Instrument :

BNA_N

ClientSampleId :

KY038PS037-190812


Tot Ion:240 Resp: 39080

Ion Ratio Lower Upper

240 100

120 7.9 4.0 6.0#




236 27.0 21.3 31.9



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

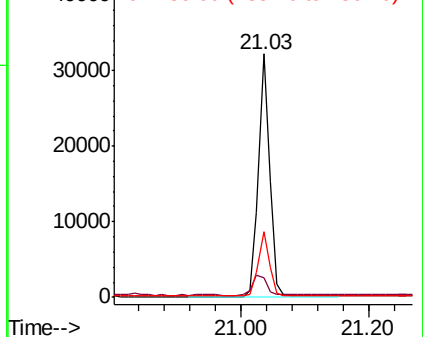

#28

Terphenyl-d14

Concen: 0.380 ng

RT: 19.48 min Scan# 1967

Delta R.T. -0.02 min

Lab File: BN007232.D

Acq: 16 Aug 2019 20:37


Tgt Ion:244 Resp: 40443

Ion Ratio Lower Upper

244 100

212 8.2 6.2 9.2



122 10.4 7.4 11.2






Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

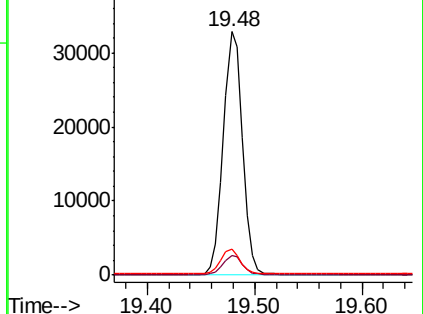

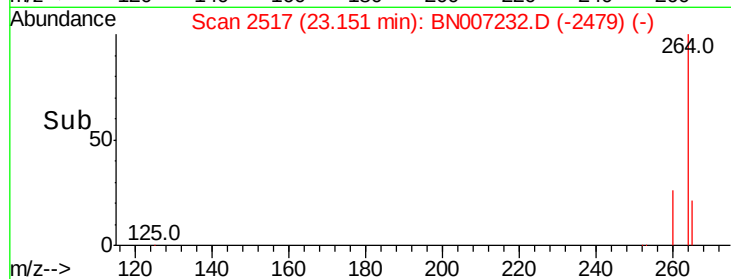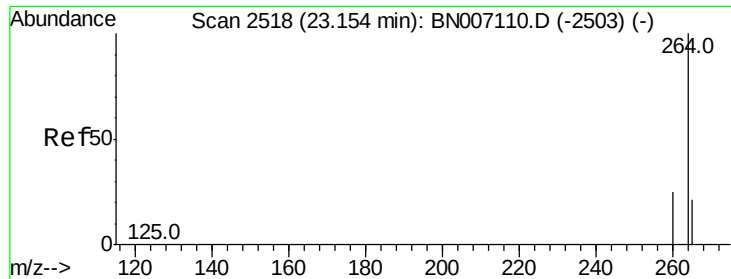

#32

Pervlene-d12

Concen: 0.400 ng

RT: 23.15 min Scan# 2517

Delta R.T. -0.02 min

Lab File: BN007232.D

Acq: 16 Aug 2019 20:37

Instrument :

BNA_N

ClientSampleId :

KY038PS037-190812

Tot Ion:264 Resp: 40997

Ion Ratio Lower Upper

264 100

260 25.1 19.8 29.8

265 31.2 26.2 39.4

