


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081619\
 Data File : BN007235.D
 Acq On : 16 Aug 2019 23:38
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 13 12:12:02 2019

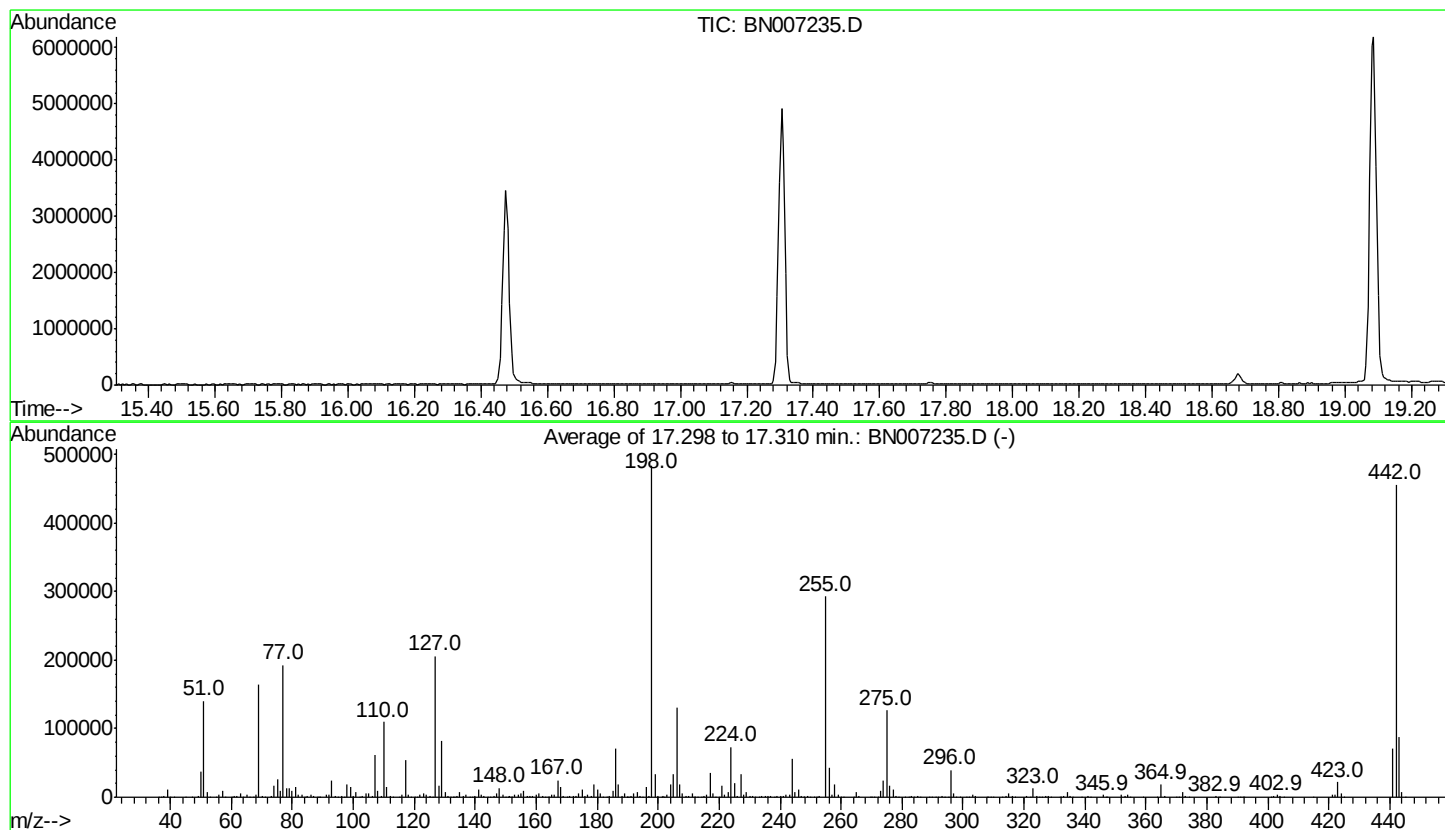

AutoFind: Scans 2433, 2434, 2435; Background Corrected with Scan 2426

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	140624	PASS
68	69	0.00	2	2.0	3272	PASS
69	198	0.00	100	34.1	164949	PASS
70	69	0.00	2	0.7	1120	PASS
127	198	10	80	42.6	206208	PASS
197	198	0.00	2	0.2	1017	PASS
198	198	100	100	100.0	483712	PASS
199	198	5	9	6.8	32930	PASS
275	198	10	60	26.2	126629	PASS
365	198	1	100	3.8	18573	PASS
441	198	0.01	100	14.6	70850	PASS
442	198	50	100	94.2	455680	PASS
443	442	15	24	19.2	87341	PASS