
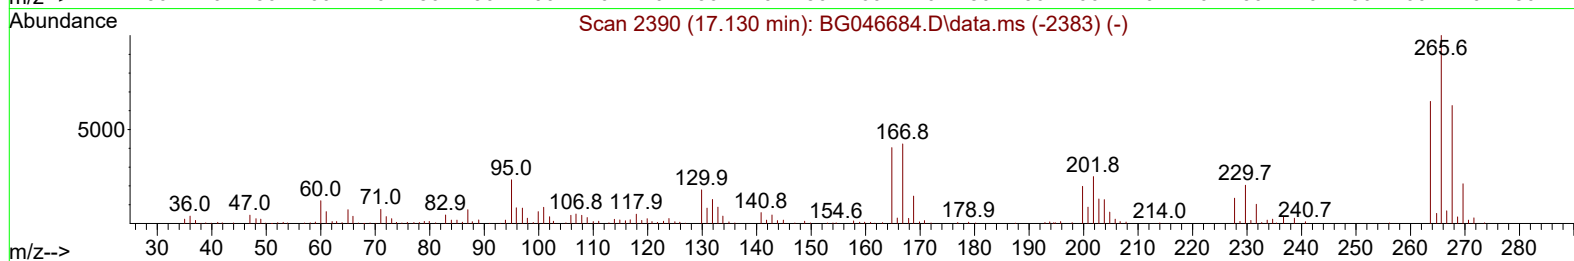
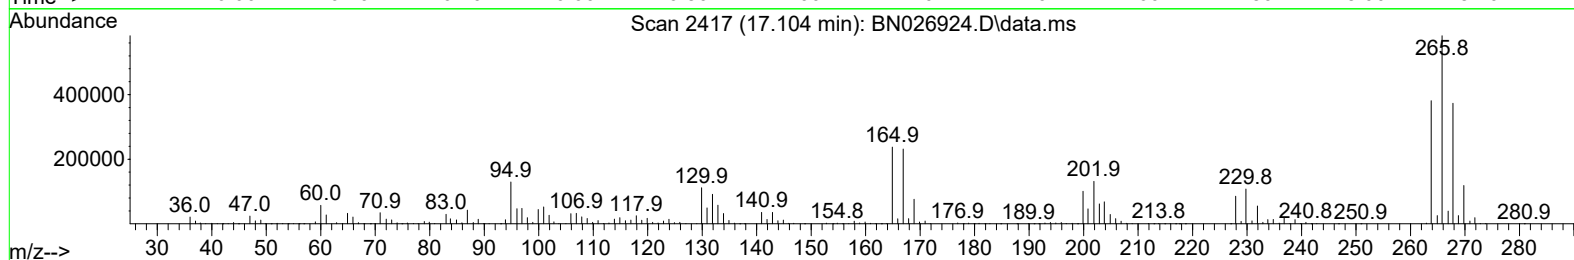


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081623\
Data File : BN026924.D
Acq On : 16 Aug 2023 09:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 03:29:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 17 03:29:54 2023
Response via : Initial Calibration

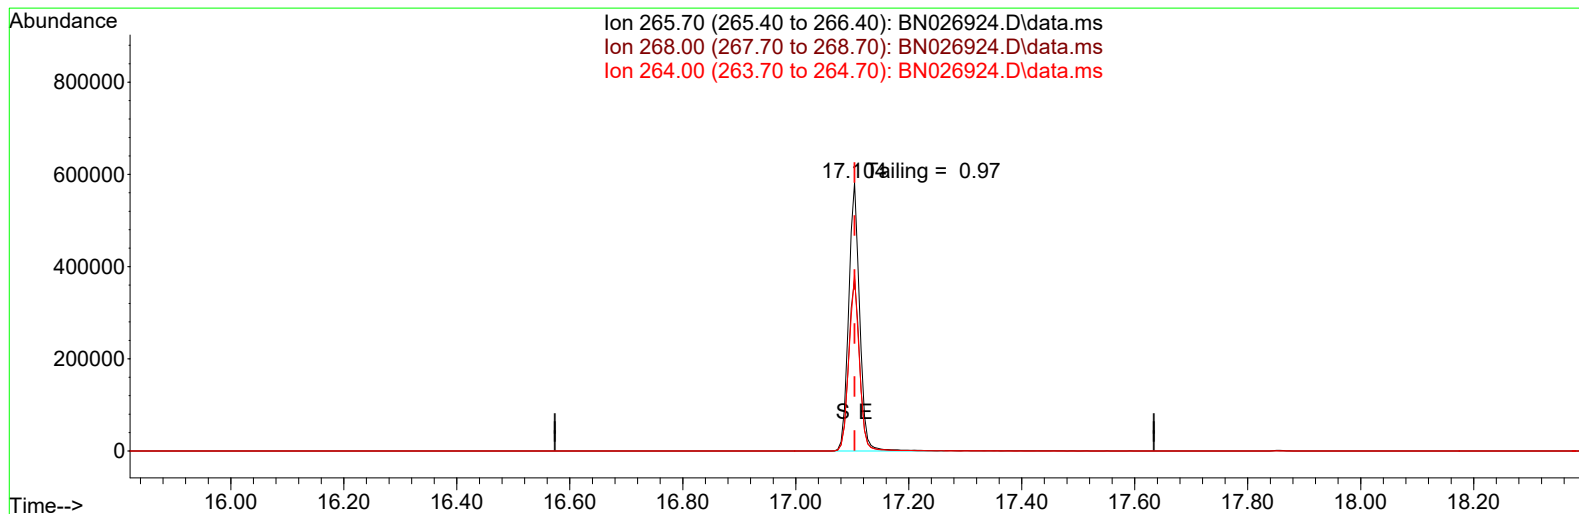

TIC: BN026924.D\data.ms

(70) Pentachlorophenol (C)




17.104min (0.000) 26665.46 ng

response 787669

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.08
264.00	61.60	65.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081623\
Data File : BN026924.D
Acq On : 16 Aug 2023 09:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 03:29:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 17 03:29:54 2023
Response via : Initial Calibration

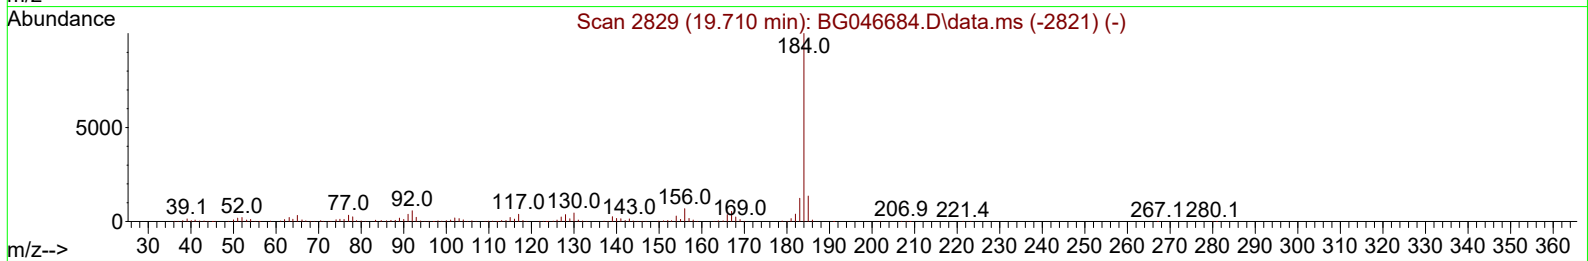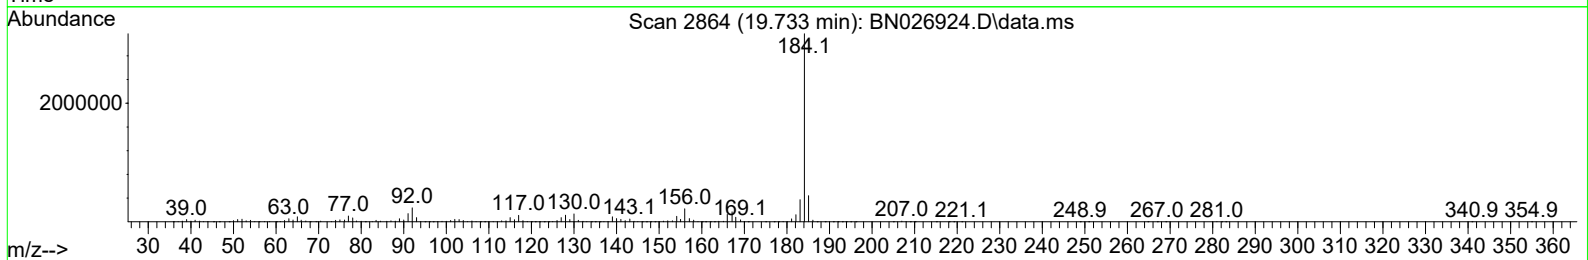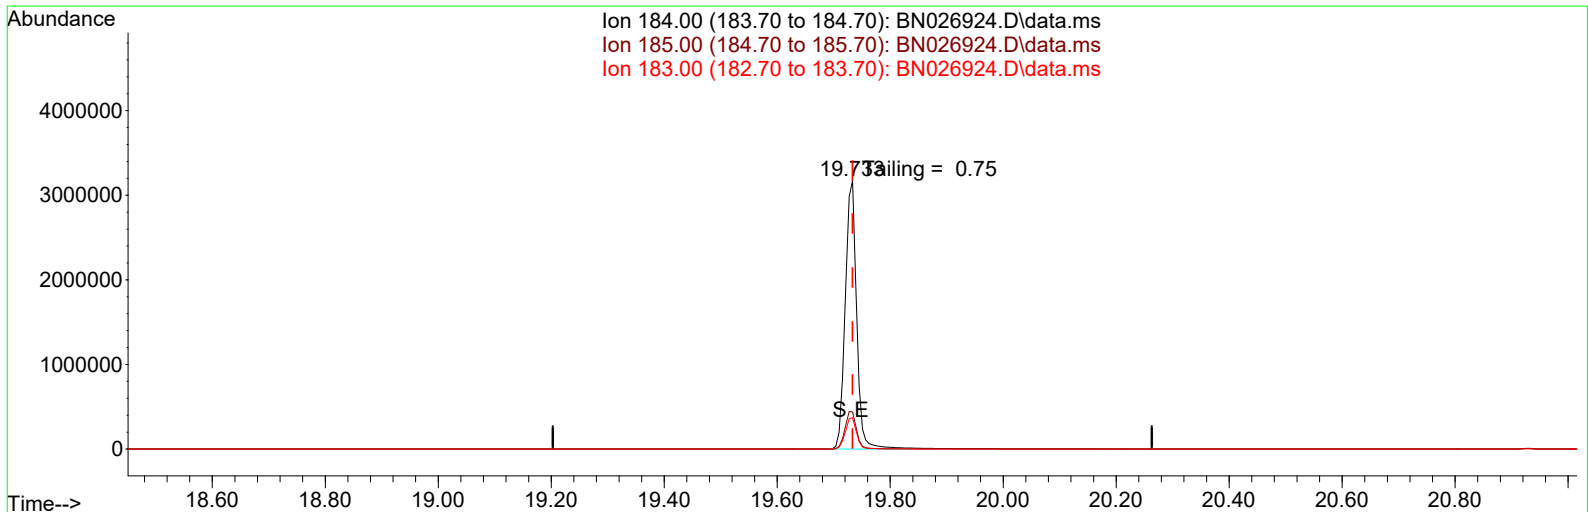

TIC: BN026924.D\data.ms

(77) Benzidine**19.733min (0.000) 2457638.72 ng****response 4469700**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.85
183.00	13.20	11.73
0.00	0.00	0.00