


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081623\
Data File : BN026924.D
Acq On : 16 Aug 2023 09:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 16 15:56:02 2023

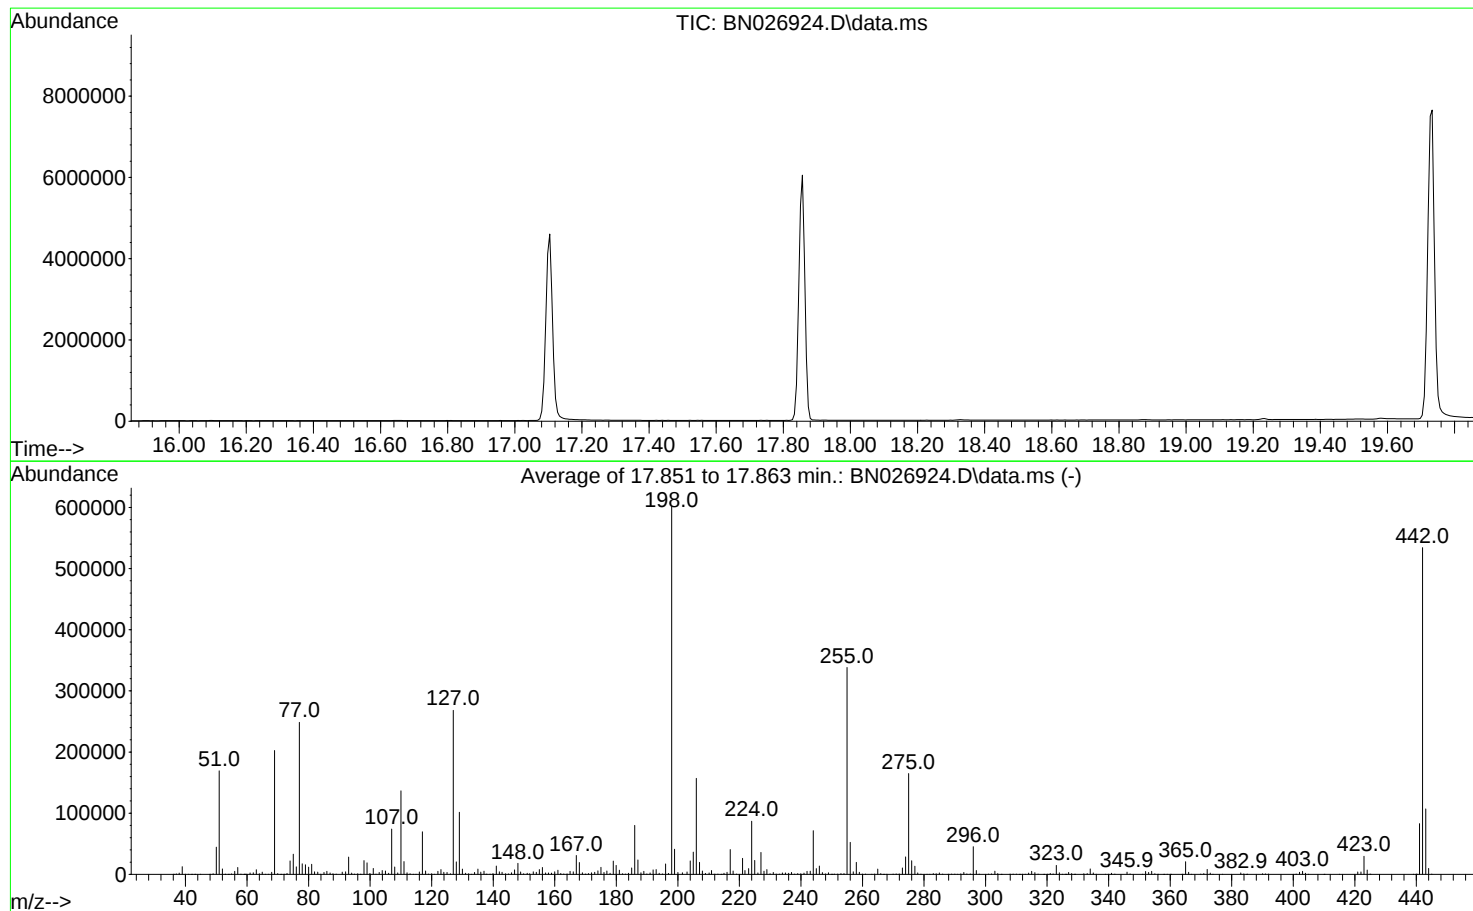




AutoFind: Scans 2544, 2545, 2546; Background Corrected with Scan 2536

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.2	169371	PASS
68	69	0.00	2	1.7	3411	PASS
69	198	0.00	100	33.7	202503	PASS
70	69	0.00	2	0.6	1267	PASS
127	198	10	80	44.6	268224	PASS
197	198	0.00	2	0.3	1700	PASS
198	198	100	100	100.0	601557	PASS
199	198	5	9	6.8	41152	PASS
275	198	10	60	27.4	164907	PASS
365	198	1	100	3.4	20723	PASS
441	198	0.01	100	13.8	83048	PASS
442	442	50	100	100.0	534187	PASS
443	442	15	24	20.1	107128	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081623\
Data File : BN026924.D
Acq On : 16 Aug 2023 09:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 17 03:29:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 17 03:29:54 2023
Response via : Initial Calibration

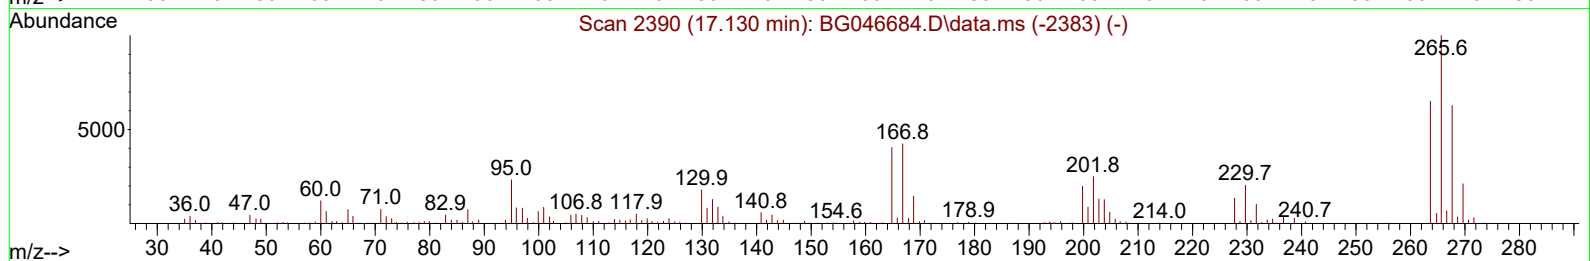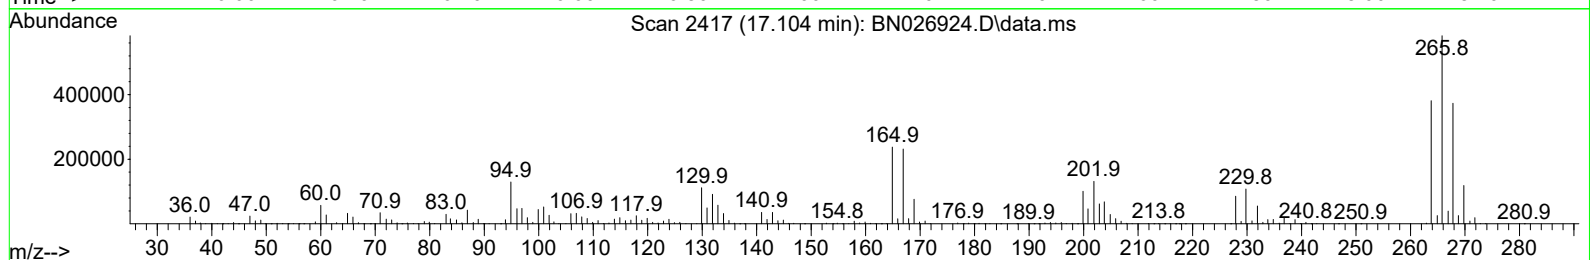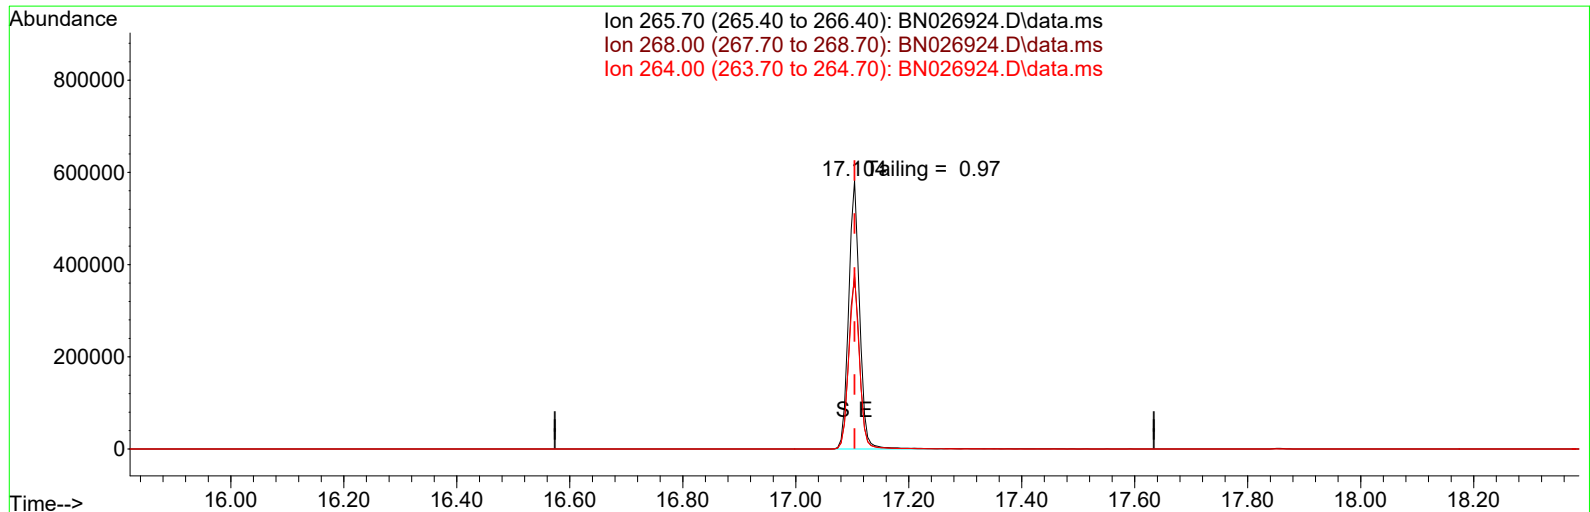

TIC: BN026924.D\data.ms

(70) Pentachlorophenol (C)

17.104min (0.000) 26665.46 ng




response 787669

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.08
264.00	61.60	65.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081623\
Data File : BN026924.D
Acq On : 16 Aug 2023 09:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 17 03:29:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 17 03:29:54 2023
Response via : Initial Calibration

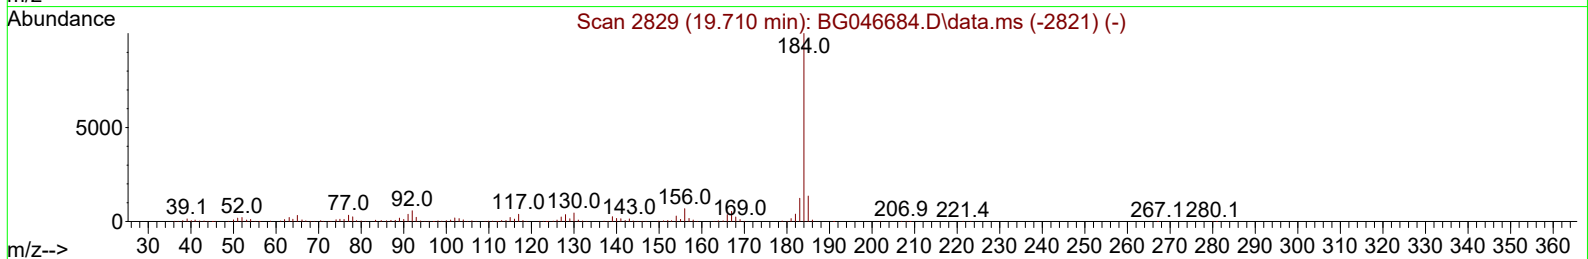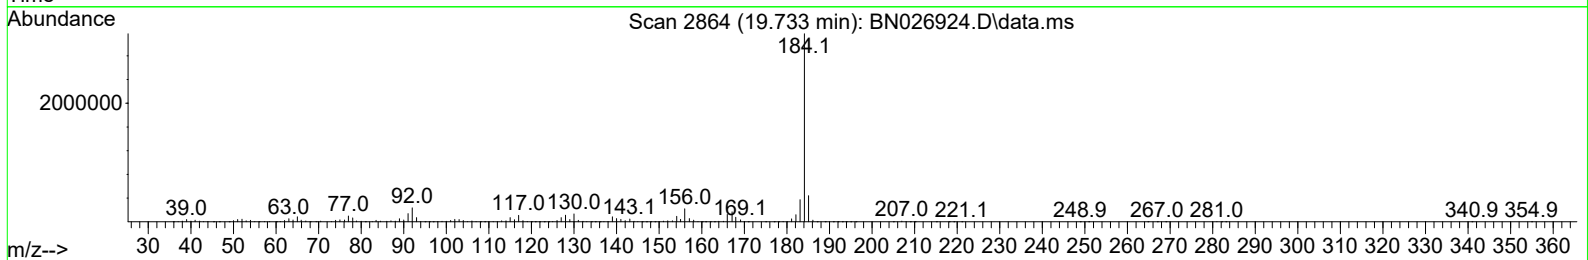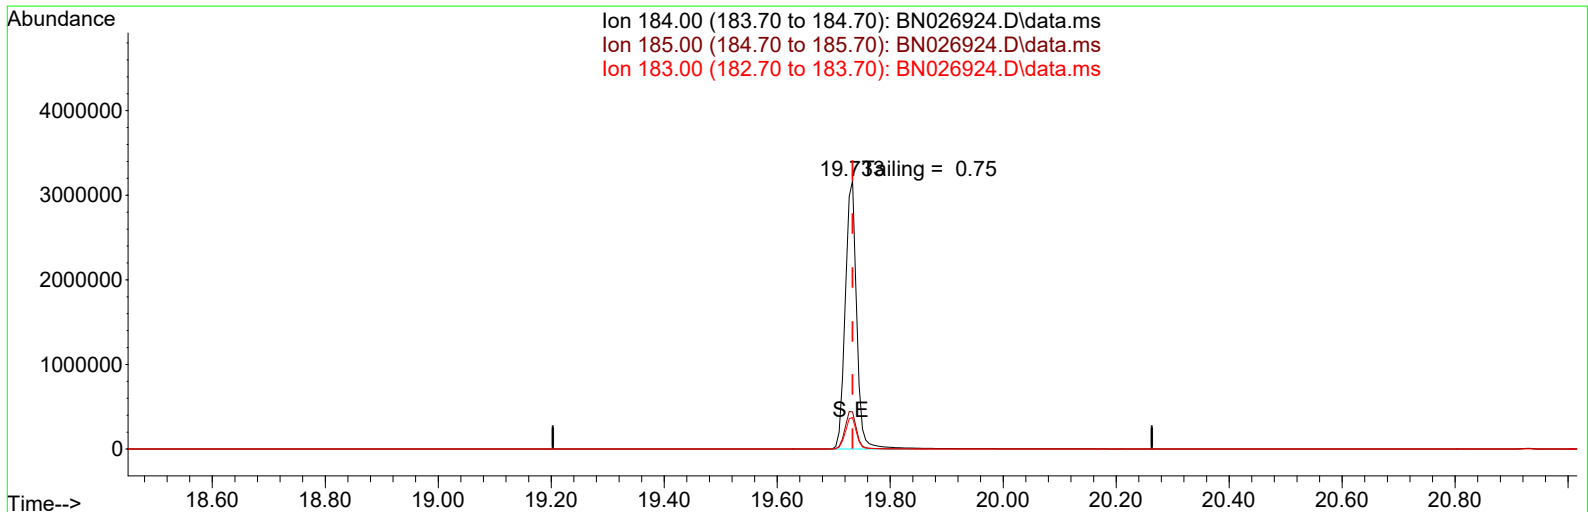

TIC: BN026924.D\data.ms

(77) Benzidine

19.733min (0.000) 2457638.72 ng

response 4469700

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.85
183.00	13.20	11.73
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/16/2023	BNA_N	<u>BN026924.D</u>
Compound Name	Response	Retention Time
DDT	2131633	20.927
DDD	21277	20.539
DDE	675	19.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21952	2153585	1.02

Instrument :
BNA_N
ClientSampleId :
DFTPP