


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015954.D
Acq On : 19 Aug 2021 01:27
Operator : CG/JU
Sample : M3399-11
Misc :
ALS Vial : 59 Sample Multiplier: 1



Quant Time: Aug 19 02:29:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 17 09:43:53 2021
Response via : Initial Calibration

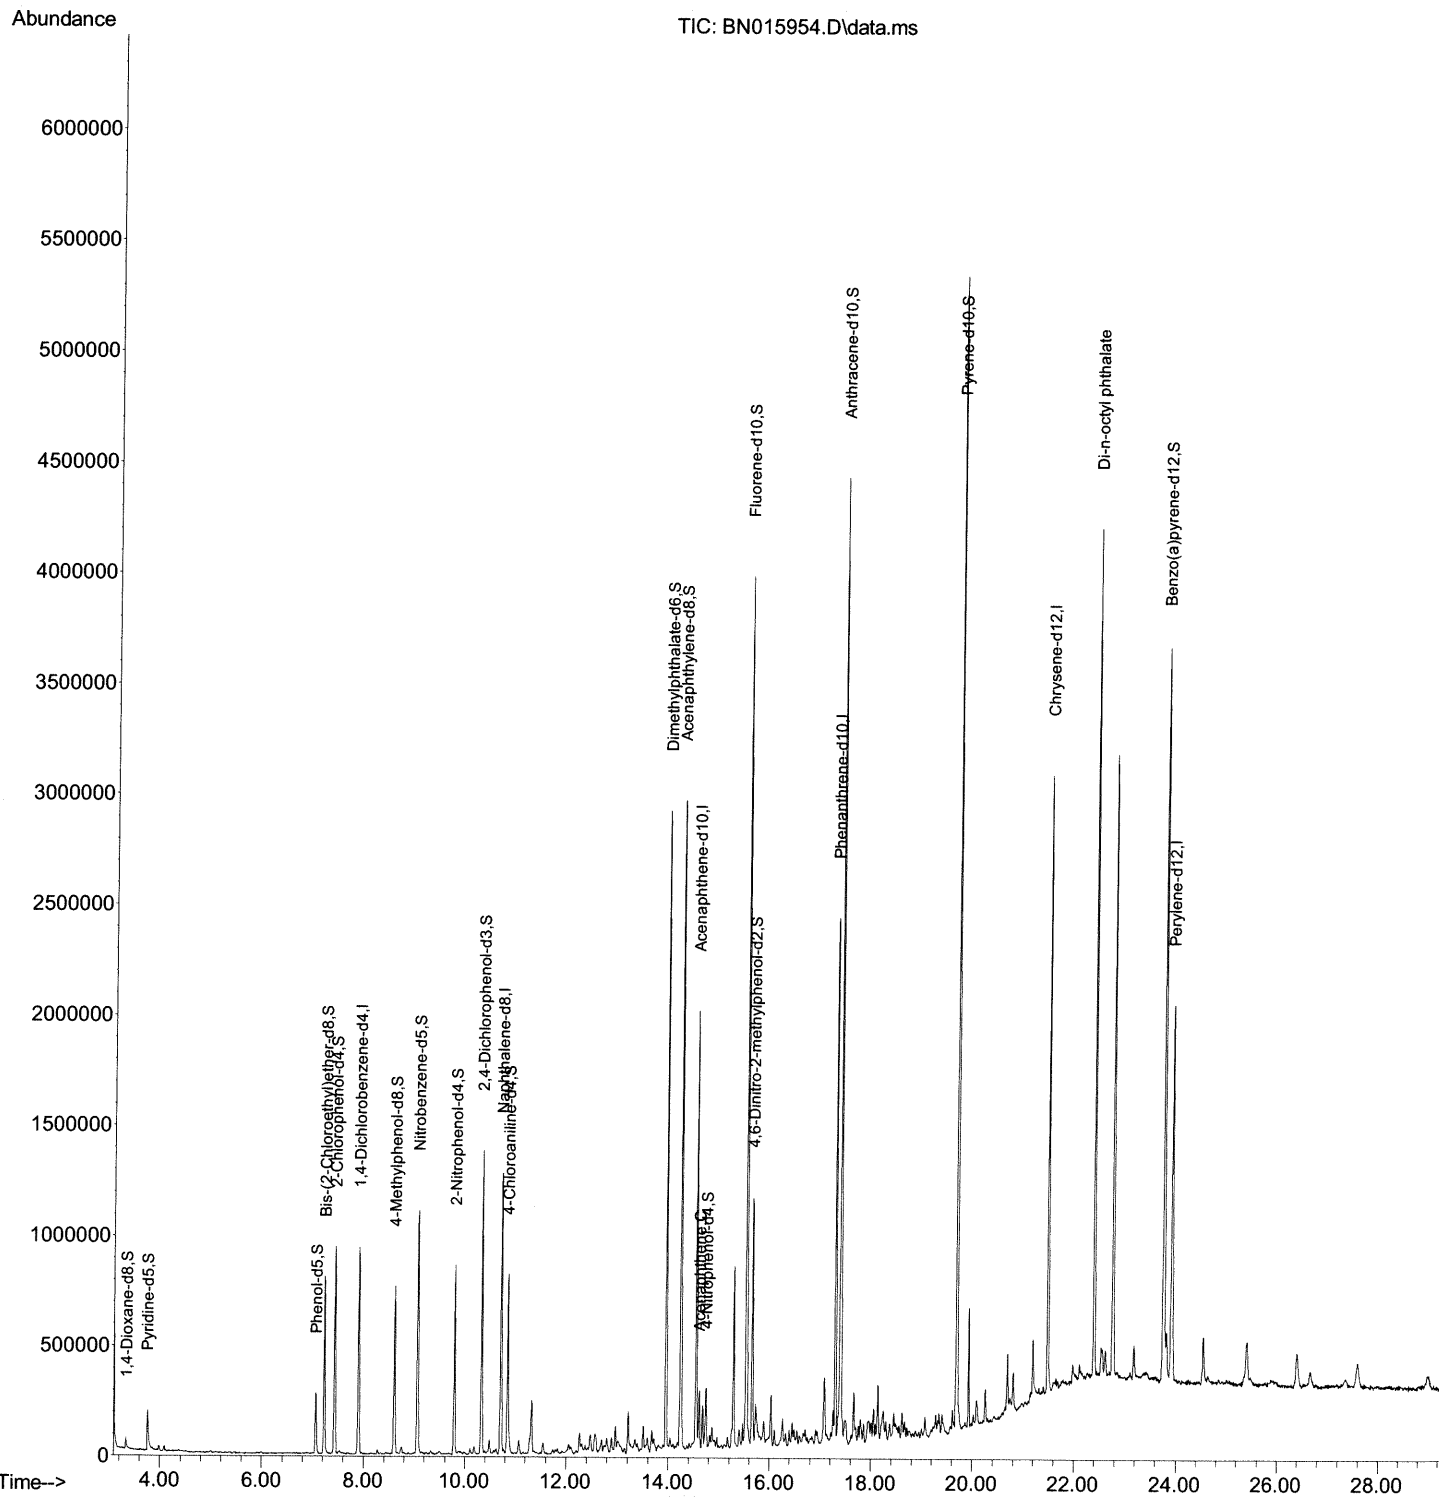

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015954.D
 Acq On : 19 Aug 2021 01:27
 Operator : CG/JU
 Sample : M3399-11
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Quant Time: Aug 19 02:29:50 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Quant Title : SVOA CALIBRATION
 Qlast Update : Tue Aug 17 09:43:53 2021
 Response via : Initial Calibration

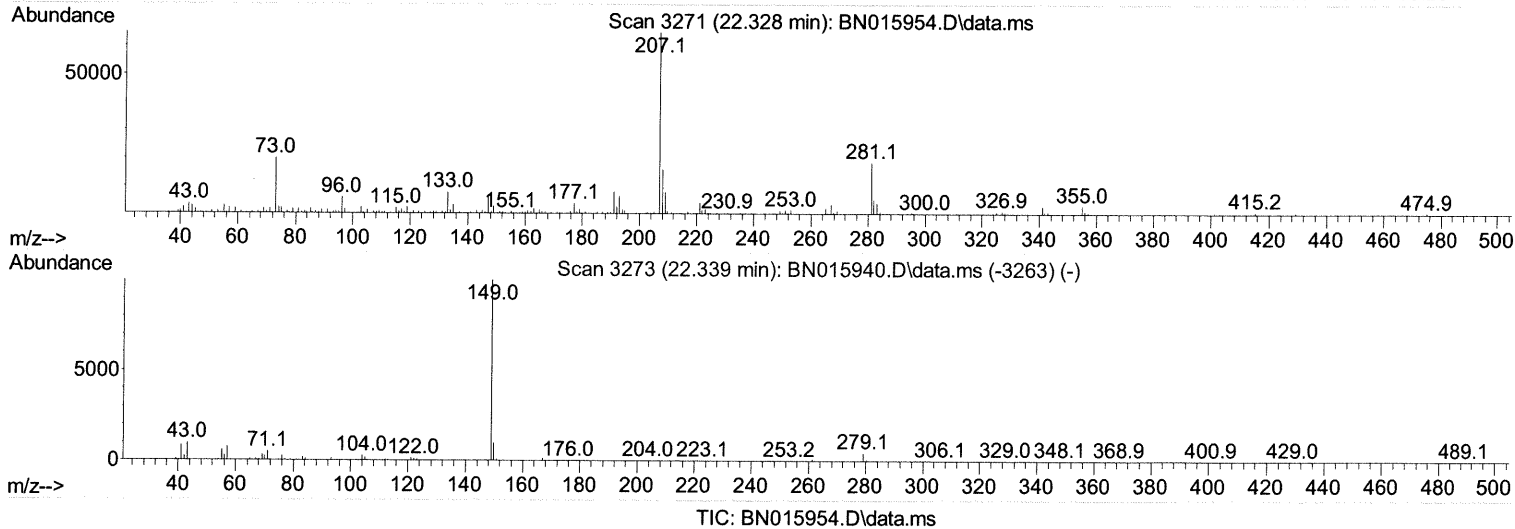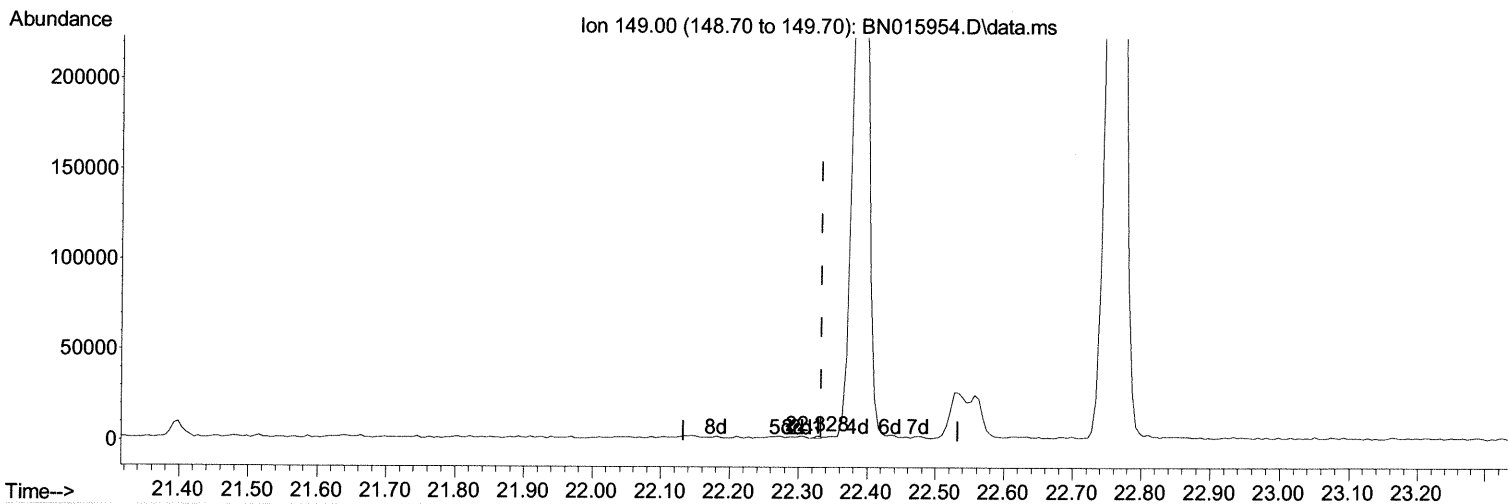

(89) Di-n-octyl phthalate

22.328min (-0.006) 0.01 ng/ul




response 860

Ion	Exp%	Act%
149.00	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015954.D
 Acq On : 19 Aug 2021 01:27
 Operator : CG/JU
 Sample : M3399-11
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Quant Time: Aug 19 02:29:50 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 17 09:43:53 2021
 Response via : Initial Calibration

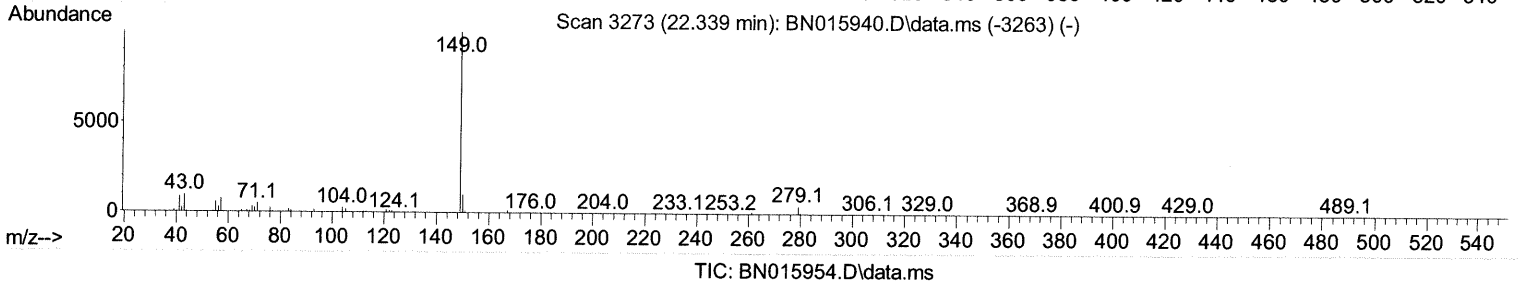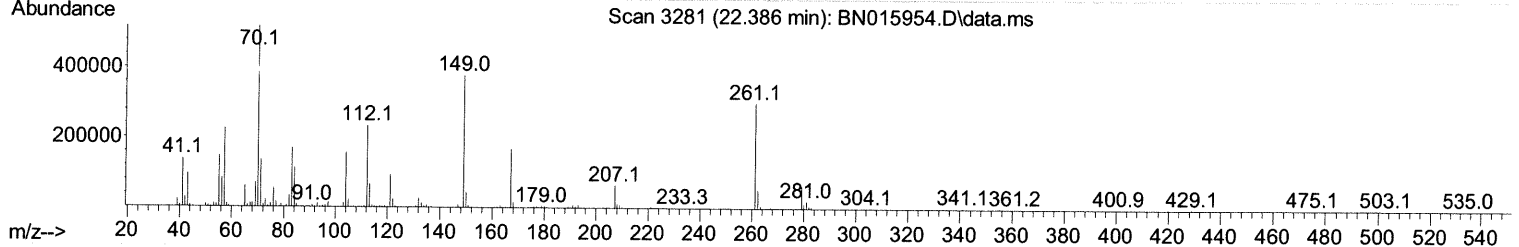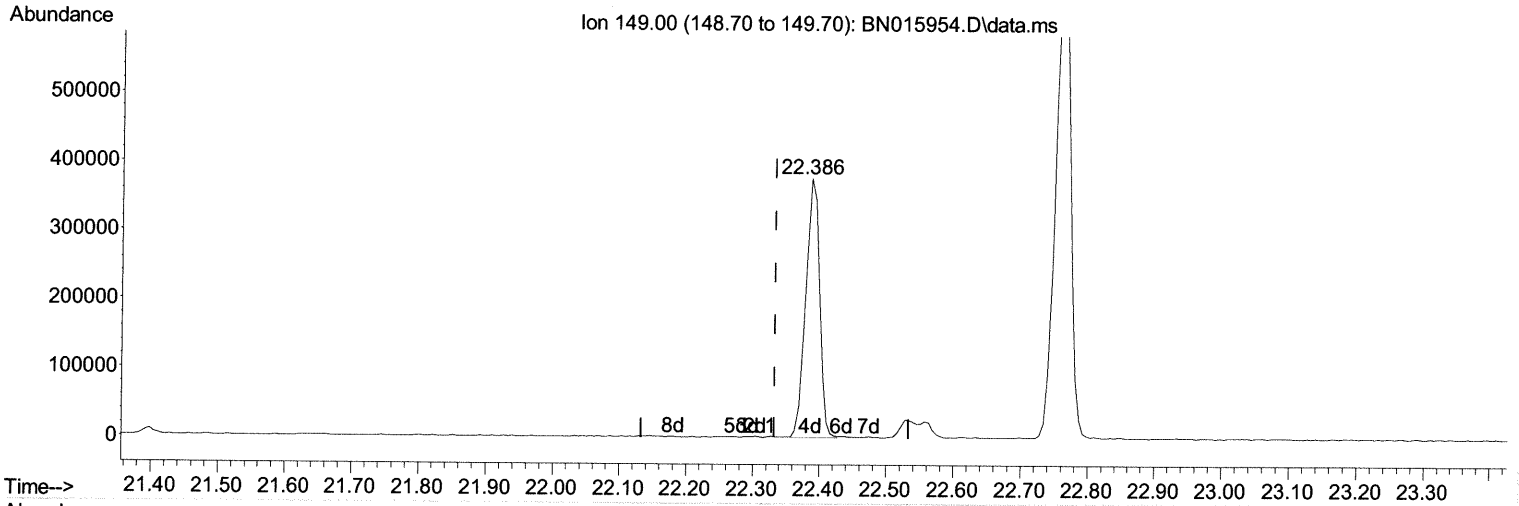

(89) Di-n-octyl phthalate

22.386min (+ 0.053) 6.61 ng/ul m 08/20/21 JU

response 538555

Ion	Exp%	Act%
149.00	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015954.D
 Acq On : 19 Aug 2021 01:27
 Operator : CG/JU
 Sample : M3399-11
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Quant Time: Aug 19 02:29:50 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 17 09:43:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	248941	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	1053580	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.546	164	665142	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.298	188	1369738	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	1276400	20.000	ng/ul	0.00
88) Perylene-d12	23.904	264	1288187	20.000	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	29772	4.659	ng/ul	0.00
4) Pyridine-d5	3.752	84	112087	6.275	ng/ul	0.00
7) Phenol-d5	7.058	99	156210	6.937	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	378458	27.297	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	400667	25.005	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	276341	15.778	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	245068	31.603	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	253614	34.945	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	464394	29.570	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	409005	17.109	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	1814212	37.217	ng/ul	0.00
49) Acenaphthylene-d8	14.240	160	2053203	33.633	ng/ul	0.00
54) 4-Nitrophenol-d4	14.746	143	63064	7.315	ng/ul	0.01
60) Fluorene-d10	15.540	176	1501684	35.317	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	226690	30.989	ng/ul	0.00
73) Anthracene-d10	17.398	188	2491134	38.802	ng/ul	0.00
81) Pyrene-d10	19.692	212	2747521	39.964	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.745	264	2622067	37.646	ng/ul	0.00

Target Compounds				Qvalue		
52) Acenaphthene	14.610	153	100513	2.395	ng/ul	98
89) Di-n-octyl phthalate	22.386	149	538555m >	6.606	ng/ul >	08/20/21 JU

(#) = qualifier out of range (m) = manual integration (+) = signals summed