

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015906.D
 Acq On : 17 Aug 2021 18:42
 Operator : CG/JU
 Sample : M3364-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBK95

Quant Time: Aug 18 01:09:09 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 17 09:43:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	277703	20.000	ng/ul	0.00
20) Naphthalene-d8	10.711	136	1135367	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.551	164	685269	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.298	188	1325911	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	1236612	20.000	ng/ul	0.00
88) Perylene-d12	23.916	264	1264249	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	42009	5.893	ng/uL	0.00
4) Pyridine-d5	3.746	84	236193	11.854	ng/ul	0.00
7) Phenol-d5	7.058	99	170579	6.791	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	460412	29.769	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	457925	25.619	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	323632	16.564	ng/ul	0.00
21) Nitrobenzene-d5	9.064	128	301857	36.123	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	302259	38.648	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	531368	31.397	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	280672	10.895	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	1880975	37.454	ng/ul	0.00
49) Acenaphthylene-d8	14.240	160	2307708	36.692	ng/ul	0.00
54) 4-Nitrophenol-d4	14.734	143	55453	6.243	ng/ul	0.00
60) Fluorene-d10	15.540	176	1580313	36.074	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	232814	32.878	ng/ul	0.00
73) Anthracene-d10	17.398	188	2332576	37.533	ng/ul	0.00
81) Pyrene-d10	19.692	212	2561275	38.453	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.757	264	2436799	35.648	ng/ul	0.00


Target Compounds					Qvalue
8) Phenol	7.081	94	29862	1.166 ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015906.D
Acq On : 17 Aug 2021 18:42
Operator : CG/JU
Sample : M3364-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBK95

Quant Time: Aug 18 01:09:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 17 09:43:53 2021
Response via : Initial Calibration

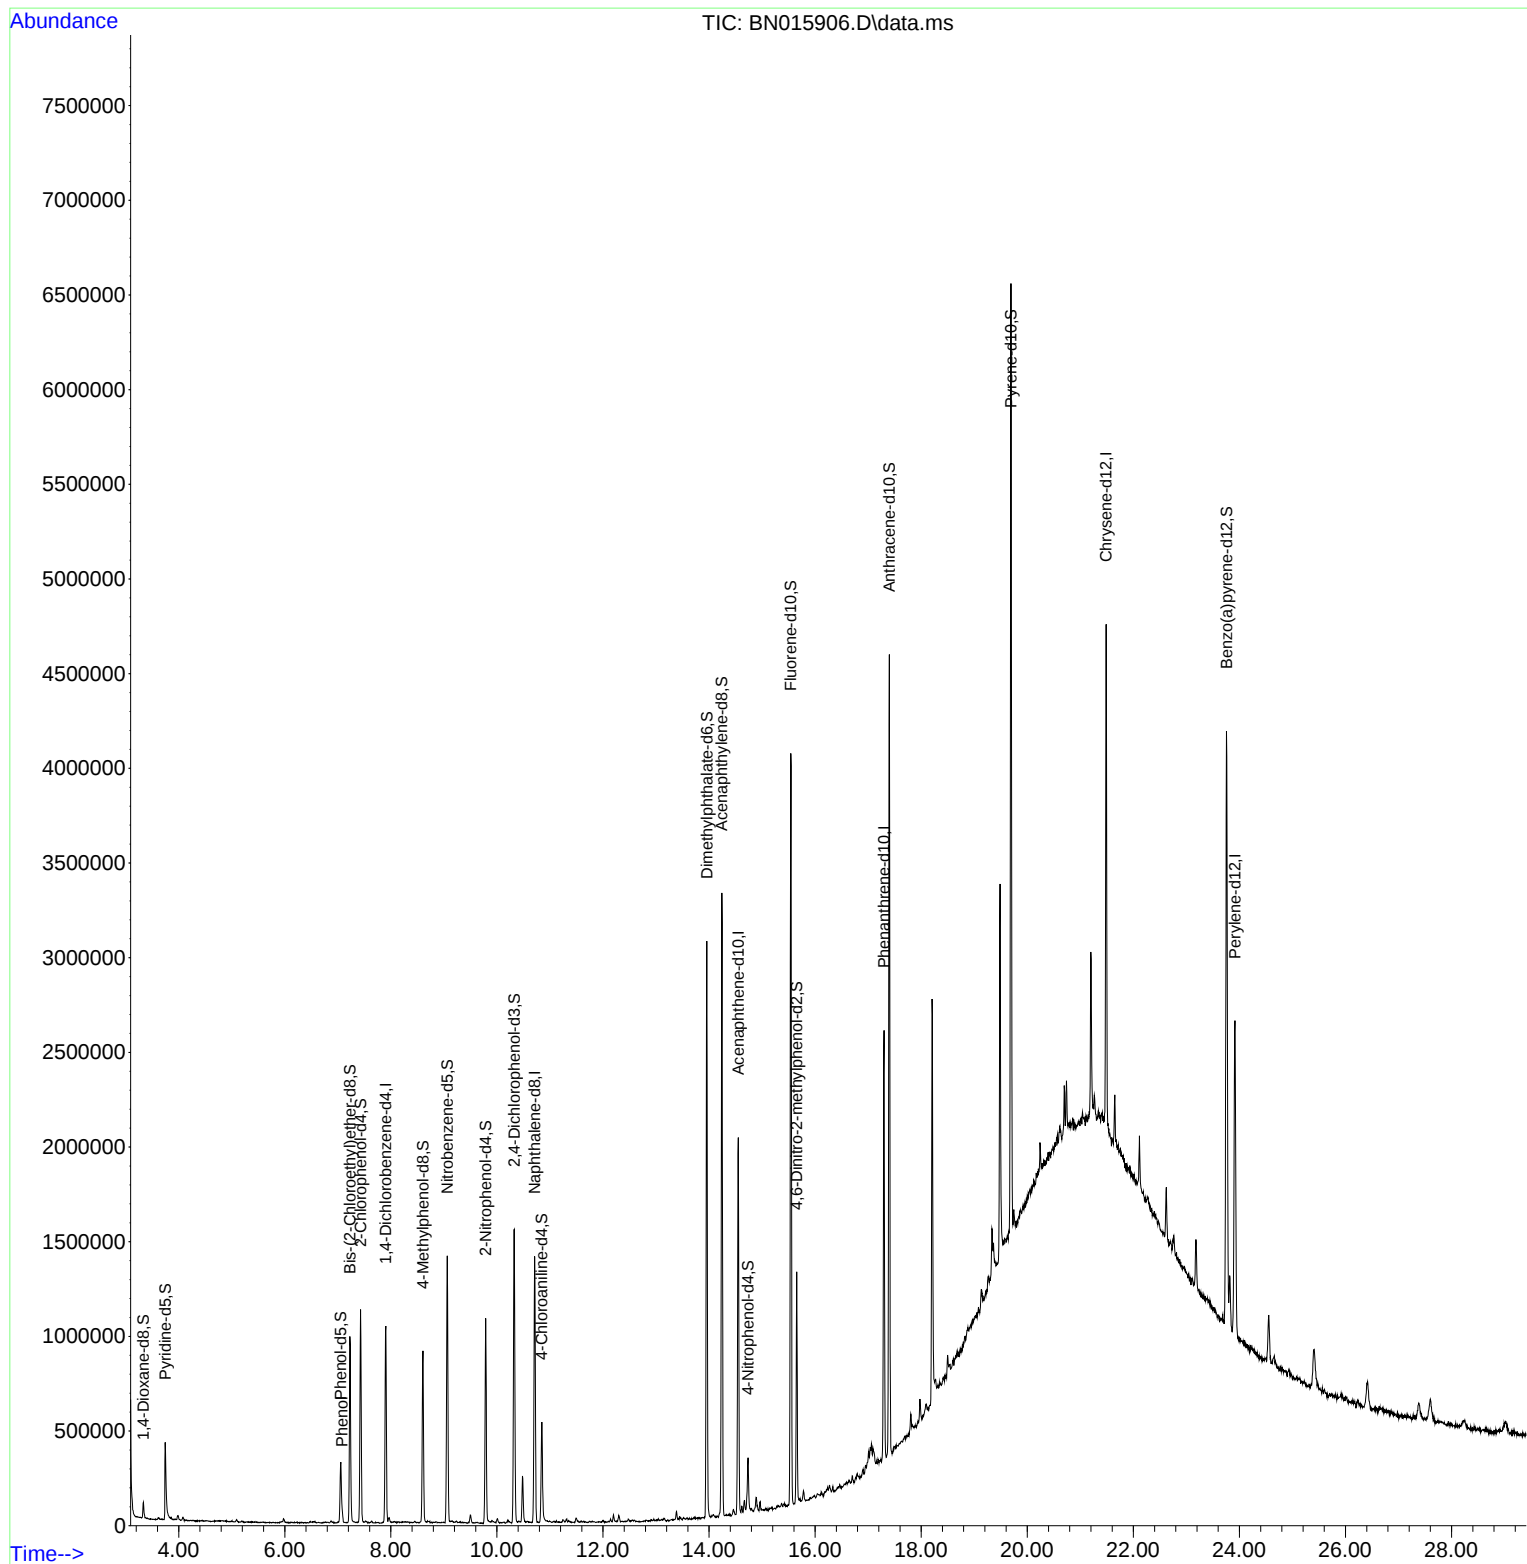

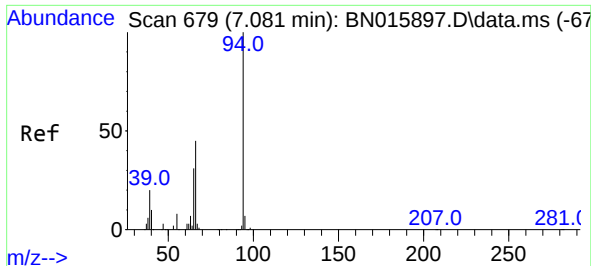

#8
Phenol
Concen: 1.166 ng/ul
RT: 7.081 min Scan# 679
Delta R.T. 0.000 min
Lab File: BN015906.D
Acq: 17 Aug 2021 18:42

Instrument :
BNA_N
ClientSampleId :
DBK95

Tgt Ion:	94	Resp:	29862
Ion	Ratio	Lower	Upper
94	100		
65	27.6	27.0	40.6
66	49.0	37.8	56.8

