

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015922.D
 Acq On : 18 Aug 2021 05:39
 Operator : CG/JU
 Sample : M3364-14
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBK98

Quant Time: Aug 18 06:24:43 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 17 09:43:53 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	262261	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	1099388	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.545	164	703788	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.298	188	1418083	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	1388062	20.000	ng/ul	0.00
88) Perylene-d12	23.910	264	1378618	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	38022	5.647	ng/uL	0.00
4) Pyridine-d5	3.758	84	68993	3.667	ng/ul	0.01
7) Phenol-d5	7.058	99	163284	6.883	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	449102	30.747	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	449580	26.633	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	315573	17.103	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	296509	36.644	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	306744	40.505	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	520181	31.742	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	483304	19.375	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	2007358	38.918	ng/ul	0.00
49) Acenaphthylene-d8	14.240	160	2323676	35.973	ng/ul	0.00
54) 4-Nitrophenol-d4	14.740	143	61631	6.756	ng/ul	0.00
60) Fluorene-d10	15.539	176	1663705	36.978	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	257663	34.023	ng/ul	0.00
73) Anthracene-d10	17.398	188	2800592	42.135	ng/ul	0.00
81) Pyrene-d10	19.692	212	3256649	43.558	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.757	264	3027813	40.620	ng/ul	0.00
Target Compounds						
77) Carbazole	17.698	167	104522	1.510	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015922.D
Acq On : 18 Aug 2021 05:39
Operator : CG/JU
Sample : M3364-14
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBK98

Quant Time: Aug 18 06:24:43 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 17 09:43:53 2021
Response via : Initial Calibration

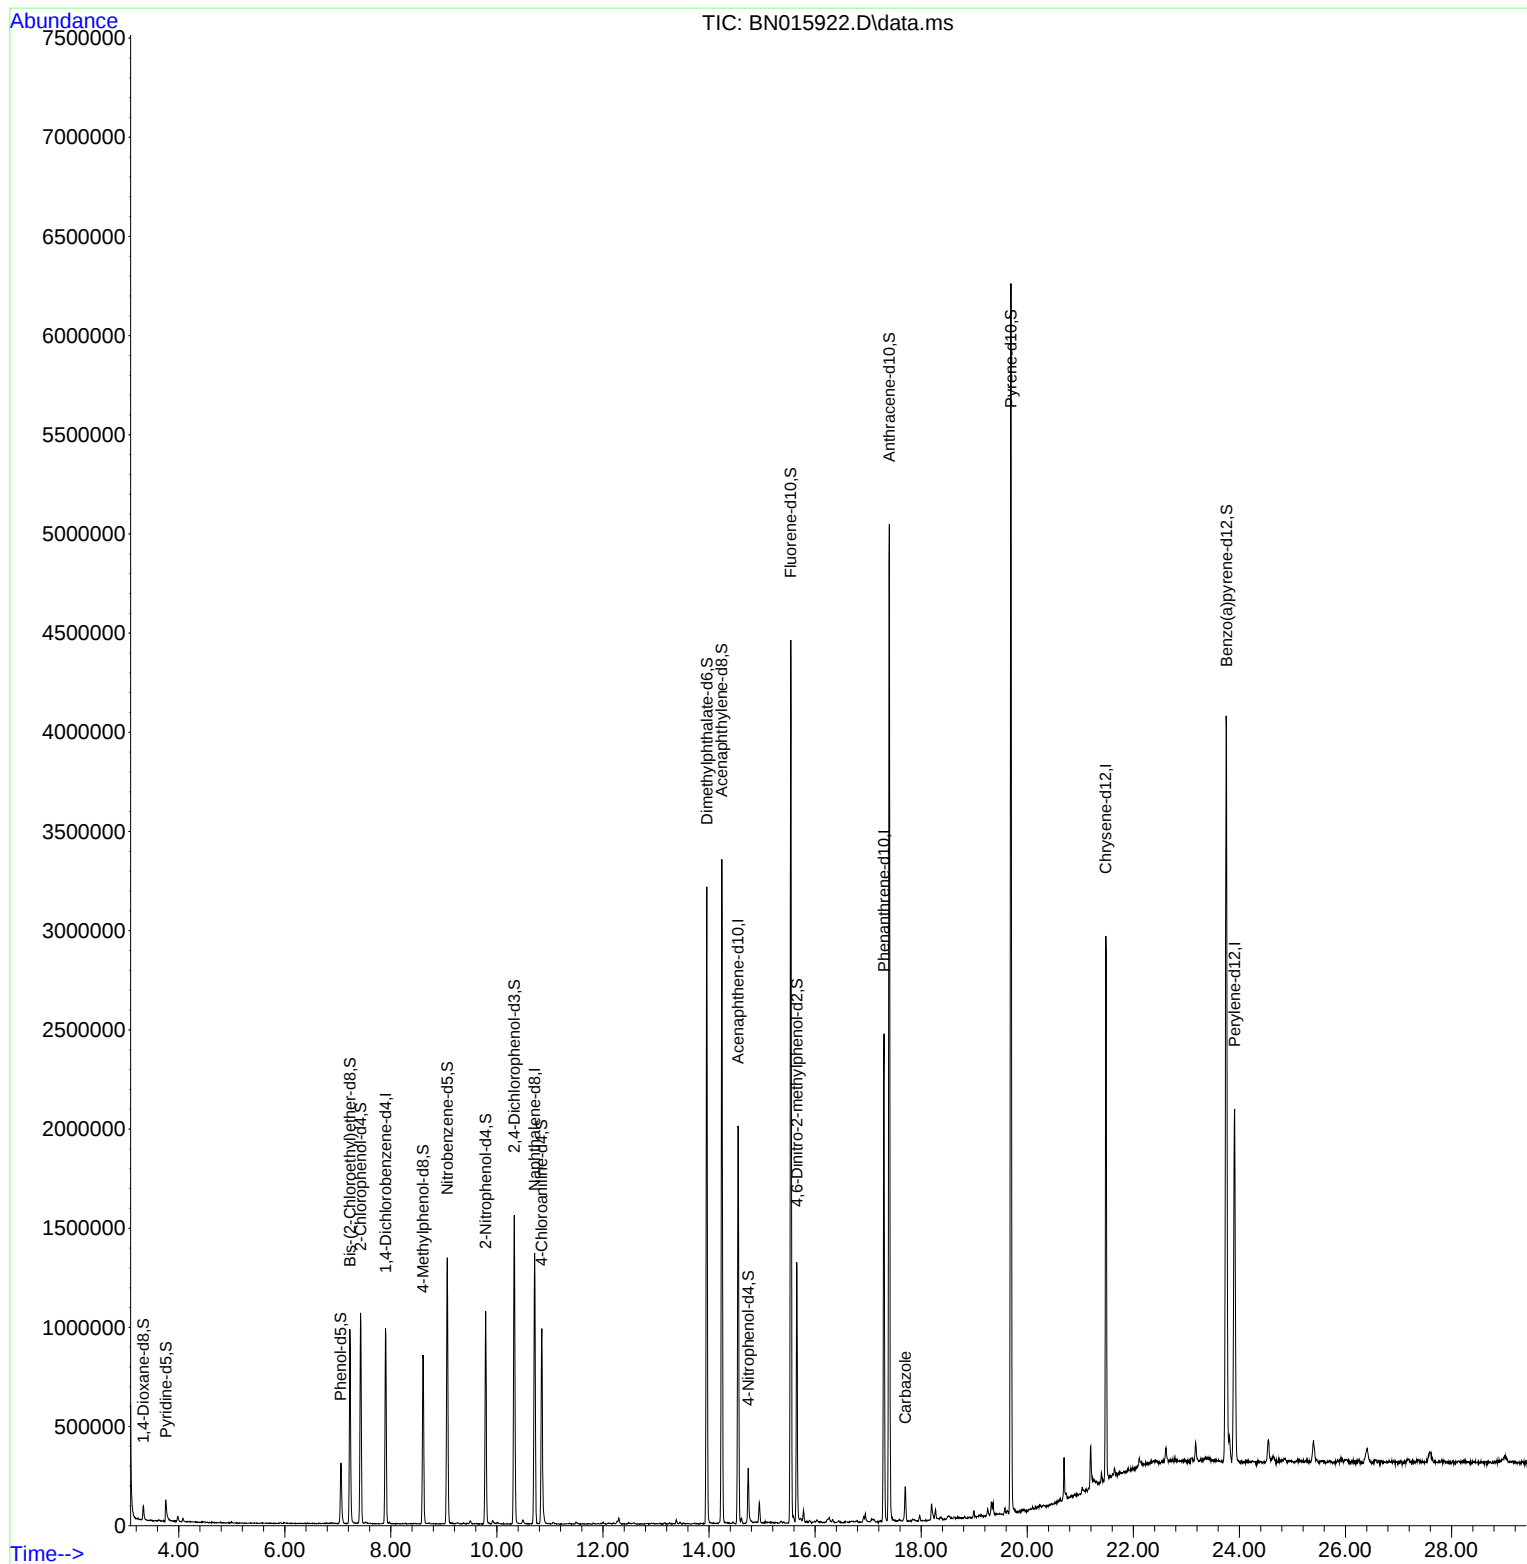

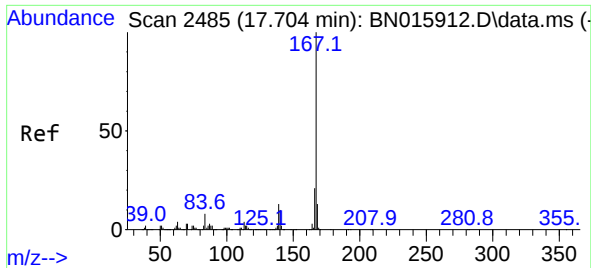

#77
Carbazole
Concen: 1.510 ng/ul
RT: 17.698 min Scan# 2484
Delta R.T. -0.000 min
Lab File: BN015922.D
Acq: 18 Aug 2021 05:39

Instrument :
BNA_N
ClientSampleId :
DBK98

Tgt Ion:167 Resp: 104522
Ion Ratio Lower Upper
167 100
166 21.1 17.1 25.7
139 15.2 11.6 17.4

