

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015930.D
 Acq On : 18 Aug 2021 10:47
 Operator : CG/JU
 Sample : M3364-10
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBK94

Quant Time: Aug 18 11:24:13 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 17 09:43:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	216600	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	907116	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.545	164	570666	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.298	188	1163048	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	1140460	20.000	ng/ul	0.00
88) Perylene-d12	23.904	264	1119290	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	21660	3.895	ng/uL	0.00
4) Pyridine-d5	3.758	84	45636	2.937	ng/ul	0.01
7) Phenol-d5	7.058	99	74642	3.810	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	257925	21.381	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	241722	17.338	ng/ul	0.00
15) 4-Methylphenol-d8	8.604	113	142571	9.356	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	161127	24.133	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	153093	24.501	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	267040	19.749	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	319679	15.532	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	1013661	24.237	ng/ul	0.00
49) Acenaphthylene-d8	14.239	160	1229727	23.479	ng/ul	0.00
54) 4-Nitrophenol-d4	14.739	143	20501	2.771	ng/ul	0.00
60) Fluorene-d10	15.539	176	904433	24.792	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	96673	15.564	ng/ul	0.00
73) Anthracene-d10	17.392	188	1472616	27.014	ng/ul	0.00
81) Pyrene-d10	19.686	212	1665919	27.120	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.751	264	1593075	26.324	ng/ul	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.945	266	12530	1.531	ng/ul	96
96) Benzo(g,h,i)perylene	27.180	276	114421	1.675	ng/ul#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015930.D
Acq On : 18 Aug 2021 10:47
Operator : CG/JU
Sample : M3364-10
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBK94

Quant Time: Aug 18 11:24:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 17 09:43:53 2021
Response via : Initial Calibration




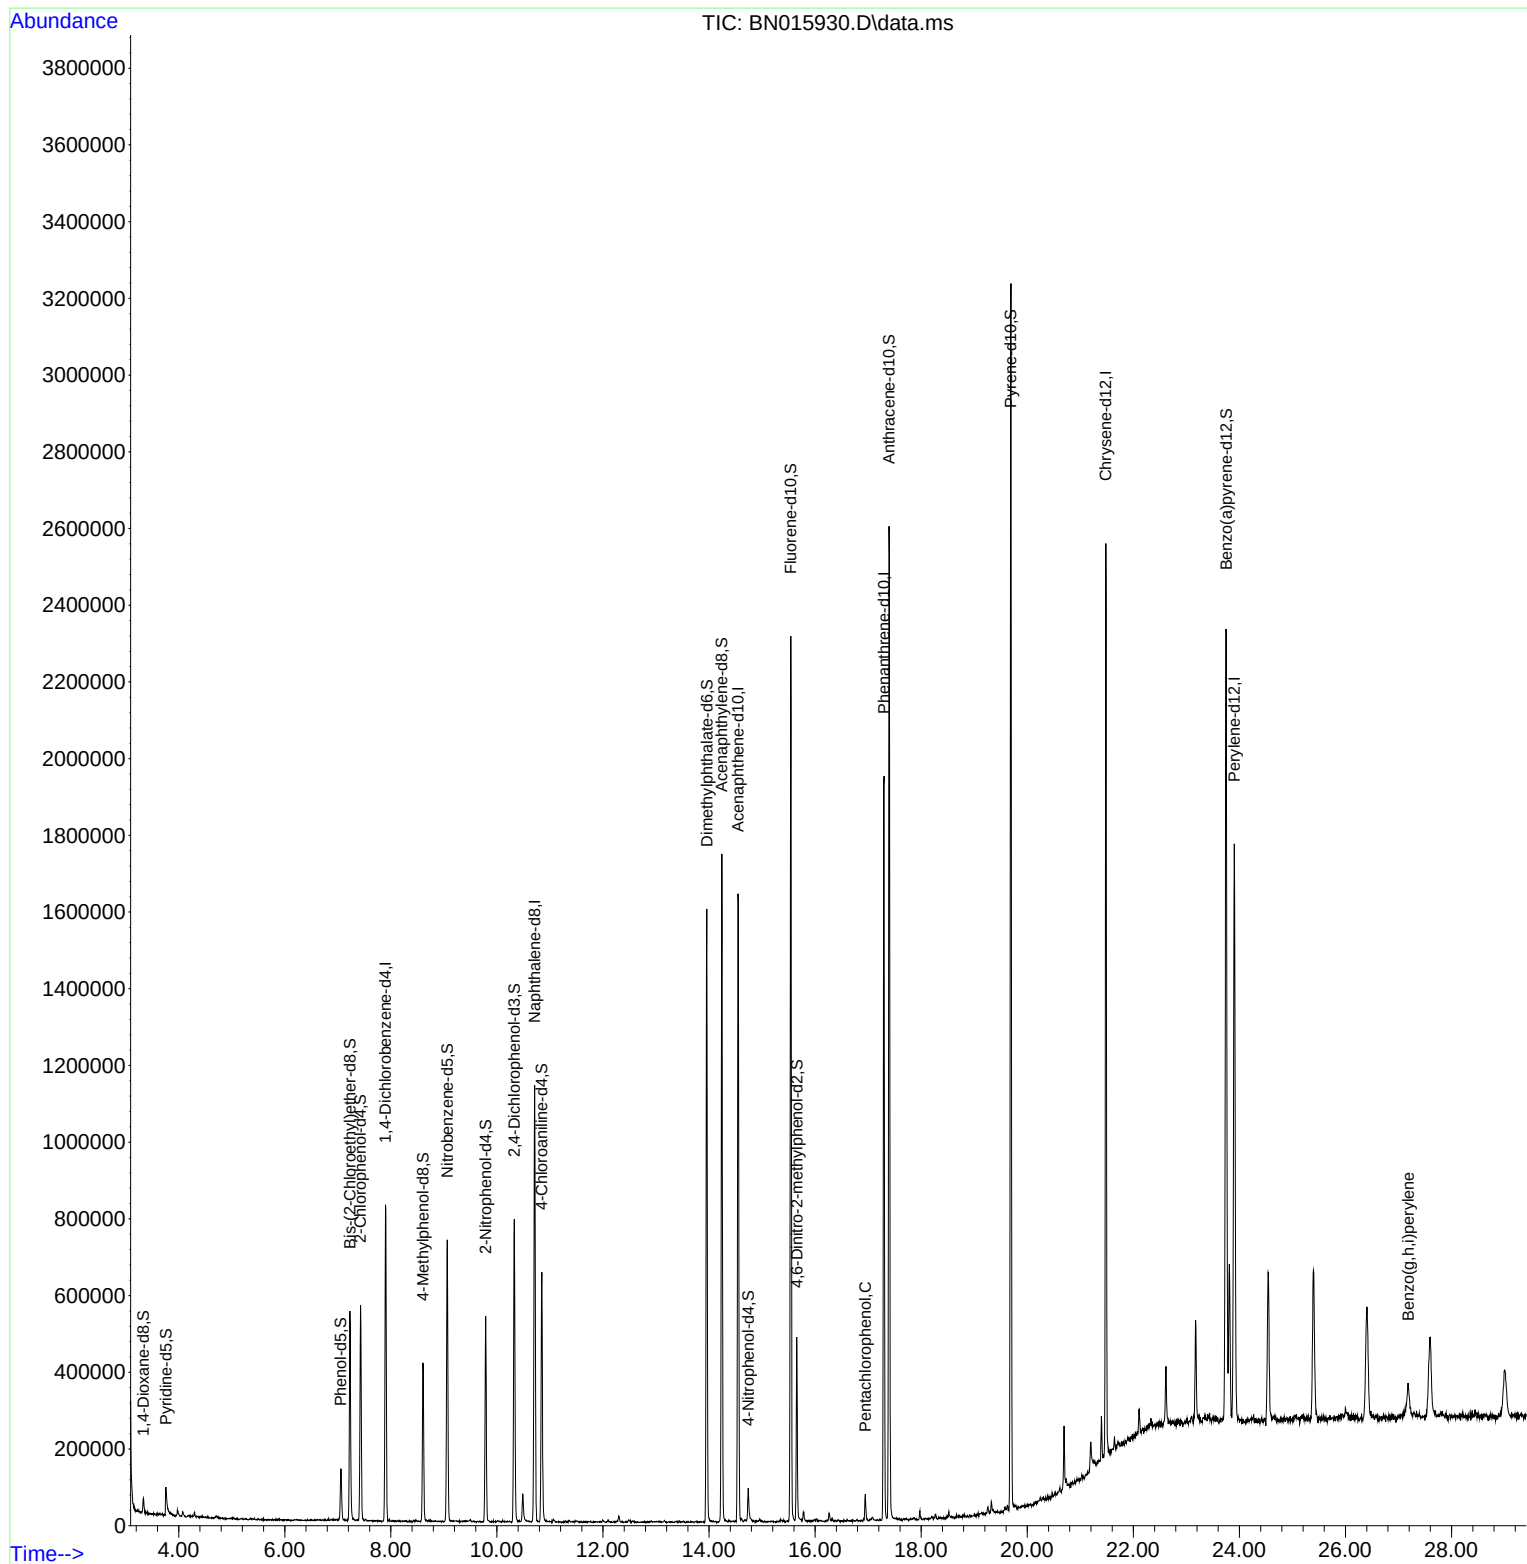


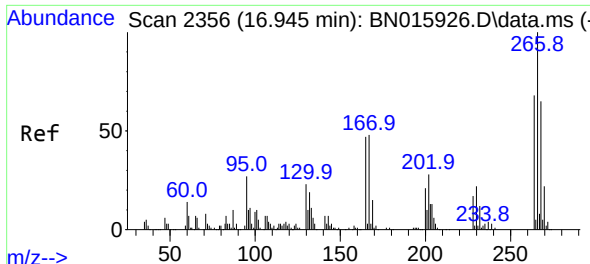

#71
 Pentachlorophenol
 Concen: 1.531 ng/ul
 RT: 16.945 min Scan# 2356
 Delta R.T. -0.000 min
 Lab File: BN015930.D
 Acq: 18 Aug 2021 10:47

Instrument :
 BNA_N
 ClientSampleId :
 DBK94

Tgt Ion:	266	Resp:	12530
Ion Ratio	Lower	Upper	
266	100		
264	64.0	53.8	80.6
268	62.0	52.7	79.1

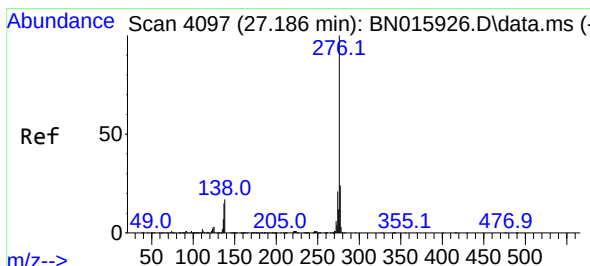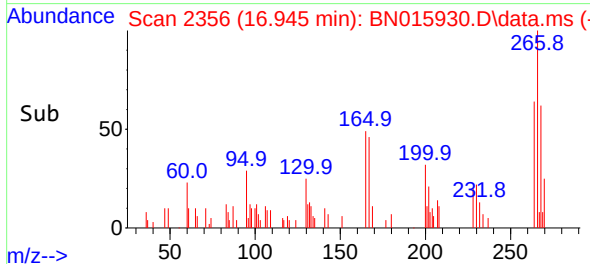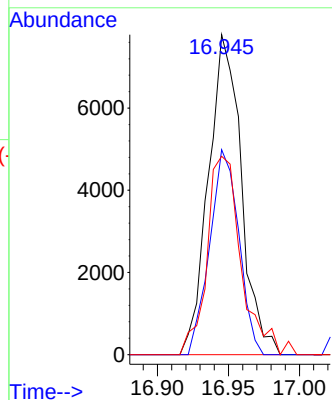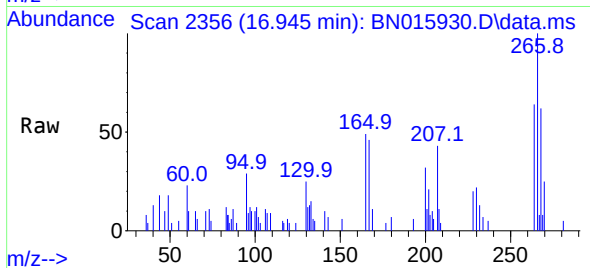

#96
 Benzo(g,h,i)perylene
 Concen: 1.675 ng/ul
 RT: 27.180 min Scan# 4096
 Delta R.T. -0.012 min
 Lab File: BN015930.D
 Acq: 18 Aug 2021 10:47

Tgt Ion:	276	Resp:	114421
Ion Ratio	Lower	Upper	
276	100		
138	24.7	13.4	20.0#
277	22.1	18.5	27.7

