

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015933.D
 Acq On : 18 Aug 2021 12:36
 Operator : CG/JU
 Sample : M3364-20
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKC7

Quant Time: Aug 18 13:24:33 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 17 09:43:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.904	152	298861	20.000	ng/u1	0.00
20) Naphthalene-d8	10.710	136	1215787	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.545	164	758858	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.298	188	1541771	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	1503842	20.000	ng/u1	0.00
88) Perylene-d12	23.910	264	1488113	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	42922	5.594	ng/uL	0.00
4) Pyridine-d5	3.752	84	121637	5.673	ng/u1	0.00
7) Phenol-d5	7.057	99	172156	6.368	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	421550	25.326	ng/u1	0.00
11) 2-Chlorophenol-d4	7.428	132	437210	22.728	ng/u1	0.00
15) 4-Methylphenol-d8	8.610	113	317388	15.095	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	264023	29.505	ng/u1	0.00
24) 2-Nitrophenol-d4	9.787	143	275141	32.853	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	496268	27.384	ng/u1	0.00
31) 4-Chloroaniline-d4	10.846	131	676186	24.512	ng/u1	0.00
46) Dimethylphthalate-d6	13.957	166	1851447	33.291	ng/u1	0.00
49) Acenaphthylene-d8	14.239	160	2135216	30.657	ng/u1	0.00
54) 4-Nitrophenol-d4	14.739	143	61946	6.298	ng/u1	0.00
60) Fluorene-d10	15.539	176	1539350	31.732	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	223440	27.137	ng/u1	0.00
73) Anthracene-d10	17.398	188	2512862	34.773	ng/u1	0.00
81) Pyrene-d10	19.692	212	2890044	35.679	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.757	264	2743207	34.094	ng/u1	0.00


Target Compounds					Qvalue
52) Acenaphthene	14.610	153	52402	1.094 ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015933.D
Acq On : 18 Aug 2021 12:36
Operator : CG/JU
Sample : M3364-20
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKC7

Quant Time: Aug 18 13:24:33 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 17 09:43:53 2021
Response via : Initial Calibration

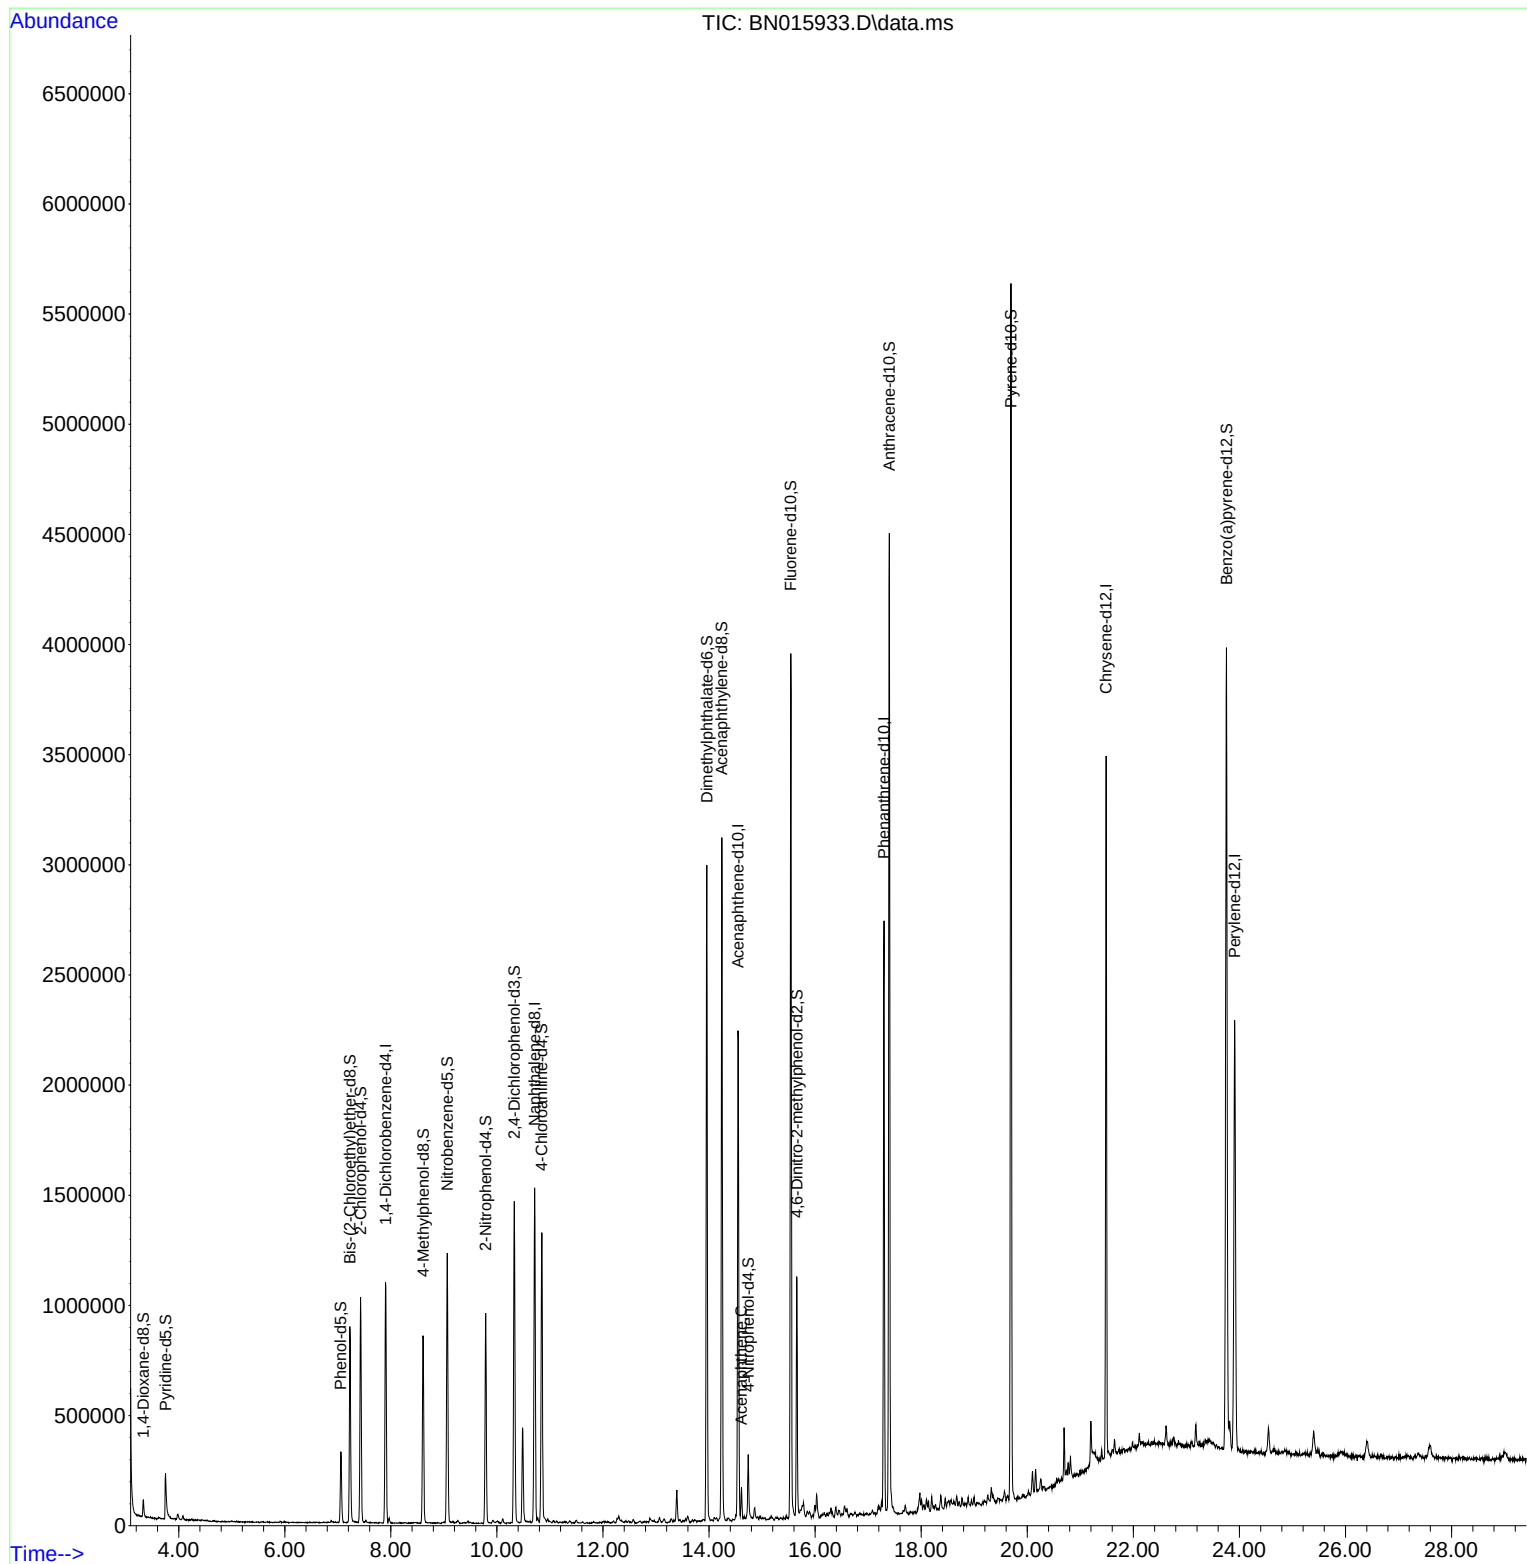

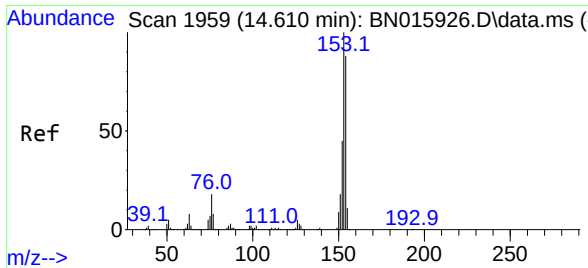

#52
Acenaphthene
Concen: 1.094 ng/ul
RT: 14.610 min Scan# 1959
Delta R.T. -0.006 min
Lab File: BN015933.D
Acq: 18 Aug 2021 12:36

Instrument :
BNA_N
ClientSampleId :
DBKC7

Tgt Ion:	153	Resp:	52402
Ion Ratio	Lower	Upper	
153	100		
152	48.0	38.6	57.8
154	85.7	69.3	103.9

