

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015937.D
 Acq On : 18 Aug 2021 15:03
 Operator : CG/JU
 Sample : M3362-01
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JMXD6

Quant Time: Aug 18 17:13:06 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 17 09:43:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.904	152	240844	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	1008475	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.551	164	652145	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.298	188	1324536	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	1297255	20.000	ng/ul	0.00
88) Perylene-d12	23.910	264	1267847	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	12379	2.002	ng/uL	0.00
4) Pyridine-d5	3.752	84	88056	5.096	ng/ul	0.00
7) Phenol-d5	7.057	99	236564	10.859	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	148093	11.041	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	185026	11.936	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	192915	11.385	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	90956	12.254	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	91154	13.122	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	175158	11.652	ng/ul	0.00
31) 4-Chloroaniline-d4	10.845	131	252638	11.041	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	611124	12.787	ng/ul	0.00
49) Acenaphthylene-d8	14.239	160	715310	11.951	ng/ul	0.00
54) 4-Nitrophenol-d4	14.739	143	66116	7.821	ng/ul	0.00
60) Fluorene-d10	15.539	176	525082	12.595	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	49521	7.001	ng/ul	0.00
73) Anthracene-d10	17.392	188	844989	13.611	ng/ul	0.00
81) Pyrene-d10	19.692	212	960391	13.745	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.757	264	852942	12.442	ng/ul	0.00
Target Compounds						
					Qvalue	
52) Acenaphthene	14.616	153	63395	1.540	ng/ul	99
72) Phenanthrene	17.339	178	174601	2.425	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015937.D
Acq On : 18 Aug 2021 15:03
Operator : CG/JU
Sample : M3362-01
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JMXD6

Quant Time: Aug 18 17:13:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 17 09:43:53 2021
Response via : Initial Calibration




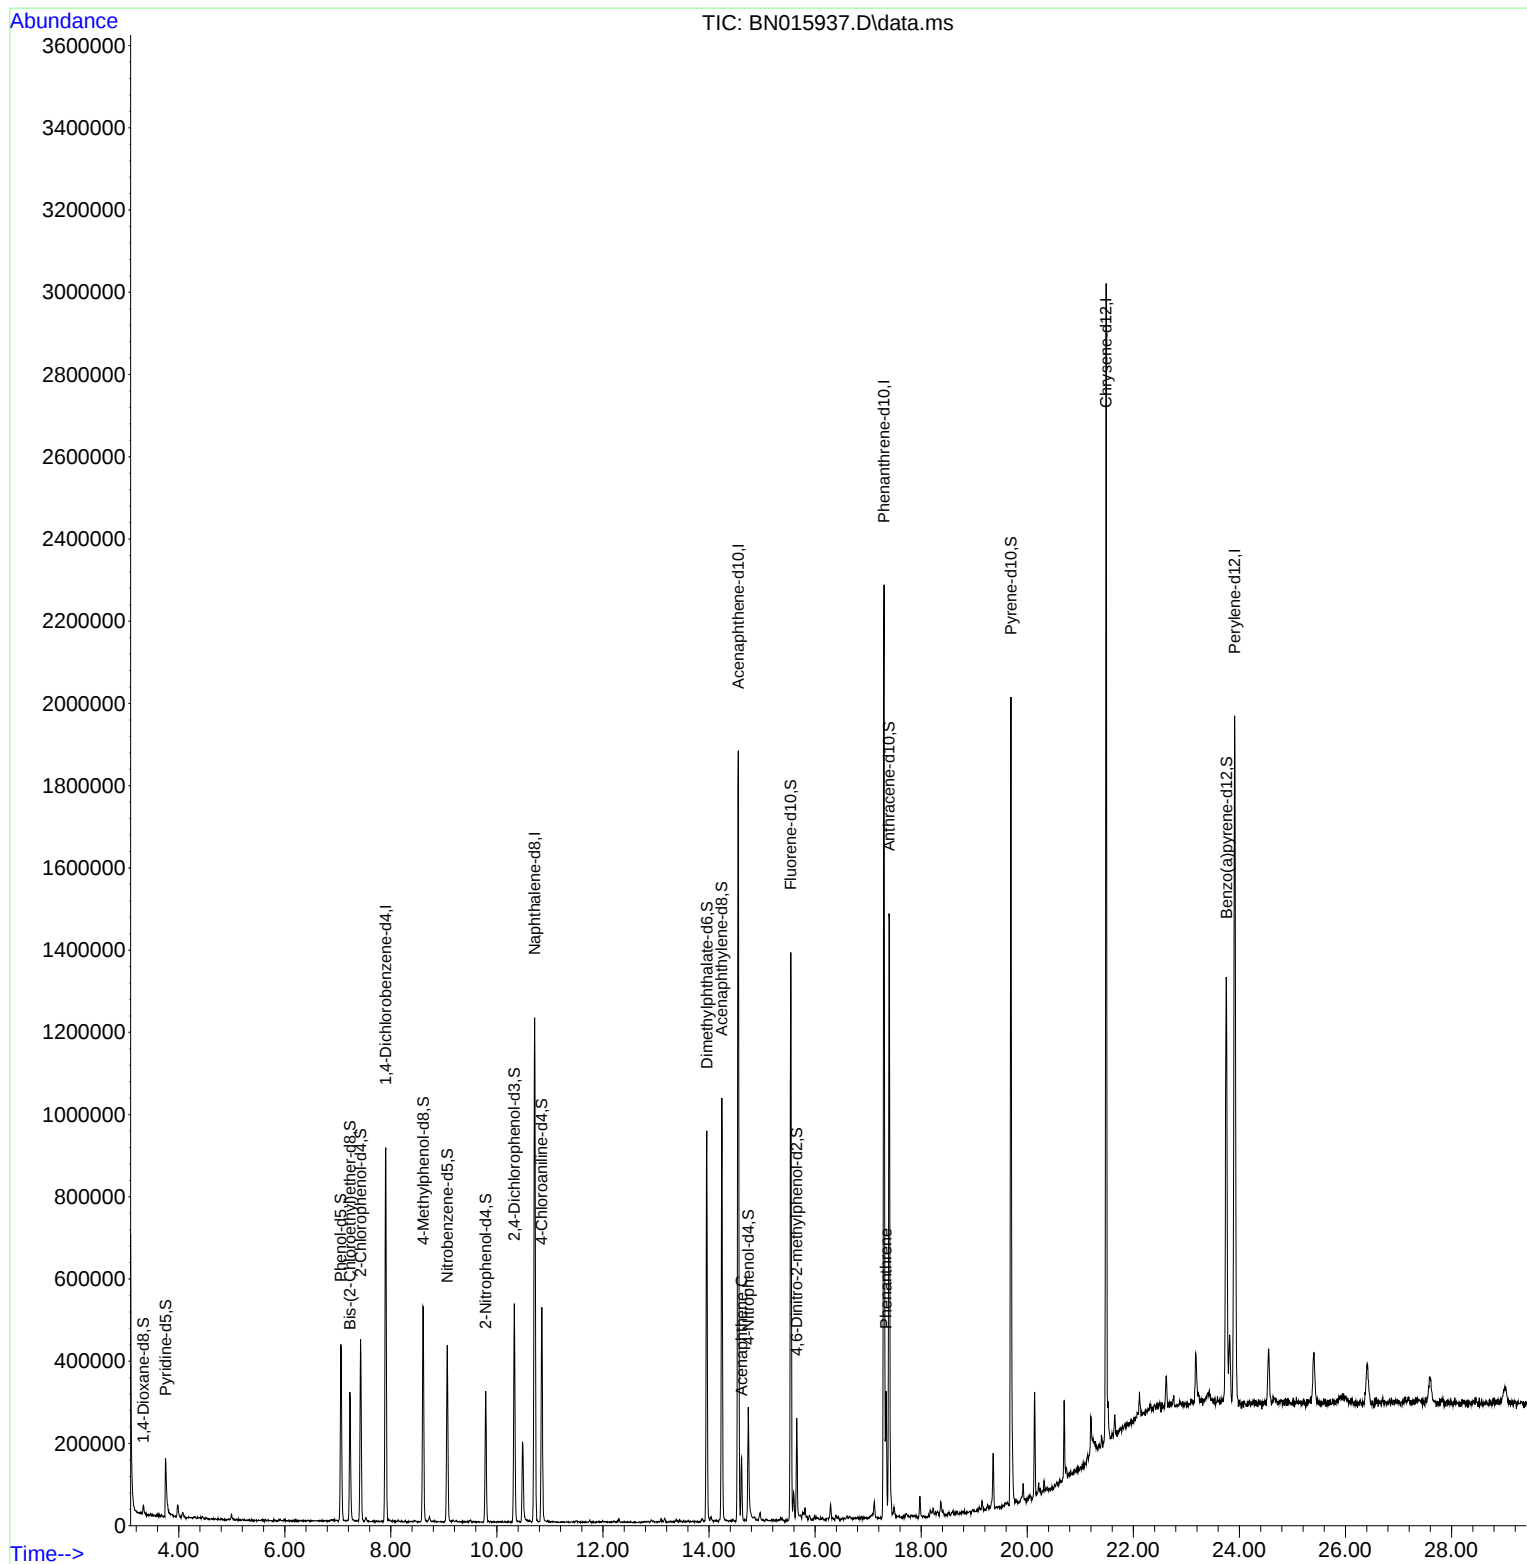


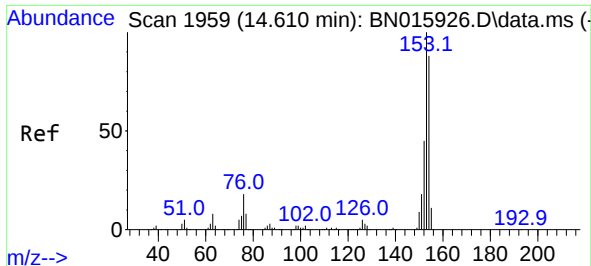

#52
Acenaphthene
Concen: 1.540 ng/ul
RT: 14.616 min Scan# 1960
Delta R.T. -0.000 min
Lab File: BN015937.D
Acq: 18 Aug 2021 15:03

Instrument :
BNA_N
ClientSampleId :
JMXD6

Tgt Ion:153	Resp:	63395
Ion Ratio	Lower	Upper
153	100	
152	49.5	38.6 57.8
154	87.5	69.3 103.9

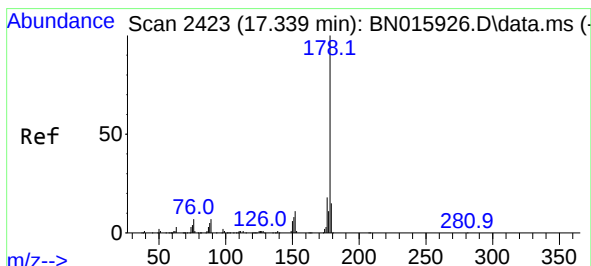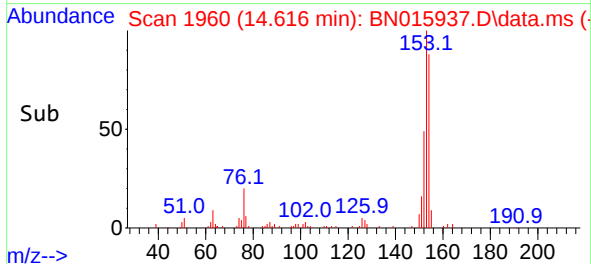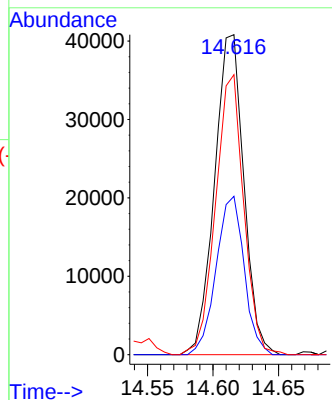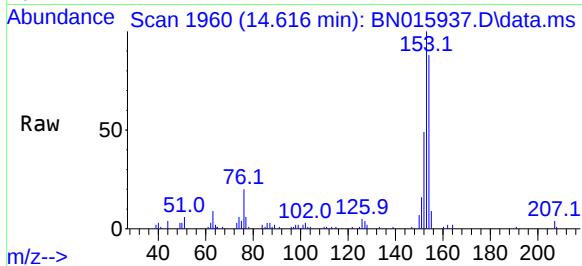

#72
Phenanthrene
Concen: 2.425 ng/ul
RT: 17.339 min Scan# 2423
Delta R.T. -0.000 min
Lab File: BN015937.D
Acq: 18 Aug 2021 15:03

Tgt Ion:178	Resp:	174601
Ion Ratio	Lower	Upper
178	100	
179	15.4	12.5 18.7
176	18.8	14.6 21.8

