

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015938.D
 Acq On : 18 Aug 2021 15:40
 Operator : CG/JU
 Sample : M3362-02MS
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JMXD6MS

Quant Time: Aug 18 17:19:42 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 17 09:43:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	172053	20.000	ng/u1	0.00
20) Naphthalene-d8	10.710	136	716938	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.551	164	470690	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.298	188	963985	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	940329	20.000	ng/u1	0.00
88) Perylene-d12	23.916	264	914022	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	14524	3.288	ng/uL	0.00
4) Pyridine-d5	3.746	84	185087	14.993	ng/u1	0.00
7) Phenol-d5	7.058	99	342725	22.022	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	210698	21.988	ng/u1	0.00
11) 2-Chlorophenol-d4	7.428	132	265851	24.006	ng/u1	0.00
15) 4-Methylphenol-d8	8.611	113	279303	23.074	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	129757	24.590	ng/u1	0.00
24) 2-Nitrophenol-d4	9.793	143	136508	27.641	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	274141	25.652	ng/u1	0.00
31) 4-Chloroaniline-d4	10.846	131	344134	21.155	ng/u1	0.00
46) Dimethylphthalate-d6	13.957	166	917434	26.596	ng/u1	0.00
49) Acenaphthylene-d8	14.240	160	1062823	24.602	ng/u1	0.00
54) 4-Nitrophenol-d4	14.740	143	139953	22.939	ng/u1	0.00
60) Fluorene-d10	15.540	176	763344	25.369	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	127613	24.788	ng/u1	0.00
73) Anthracene-d10	17.398	188	1223407	27.077	ng/u1	0.00
81) Pyrene-d10	19.692	212	1362792	26.907	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.757	264	1232915	24.948	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.370	88	53787	11.846	ng/uL	92
5) Pyridine	3.764	79	296627	23.307	ng/u1	97
6) Benzaldehyde	7.034	77	278913	34.831	ng/u1	97
8) Phenol	7.087	94	500587	31.552	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.322	93	381808	30.718	ng/u1	99
12) 2-Chlorophenol	7.464	128	375377	32.977	ng/u1	96
13) 2-Methylphenol	8.346	108	367852	31.652	ng/u1	97
14) 2,2'-oxybis(1-Chloropr...	8.440	45	467495	29.452	ng/u1	98
16) Acetophenone	8.728	105	618106	31.643	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.710	70	319291	33.472	ng/u1	98
18) 4-Methylphenol	8.675	108	398100	32.006	ng/u1	99
19) Hexachloroethane	8.987	117	160645	31.078	ng/u1	88
22) Nitrobenzene	9.105	77	477707	32.016	ng/u1	97
23) Isophorone	9.628	82	858959	33.090	ng/u1	98
25) 2-Nitrophenol	9.822	139	207017	38.439	ng/u1	99
26) 2,4-Dimethylphenol	9.881	107	446249	31.022	ng/u1	97
27) Bis(2-Chloroethoxy)met...	10.122	93	512066	32.116	ng/u1	97
29) 2,4-Dichlorophenol	10.357	162	363478	34.497	ng/u1	97
30) Naphthalene	10.763	128	1240639	32.310	ng/u1	98
32) 4-Chloroaniline	10.869	127	462997	28.829	ng/u1	98
33) Hexachlorobutadiene	11.052	225	262050	32.368	ng/u1	96
34) Caprolactam	11.628	113	113259	34.307	ng/u1	98
35) 4-Chloro-3-methylphenol	11.999	107	446067	35.741	ng/u1	98
36) 2-Methylnaphthalene	12.375	142	887037	33.220	ng/u1	95


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015938.D
 Acq On : 18 Aug 2021 15:40
 Operator : CG/JU
 Sample : M3362-02MS
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JMXD6MS

Quant Time: Aug 18 17:19:42 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 17 09:43:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.593	142	847856	31.901	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.746	216	486591	31.955	ng/ul	96
40) Hexachlorocyclopentadiene	12.722	237	245733	24.892	ng/ul	97
41) 2,4,6-Trichlorophenol	12.981	196	315117	37.847	ng/ul	95
42) 2,4,5-Trichlorophenol	13.051	196	335628	36.922	ng/ul	98
43) 1,1'-Biphenyl	13.387	154	1144864	31.455	ng/ul	98
44) 2-Chloronaphthalene	13.422	162	887878	31.593	ng/ul	99
45) 2-Nitroaniline	13.628	65	302111	37.937	ng/ul	98
47) Dimethylphthalate	14.004	163	1177248	34.427	ng/ul	99
48) 2,6-Dinitrotoluene	14.122	165	232575	37.556	ng/ul	98
50) Acenaphthylene	14.269	152	1326413	32.299	ng/ul	98
51) 3-Nitroaniline	14.451	138	227497	34.167	ng/ul	96
52) Acenaphthene	14.616	153	1048505	35.299	ng/ul	97
53) 2,4-Dinitrophenol	14.651	184	108922	31.655	ng/ul	95
55) 4-Nitrophenol	14.757	109	205058	34.348	ng/ul	95
56) Dibenzofuran	14.945	168	1359293	33.100	ng/ul	97
57) 2,4-Dinitrotoluene	14.910	165	345990	38.790	ng/ul	93
58) 2,3,4,6-Tetrachlorophenol	15.175	232	292029	38.824	ng/ul	98
59) Diethylphthalate	15.369	149	1214574	35.521	ng/ul	99
61) Fluorene	15.598	166	1155075	34.468	ng/ul	93
62) 4-Chlorophenyl-phenyle...	15.592	204	584285	33.436	ng/ul	98
63) 4-Nitroaniline	15.610	138	256167	40.153	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.675	198	176111	34.394	ng/ul	98
67) N-Nitrosodiphenylamine	15.804	169	992983	35.291	ng/ul	98
68) 4-Bromophenyl-phenylether	16.487	248	374783	36.230	ng/ul	97
69) Hexachlorobenzene	16.604	284	418874	34.651	ng/ul	95
70) Atrazine	16.757	200	381505	37.382	ng/ul	95
71) Pentachlorophenol	16.945	266	226771	33.439	ng/ul	96
72) Phenanthrene	17.339	178	2084866	39.784	ng/ul	99
74) Anthracene	17.434	178	1895069	35.420	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.346	216	488418	32.166	ng/ul	97
76) Pentachlorobenzene	14.869	250	498043	33.697	ng/ul	93
77) Carbazole	17.704	167	1634117	34.739	ng/ul	97
78) Di-n-butylphthalate	18.269	149	2108220	39.417	ng/ul	99
80) Fluoranthene	19.357	202	2288613	37.347	ng/ul	99
82) Pyrene	19.722	202	2315249	36.301	ng/ul	96
83) Butylbenzylphthalate	20.622	149	895756	41.765	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.404	252	599085	31.112	ng/ul	96
85) Benzo(a)anthracene	21.475	228	2168683	35.845	ng/ul	95
86) Bis(2-ethylhexyl)phtha...	21.404	149	1346831	39.595	ng/ul	98
87) Chrysene	21.527	228	2103087	35.903	ng/ul	97
89) Di-n-octyl phthalate	22.339	149	2226592	38.489	ng/ul	100
90) Benzo(b)fluoranthene	23.174	252	2205855	36.708	ng/ul	100
91) Benzo(k)fluoranthene	23.227	252	2125663	35.528	ng/ul	97
93) Benzo(a)pyrene	23.804	252	1666781	30.641	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.433	276	2272581	33.694	ng/ul	98
95) Dibenzo(a,h)anthracene	26.451	278	2040817	36.651	ng/ul	96
96) Benzo(g,h,i)perylene	27.192	276	257707	4.621	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed







#2
1,4-Dioxane
Concen: 11.846 ng/uL
RT: 3.370 min Scan# 48
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Instrument :
BNA_N
ClientSampleId :
JMXD6MS

Tgt Ion: 88 Resp: 53787




Ion	Ratio	Lower	Upper
88	100		
43	35.6	26.4	39.6
58	72.9	65.0	97.4

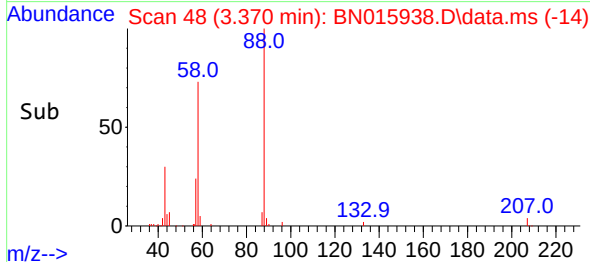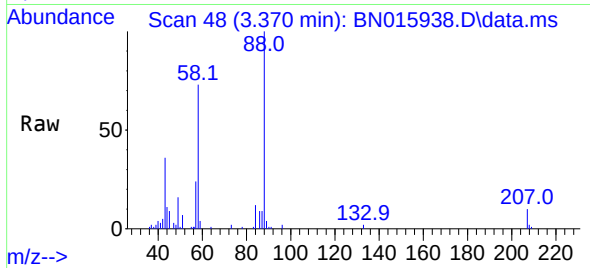


#5
Pyridine
Concen: 23.307 ng/uL
RT: 3.764 min Scan# 115
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion: 79 Resp: 296627

Ion	Ratio	Lower	Upper
79	100		
52	76.5	62.9	94.3
51	37.6	32.0	48.0


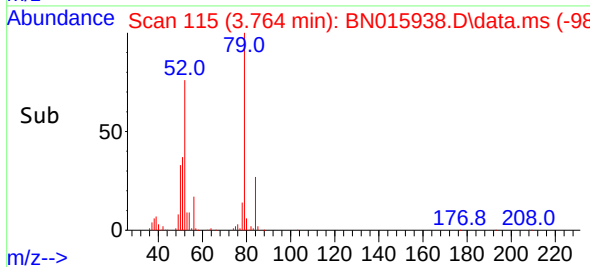

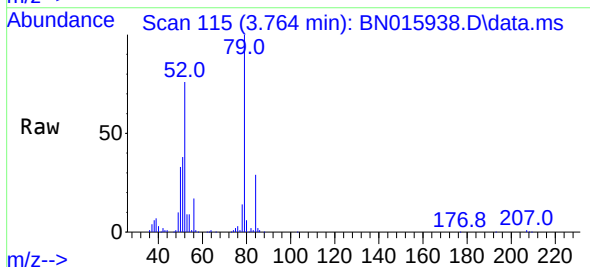




#6
Benzaldehyde
Concen: 34.831 ng/ul
RT: 7.034 min Scan# 671
Delta R.T. -0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion: 77 Resp: 278913
Ion Ratio Lower Upper
77 100
105 91.2 73.4 110.0
106 82.9 70.3 105.5

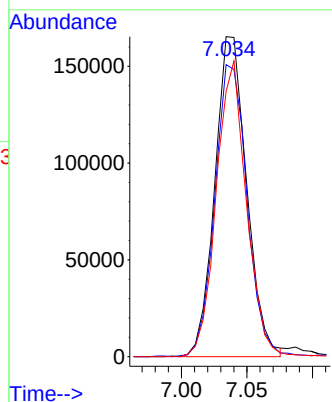

#8
Phenol
Concen: 31.552 ng/ul
RT: 7.087 min Scan# 680
Delta R.T. 0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion: 94 Resp: 500587
Ion Ratio Lower Upper
94 100
65 33.0 27.0 40.6
66 48.7 37.8 56.8









#10
Bis(2-Chloroethyl)ether
Concen: 30.718 ng/ul
RT: 7.322 min Scan# 720
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Instrument :
BNA_N
ClientSampleId :
JMXD6MS

Tgt Ion: 93 Resp: 381808




Ion	Ratio	Lower	Upper
93	100		
63	79.8	63.4	95.0
95	32.7	25.2	37.8




#12
2-Chlorophenol
Concen: 32.977 ng/ul
RT: 7.464 min Scan# 744
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:128 Resp: 375377

Ion	Ratio	Lower	Upper
128	100		
64	55.0	41.4	62.2
130	33.1	25.2	37.8



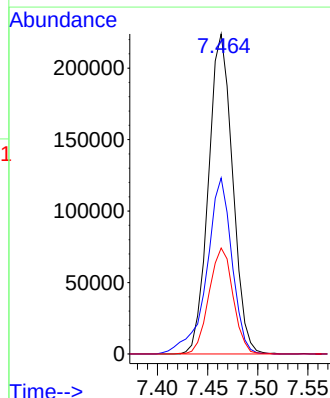





#13
2-Methylphenol
Concen: 31.652 ng/ul
RT: 8.346 min Scan# 894
Delta R.T. 0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:108 Resp: 367852
Ion Ratio Lower Upper
108 100
107 90.7 74.9 112.3

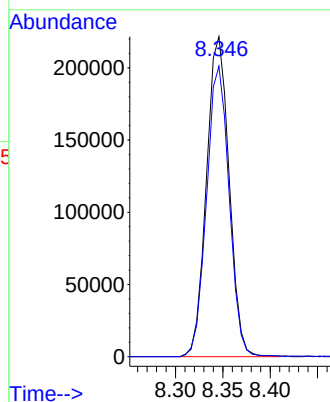

#14
2,2'-oxybis(1-Chloropropane)
Concen: 29.452 ng/ul
RT: 8.440 min Scan# 910
Delta R.T. 0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion: 45 Resp: 467495
Ion Ratio Lower Upper
45 100
77 16.9 13.2 19.8
79 12.1 8.7 13.1



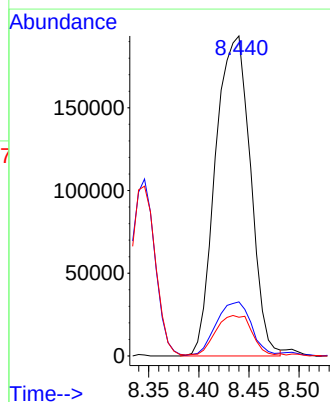





#16
Acetophenone
Concen: 31.643 ng/ul
RT: 8.728 min Scan# 959
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:105 Resp: 618106
Ion Ratio Lower Upper
105 100
77 80.9 66.3 99.5
51 28.2 23.7 35.5

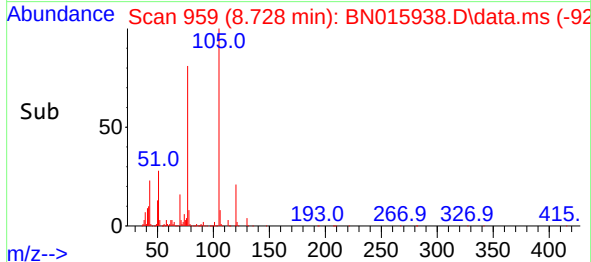

#17
N-Nitroso-di-n-propylamine
Concen: 33.472 ng/ul
RT: 8.710 min Scan# 956
Delta R.T. -0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion: 70 Resp: 319291
Ion Ratio Lower Upper
70 100
42 54.9 45.3 67.9
101 9.7 7.6 11.4
130 19.5 15.0 22.6



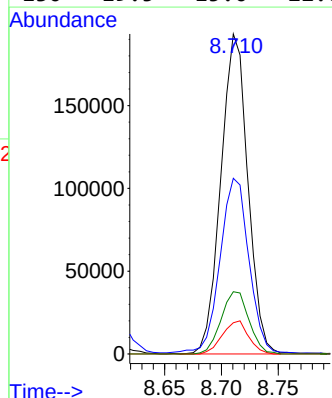





#18
4-Methylphenol
Concen: 32.006 ng/ul
RT: 8.675 min Scan# 950
Delta R.T. 0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:108 Resp: 398100
Ion Ratio Lower Upper
108 100
107 107.6 85.3 127.9

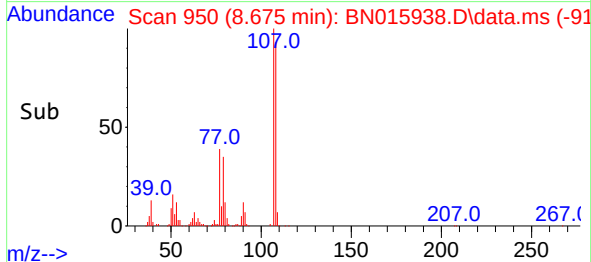

#19
Hexachloroethane
Concen: 31.078 ng/ul
RT: 8.987 min Scan# 1003
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:117 Resp: 160645
Ion Ratio Lower Upper
117 100
201 105.3 74.0 111.0
199 63.8 45.0 67.4









#22
Nitrobenzene
Concen: 32.016 ng/u1
RT: 9.105 min Scan# 1023
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion: 77 Resp: 477707
Ion Ratio Lower Upper
77 100
123 42.2 32.2 48.4
65 14.3 10.9 16.3

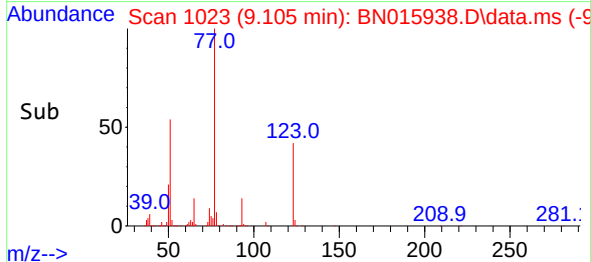

#23
Isophorone
Concen: 33.090 ng/u1
RT: 9.628 min Scan# 1112
Delta R.T. -0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion: 82 Resp: 858959
Ion Ratio Lower Upper
82 100
95 8.0 6.1 9.1
138 15.0 13.0 19.4


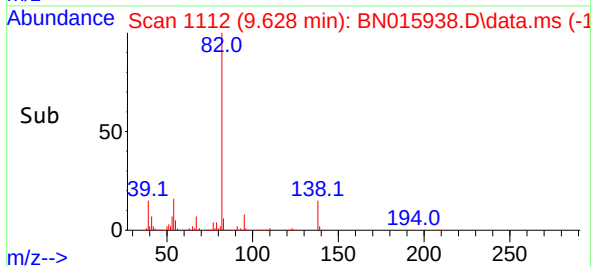

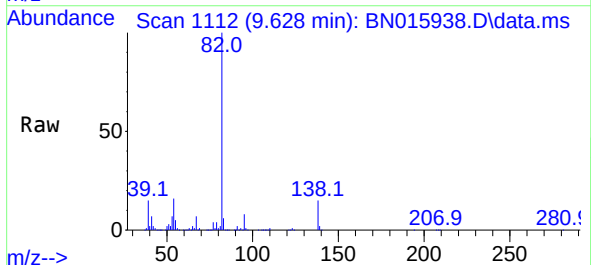


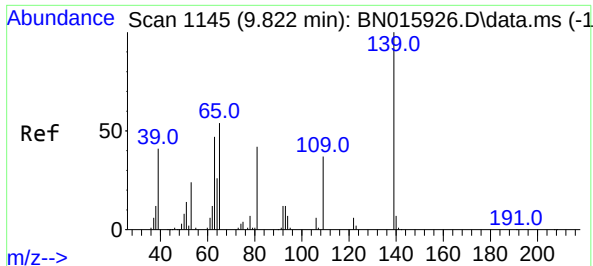

#25
2-Nitrophenol
Concen: 38.439 ng/ul
RT: 9.822 min Scan# 1145
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampled :
JMXD6MS


Tgt Ion:139 Resp: 207017
Ion Ratio Lower Upper
139 100
65 60.9 48.1 72.1
109 37.0 29.7 44.5

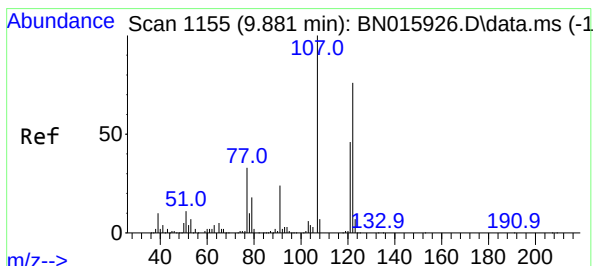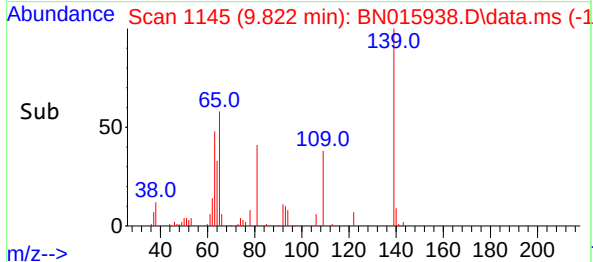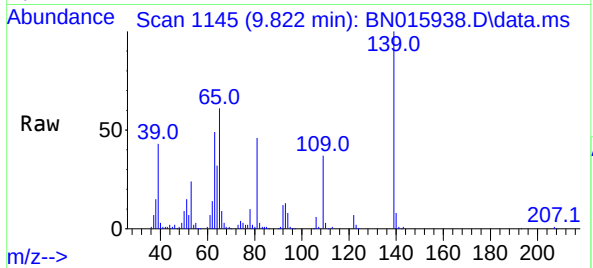

#26
2,4-Dimethylphenol
Concen: 31.022 ng/ul
RT: 9.881 min Scan# 1155
Delta R.T. 0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:107 Resp: 446249
Ion Ratio Lower Upper
107 100
121 46.5 35.3 52.9
122 72.4 59.4 89.0

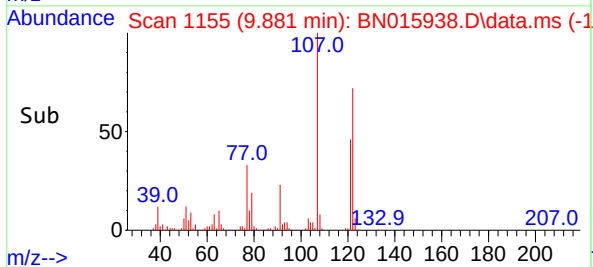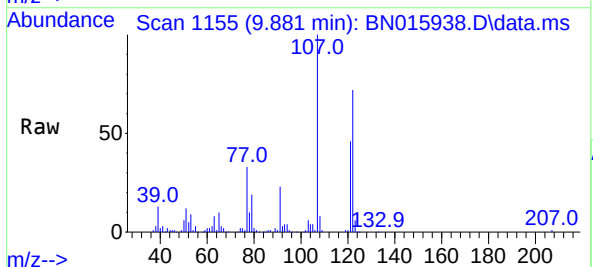







#27
 Bis(2-Chloroethoxy)methane
 Concen: 32.116 ng/ul
 RT: 10.122 min Scan# 1196
 Delta R.T. 0.000 min
 Lab File: BN015938.D
 Acq: 18 Aug 2021 15:40

Instrument :
 BNA_N
 ClientSampleId :
 JMXD6MS

Tgt Ion: 93 Resp: 512066




Ion	Ratio	Lower	Upper
93	100		
95	31.8	26.9	40.3
123	9.3	8.3	12.5

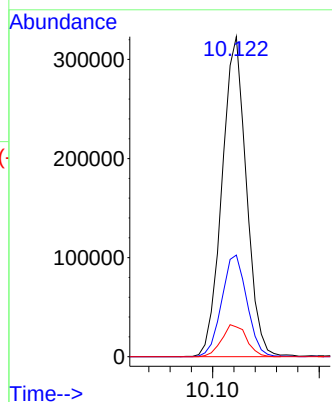


#29
 2,4-Dichlorophenol
 Concen: 34.497 ng/ul
 RT: 10.357 min Scan# 1236
 Delta R.T. 0.006 min
 Lab File: BN015938.D
 Acq: 18 Aug 2021 15:40

Tgt Ion: 162 Resp: 363478

Ion	Ratio	Lower	Upper
162	100		
164	63.6	51.9	77.9
98	39.5	34.2	51.2









#30
Naphthalene
Concen: 32.310 ng/ul
RT: 10.763 min Scan# 1305
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:128 Resp: 1240639
Ion Ratio Lower Upper
128 100
129 10.6 8.8 13.2
127 12.6 11.1 16.7

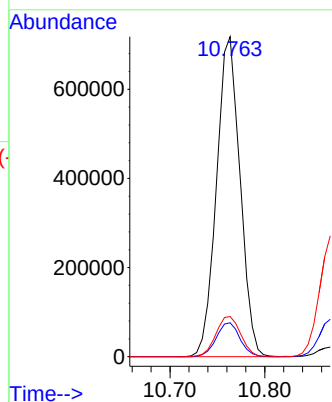

#32
4-Chloroaniline
Concen: 28.829 ng/ul
RT: 10.869 min Scan# 1323
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:127 Resp: 462997
Ion Ratio Lower Upper
127 100
129 31.0 25.6 38.4


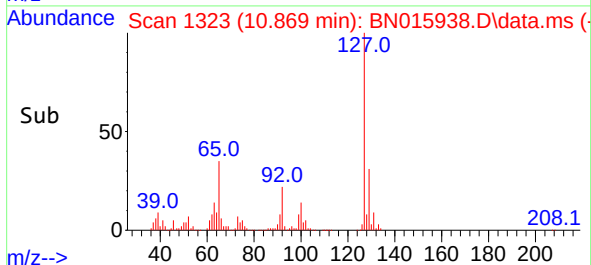

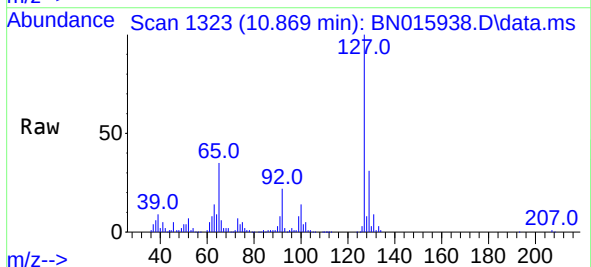


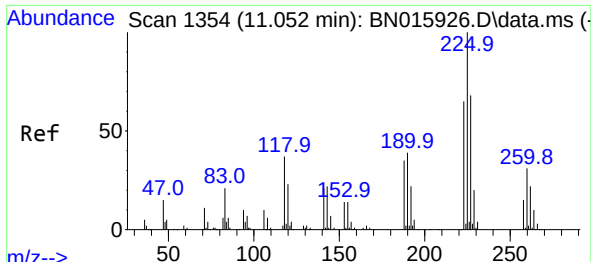

#33
Hexachlorobutadiene
Concen: 32.368 ng/ul
RT: 11.052 min Scan# 1354
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampled :
JMXD6MS


Tgt Ion:225 Resp: 262050
Ion Ratio Lower Upper
225 100
223 64.2 50.5 75.7
227 61.9 53.9 80.9



#34
Caprolactam
Concen: 34.307 ng/ul
RT: 11.628 min Scan# 1452
Delta R.T. 0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:113 Resp: 113259
Ion Ratio Lower Upper
113 100
55 158.9 130.4 195.6
56 128.5 102.2 153.4









#35
4-Chloro-3-methylphenol
Concen: 35.741 ng/ul
RT: 11.999 min Scan# 1515
Delta R.T. 0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:107 Resp: 446067
Ion Ratio Lower Upper
107 100
144 23.0 18.2 27.4
142 69.5 57.1 85.7



#36
2-Methylnaphthalene
Concen: 33.220 ng/ul
RT: 12.375 min Scan# 1579
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:142 Resp: 887037
Ion Ratio Lower Upper
142 100
141 86.7 73.4 110.0









#37
1-Methylnaphthalene
Concen: 31.901 ng/ul
RT: 12.593 min Scan# 1616
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampled :
JMXD6MS


Tgt Ion:142 Resp: 847856
Ion Ratio Lower Upper
142 100
141 93.4 74.2 111.4
116 4.0 3.4 5.0

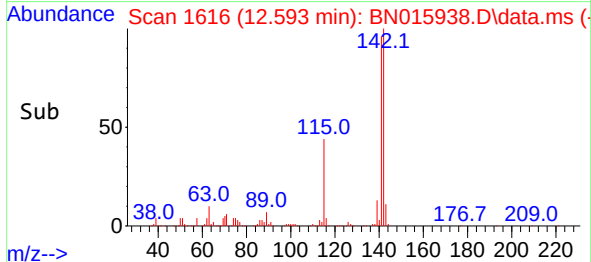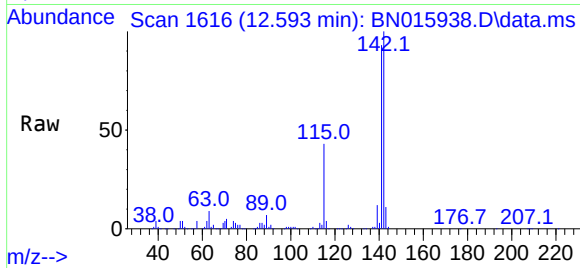

#39
1,2,4,5-Tetrachlorobenzene
Concen: 31.955 ng/ul
RT: 12.746 min Scan# 1642
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:216 Resp: 486591
Ion Ratio Lower Upper
216 100
214 74.7 62.7 94.1
179 22.2 18.6 27.8
108 16.8 15.2 22.8


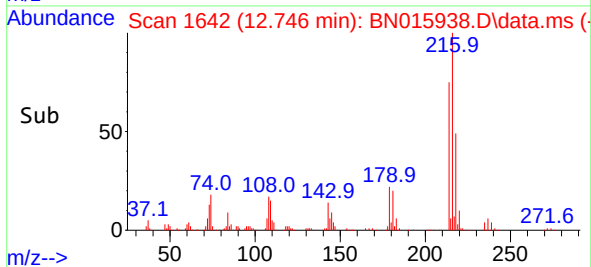

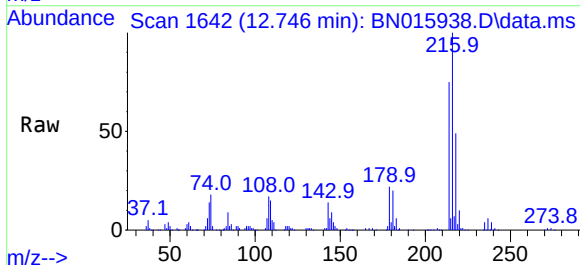




#40
Hexachlorocyclopentadiene
Concen: 24.892 ng/ul
RT: 12.722 min Scan# 1638
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:237 Resp: 245733
Ion Ratio Lower Upper
237 100
235 58.6 49.0 73.4
272 12.6 9.8 14.8

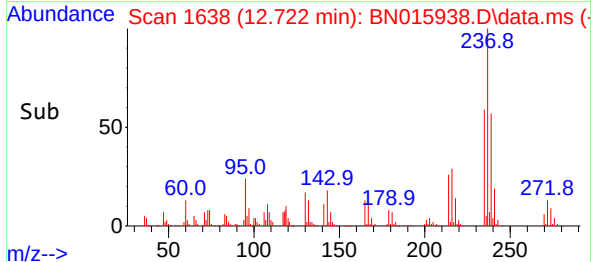

#41
2,4,6-Trichlorophenol
Concen: 37.847 ng/ul
RT: 12.981 min Scan# 1682
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:196 Resp: 315117
Ion Ratio Lower Upper
196 100
198 93.6 79.9 119.9
200 30.7 23.6 35.4









#42
2,4,5-Trichlorophenol
Concen: 36.922 ng/ul
RT: 13.051 min Scan# 1694
Delta R.T. 0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:196 Resp: 335628
Ion Ratio Lower Upper
196 100
198 97.5 76.5 114.7
200 30.6 24.6 37.0

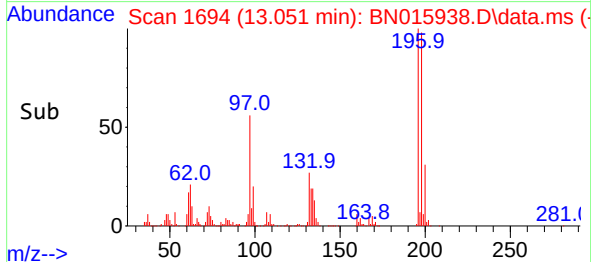

#43
1,1'-Biphenyl
Concen: 31.455 ng/ul
RT: 13.387 min Scan# 1751
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:154 Resp: 1144864
Ion Ratio Lower Upper
154 100
153 41.6 32.1 48.1
76 12.7 11.0 16.6









#44
2-Chloronaphthalene
Concen: 31.593 ng/ul
RT: 13.422 min Scan# 1757
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Instrument :
BNA_N
ClientSampleId :
JMXD6MS

Tgt Ion:162 Resp: 887878




Ion	Ratio	Lower	Upper
162	100		
164	33.3	26.6	40.0
127	43.9	36.3	54.5

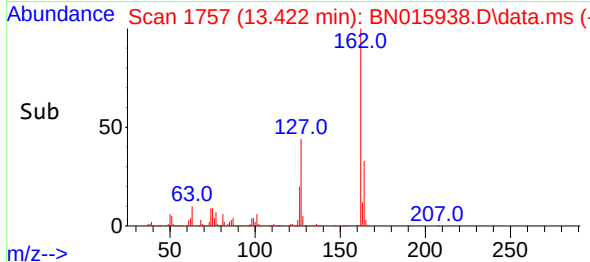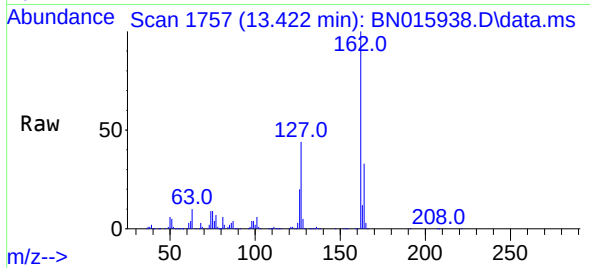


#45
2-Nitroaniline
Concen: 37.937 ng/ul
RT: 13.628 min Scan# 1792
Delta R.T. 0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion: 65 Resp: 302111

Ion	Ratio	Lower	Upper
65	100		
92	66.5	54.5	81.7
138	92.4	75.4	113.0


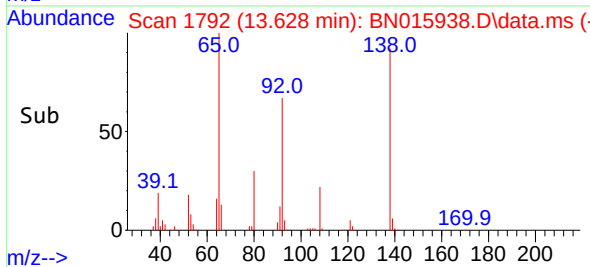

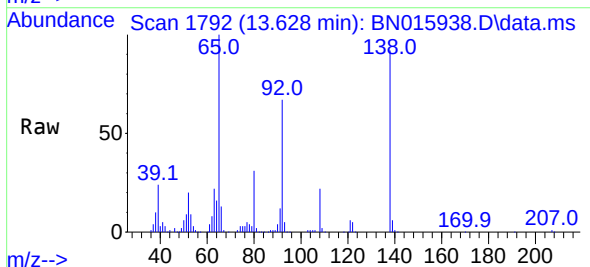


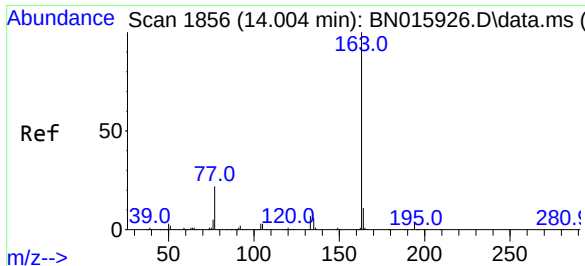

#47
Dimethylphthalate
Concen: 34.427 ng/ul
RT: 14.004 min Scan# 1856
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:163 Resp: 1177248
Ion Ratio Lower Upper
163 100
194 4.1 3.3 4.9
164 10.2 8.6 12.8

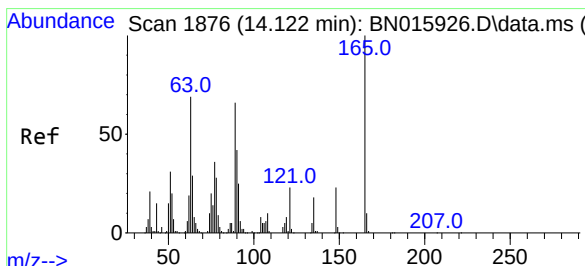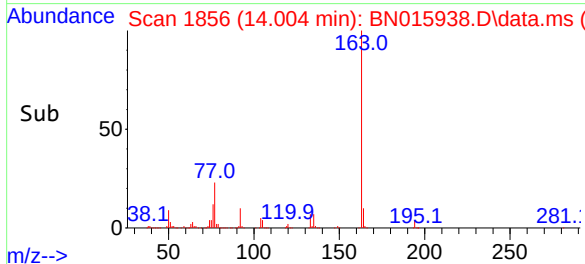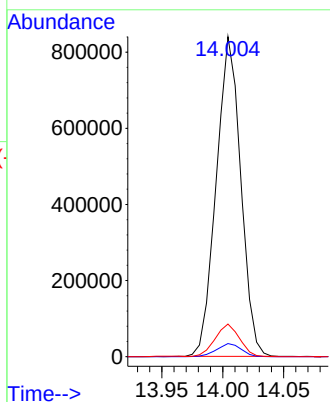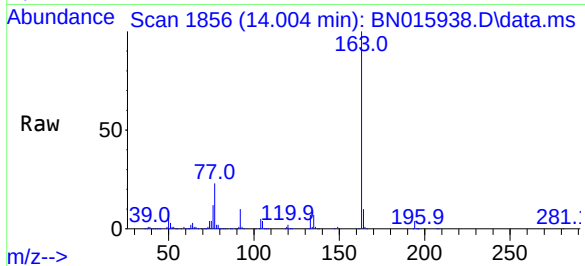

#48
2,6-Dinitrotoluene
Concen: 37.556 ng/ul
RT: 14.122 min Scan# 1876
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:165 Resp: 232575
Ion Ratio Lower Upper
165 100
89 71.8 59.5 89.3
121 24.9 20.0 30.0

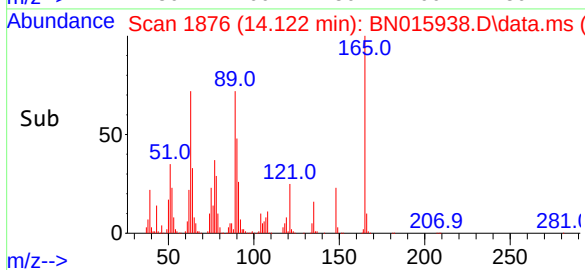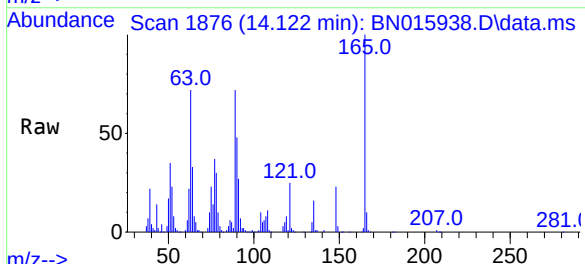







#50
Acenaphthylene
Concen: 32.299 ng/ul
RT: 14.269 min Scan# 1901
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Instrument :
BNA_N
ClientSampleId :
JMXD6MS

Tgt Ion:152 Resp: 1326413




Ion	Ratio	Lower	Upper
152	100		
151	21.0	16.2	24.2
153	13.4	10.3	15.5




#51
3-Nitroaniline
Concen: 34.167 ng/ul
RT: 14.451 min Scan# 1932
Delta R.T. 0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:138 Resp: 227497

Ion	Ratio	Lower	Upper
138	100		
108	12.8	10.3	15.5
92	134.7	103.9	155.9









#52
Acenaphthene
Concen: 35.299 ng/ul
RT: 14.616 min Scan# 1960
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:153 Resp: 1048505
Ion Ratio Lower Upper
153 100
152 44.8 38.6 57.8
154 88.2 69.3 103.9

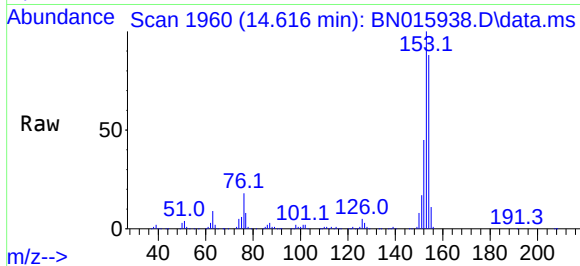

#53
2,4-Dinitrophenol
Concen: 31.655 ng/ul
RT: 14.651 min Scan# 1966
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:184 Resp: 108922
Ion Ratio Lower Upper
184 100
63 77.1 64.8 97.2
154 70.0 59.7 89.5



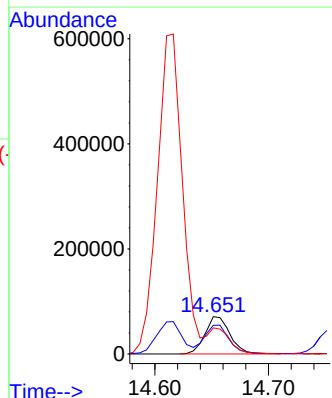
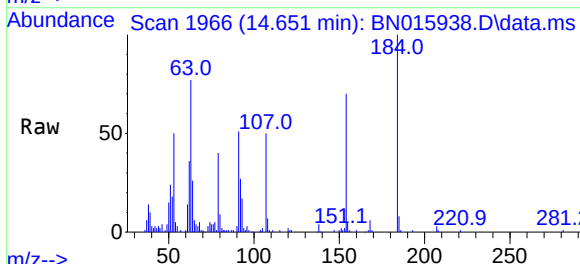




#55
4-Nitrophenol
Concen: 34.348 ng/ul
RT: 14.757 min Scan# 1984
Delta R.T. 0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:109 Resp: 205058
Ion Ratio Lower Upper
109 100
139 104.1 84.7 127.1
65 122.0 105.0 157.6



#56
Dibenzofuran
Concen: 33.100 ng/ul
RT: 14.945 min Scan# 2016
Delta R.T. -0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:168 Resp: 1359293
Ion Ratio Lower Upper
168 100
139 41.8 31.8 47.6


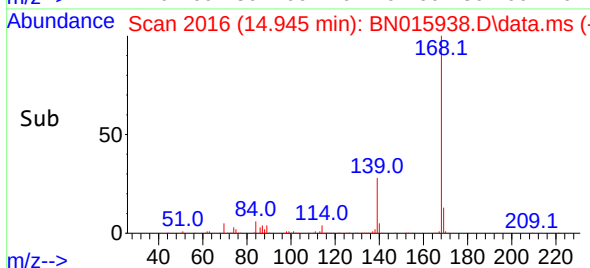






#57
2,4-Dinitrotoluene
Concen: 38.790 ng/ul
RT: 14.910 min Scan# 2010
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:165 Resp: 345990
Ion Ratio Lower Upper
165 100
63 48.2 42.8 64.2
182 2.8 2.2 3.4

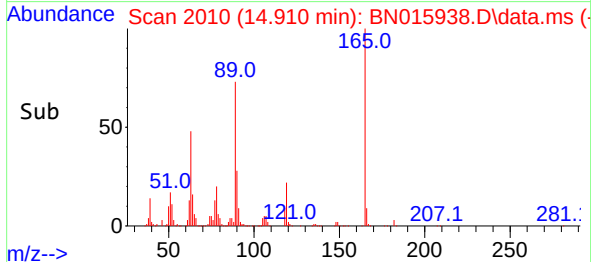

#58
2,3,4,6-Tetrachlorophenol
Concen: 38.824 ng/ul
RT: 15.175 min Scan# 2055
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:232 Resp: 292029
Ion Ratio Lower Upper
232 100
131 47.1 37.5 56.3
130 2.7 2.2 3.4
166 30.4 26.2 39.2


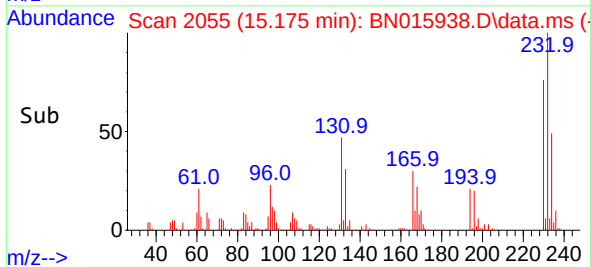

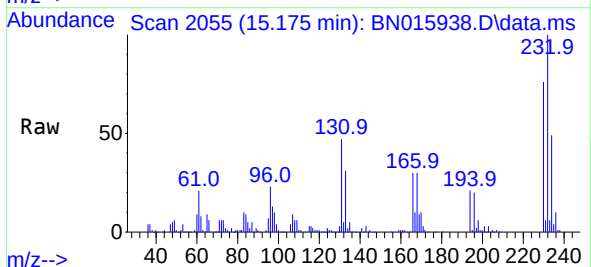




#59
Diethylphthalate
Concen: 35.521 ng/ul
RT: 15.369 min Scan# 2088
Delta R.T. -0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:149 Resp: 1214574
Ion Ratio Lower Upper
149 100
177 21.2 17.2 25.8
150 13.1 10.2 15.2

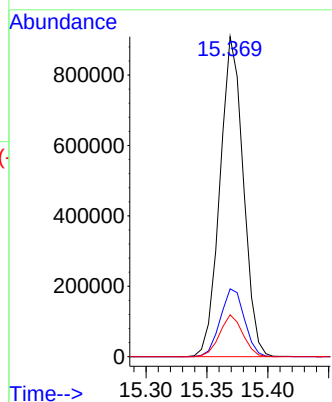

#61
Fluorene
Concen: 34.468 ng/ul
RT: 15.598 min Scan# 2127
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:166 Resp: 1155075
Ion Ratio Lower Upper
166 100
165 106.0 78.4 117.6
167 13.8 10.8 16.2









#62
4-Chlorophenyl-phenylether
Concen: 33.436 ng/ul
RT: 15.592 min Scan# 2126
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampled :
JMXD6MS


Tgt Ion:204 Resp: 584285
Ion Ratio Lower Upper
204 100
206 32.8 26.1 39.1
141 64.0 53.4 80.0

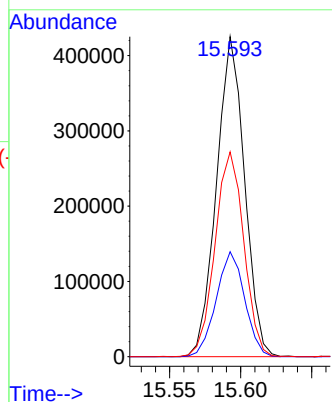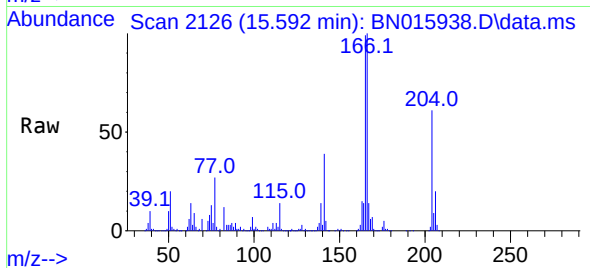

#63
4-Nitroaniline
Concen: 40.153 ng/ul
RT: 15.610 min Scan# 2129
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:138 Resp: 256167
Ion Ratio Lower Upper
138 100
92 59.0 48.6 72.8
108 102.9 80.7 121.1


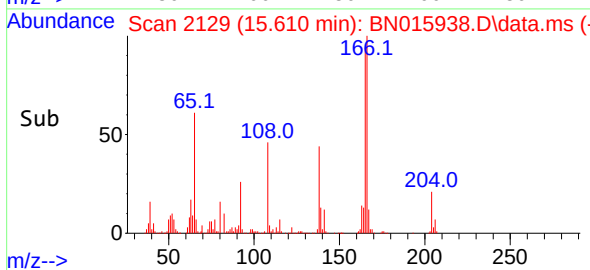
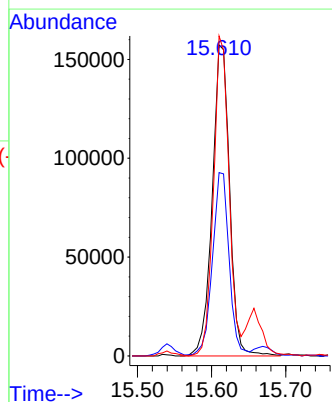





#66
 4,6-Dinitro-2-methylphenol
 Concen: 34.394 ng/ul
 RT: 15.675 min Scan# 2140
 Delta R.T. 0.006 min
 Lab File: BN015938.D
 Acq: 18 Aug 2021 15:40




Instrument :
 BNA_N
 ClientSampleID :
 JMXD6MS


Tgt Ion:198 Resp: 176111
 Ion Ratio Lower Upper
 198 100
 182 4.0 3.0 4.4
 77 28.0 23.4 35.0



#67
 N-Nitrosodiphenylamine
 Concen: 35.291 ng/ul
 RT: 15.804 min Scan# 2162
 Delta R.T. 0.000 min
 Lab File: BN015938.D
 Acq: 18 Aug 2021 15:40

Tgt Ion:169 Resp: 992983
 Ion Ratio Lower Upper
 169 100
 168 65.0 53.5 80.3
 167 35.4 27.9 41.9


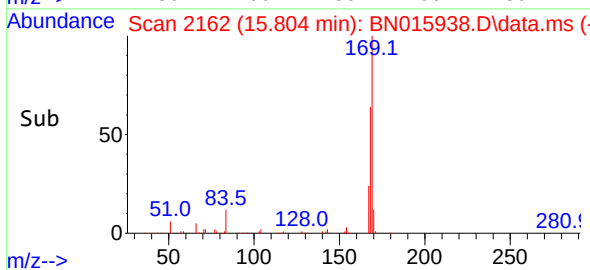






#68
4-Bromophenyl-phenylether
Concen: 36.230 ng/ul
RT: 16.487 min Scan# 2278
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:248 Resp: 374783
Ion Ratio Lower Upper
248 100
250 96.4 81.1 121.7
141 80.7 64.7 97.1

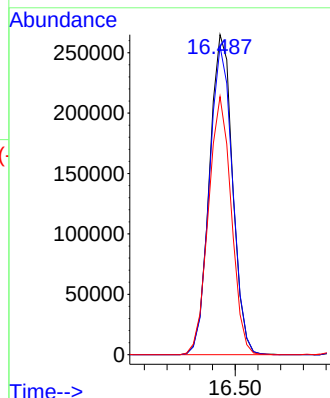

#69
Hexachlorobenzene
Concen: 34.651 ng/ul
RT: 16.604 min Scan# 2298
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:284 Resp: 418874
Ion Ratio Lower Upper
284 100
142 33.0 30.3 45.5
249 31.9 26.3 39.5


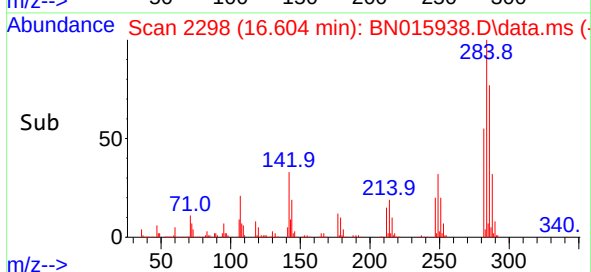
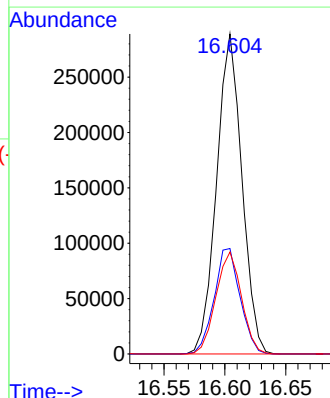





#70
Atrazine
Concen: 37.382 ng/ul
RT: 16.757 min Scan# 2324
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:200 Resp: 381505
Ion Ratio Lower Upper
200 100
173 25.3 22.2 33.2
215 50.4 37.6 56.4

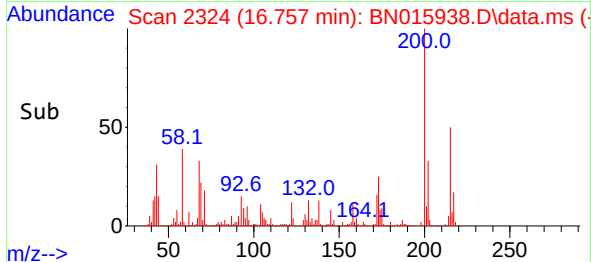

#71
Pentachlorophenol
Concen: 33.439 ng/ul
RT: 16.945 min Scan# 2356
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:266 Resp: 226771
Ion Ratio Lower Upper
266 100
264 62.1 53.8 80.6
268 64.2 52.7 79.1


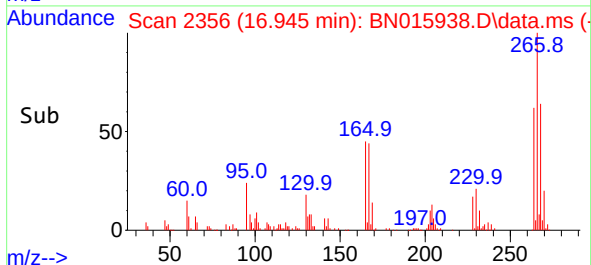
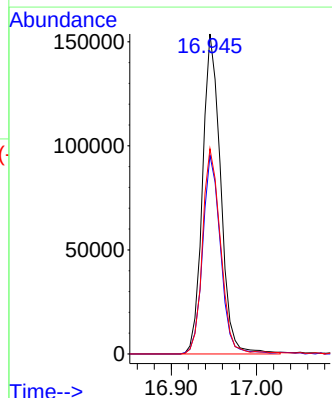
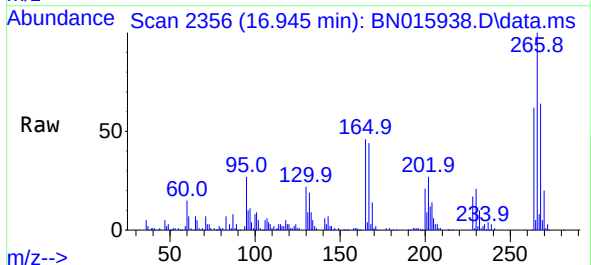




#72
Phenanthrene
Concen: 39.784 ng/u1
RT: 17.339 min Scan# 2423
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:178 Resp: 2084866
Ion Ratio Lower Upper
178 100
179 15.3 12.5 18.7
176 18.4 14.6 21.8

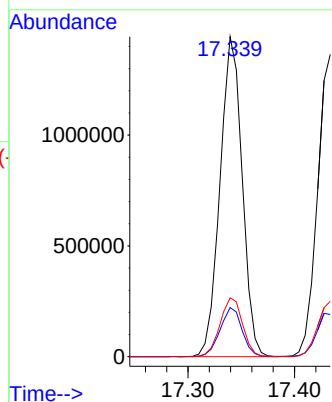

#74
Anthracene
Concen: 35.420 ng/u1
RT: 17.434 min Scan# 2439
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:178 Resp: 1895069
Ion Ratio Lower Upper
178 100
179 14.0 11.6 17.4
176 18.3 14.4 21.6


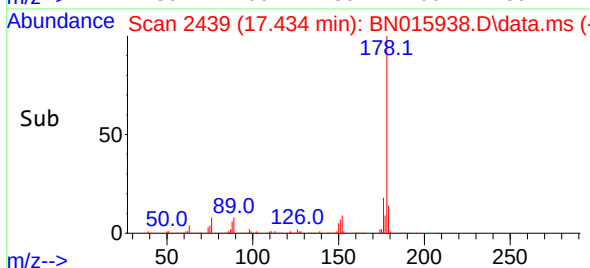






#75
1,2,3,4-Tetrachlorobenzene
Concen: 32.166 ng/uL
RT: 13.346 min Scan# 1744
Delta R.T. -0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:216 Resp: 488418
Ion Ratio Lower Upper
216 100
214 78.0 64.6 97.0
218 45.8 38.7 58.1



#76
Pentachlorobenzene
Concen: 33.697 ng/uL
RT: 14.869 min Scan# 2003
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:250 Resp: 498043
Ion Ratio Lower Upper
250 100
248 61.5 51.9 77.9
252 61.2 54.7 82.1









#77
 Carbazole
 Concen: 34.739 ng/ul
 RT: 17.704 min Scan# 2485
 Delta R.T. 0.006 min
 Lab File: BN015938.D
 Acq: 18 Aug 2021 15:40

Instrument :
 BNA_N
 ClientSampleId :
 JMXD6MS

Tgt Ion:167 Resp: 1634117




Ion	Ratio	Lower	Upper
167	100		
166	22.6	17.1	25.7
139	13.5	11.6	17.4




#78
 Di-n-butylphthalate
 Concen: 39.417 ng/ul
 RT: 18.269 min Scan# 2581
 Delta R.T. 0.000 min
 Lab File: BN015938.D
 Acq: 18 Aug 2021 15:40

Tgt Ion:149 Resp: 2108220

Ion	Ratio	Lower	Upper
149	100		
150	8.7	7.5	11.3
104	5.9	5.0	7.4









#80
Fluoranthene
Concen: 37.347 ng/ul
RT: 19.357 min Scan# 2766
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:202 Resp: 2288613
Ion Ratio Lower Upper
202 100
101 9.9 8.0 12.0
100 7.6 6.7 10.1



#82
Pyrene
Concen: 36.301 ng/ul
RT: 19.722 min Scan# 2828
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:202 Resp: 2315249
Ion Ratio Lower Upper
202 100
101 10.8 10.1 15.1
100 10.1 9.2 13.8



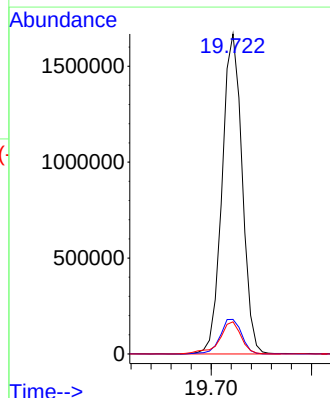





#83
Butylbenzylphthalate
Concen: 41.765 ng/ul
RT: 20.622 min Scan# 2981
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:149 Resp: 895756
Ion Ratio Lower Upper
149 100
91 78.5 65.2 97.8
206 21.2 17.1 25.7



#84
3,3'-Dichlorobenzidine
Concen: 31.112 ng/ul
RT: 21.404 min Scan# 3114
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:252 Resp: 599085
Ion Ratio Lower Upper
252 100
254 61.6 52.0 78.0
126 11.0 8.5 12.7









#85
Benzo(a)anthracene
Concen: 35.845 ng/ul
RT: 21.475 min Scan# 3126
Delta R.T. 0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:228 Resp: 2168683
Ion Ratio Lower Upper
228 100
229 20.9 14.5 21.7
226 27.7 20.9 31.3

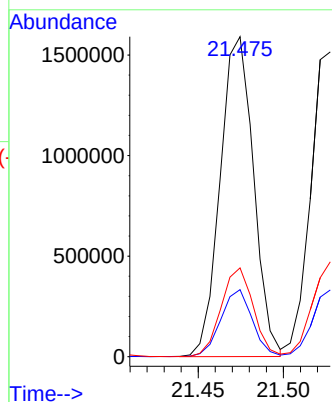

#86
Bis(2-ethylhexyl)phthalate
Concen: 39.595 ng/ul
RT: 21.404 min Scan# 3114
Delta R.T. 0.000 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:149 Resp: 1346831
Ion Ratio Lower Upper
149 100
167 26.7 20.6 30.8
279 4.7 3.4 5.2

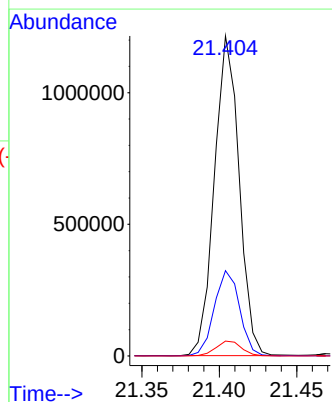







#87
Chrysene
Concen: 35.903 ng/ul
RT: 21.527 min Scan# 3135
Delta R.T. 0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Instrument :
BNA_N
ClientSampleId :
JMXD6MS




Tgt Ion:228 Resp: 2103087


Ion	Ratio	Lower	Upper
228	100		
226	31.2	24.2	36.2
229	21.9	15.9	23.9



#89
Di-n-octyl phthalate
Concen: 38.489 ng/ul
RT: 22.339 min Scan# 3273
Delta R.T. 0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:149 Resp: 2226592


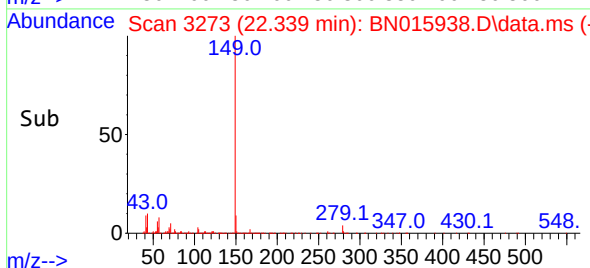
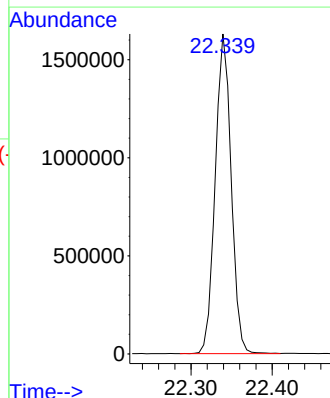





#90
Benzo(b)fluoranthene
Concen: 36.708 ng/ul
RT: 23.174 min Scan# 3415
Delta R.T. 0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:252 Resp: 2205855
Ion Ratio Lower Upper
252 100
253 21.1 16.6 25.0
125 8.9 7.1 10.7



#91
Benzo(k)fluoranthene
Concen: 35.528 ng/ul
RT: 23.227 min Scan# 3424
Delta R.T. 0.012 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40

Tgt Ion:252 Resp: 2125663
Ion Ratio Lower Upper
252 100
253 20.9 17.7 26.5
125 7.9 7.0 10.6









#93
Benzo(a)pyrene
Concen: 30.641 ng/ul
RT: 23.804 min Scan# 3522
Delta R.T. 0.006 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40




Instrument :
BNA_N
ClientSampleId :
JMXD6MS


Tgt Ion:252 Resp: 1666781
Ion Ratio Lower Upper
252 100
253 23.4 18.0 27.0
125 9.9 7.2 10.8



#94
Indeno(1,2,3-cd)pyrene
Concen: 33.694 ng/ul
RT: 26.433 min Scan# 3969
Delta R.T. 0.012 min
Lab File: BN015938.D
Acq: 18 Aug 2021 15:40


Tgt Ion:276 Resp: 2272581
Ion Ratio Lower Upper
276 100
138 20.1 15.9 23.9
277 26.2 19.5 29.3








#95
 Dibenzo(a,h)anthracene
 Concen: 36.651 ng/ul
 RT: 26.451 min Scan# 3972
 Delta R.T. 0.006 min
 Lab File: BN015938.D
 Acq: 18 Aug 2021 15:40

Instrument :
 BNA_N
 ClientSampleId :
 JMXD6MS



Tgt Ion:278 Resp: 2040817

Ion	Ratio	Lower	Upper
278	100		
139	12.5	11.0	16.6
279	22.7	19.9	29.9



#96
 Benzo(g,h,i)perylene
 Concen: 4.621 ng/ul
 RT: 27.192 min Scan# 4098
 Delta R.T. 0.000 min
 Lab File: BN015938.D
 Acq: 18 Aug 2021 15:40

Tgt Ion:276 Resp: 257707

Ion	Ratio	Lower	Upper
276	100		
138	16.8	13.4	20.0
277	24.2	18.5	27.7

