

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015949.D
 Acq On : 18 Aug 2021 22:24
 Operator : CG/JU
 Sample : M3399-03
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKA5

Quant Time: Aug 19 01:05:00 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 17 09:43:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	257931	20.000	ng/u1	0.00
20) Naphthalene-d8	10.710	136	1105566	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.551	164	703014	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.292	188	1431688	20.000	ng/u1	0.00
79) Chrysene-d12	21.480	240	1346722	20.000	ng/u1	0.00
88) Perylene-d12	23.904	264	1327571	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	29964	4.525	ng/uL	0.00
4) Pyridine-d5	3.752	84	104006	5.620	ng/u1	0.00
7) Phenol-d5	7.064	99	156068	6.689	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	402477	28.018	ng/u1	0.00
11) 2-Chlorophenol-d4	7.428	132	411804	24.805	ng/u1	0.00
15) 4-Methylphenol-d8	8.605	113	289711	15.965	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	257661	31.665	ng/u1	0.00
24) 2-Nitrophenol-d4	9.787	143	262256	34.437	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	493467	29.944	ng/u1	0.00
31) 4-Chloroaniline-d4	10.846	131	556071	22.167	ng/u1	0.00
46) Dimethylphthalate-d6	13.957	166	1879945	36.488	ng/u1	0.00
49) Acenaphthylene-d8	14.240	160	2185481	33.871	ng/u1	0.00
54) 4-Nitrophenol-d4	14.740	143	55940	6.139	ng/u1	0.00
60) Fluorene-d10	15.540	176	1566344	34.853	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	224541	29.367	ng/u1	0.00
73) Anthracene-d10	17.398	188	2539332	37.841	ng/u1	0.00
81) Pyrene-d10	19.692	212	2869009	39.552	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.745	264	2748975	38.297	ng/u1	0.00


Target Compounds					Qvalue
71) Pentachlorophenol	16.945	266	33867	3.362 ng/u1	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015949.D
Acq On : 18 Aug 2021 22:24
Operator : CG/JU
Sample : M3399-03
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKA5

Quant Time: Aug 19 01:05:00 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 17 09:43:53 2021
Response via : Initial Calibration

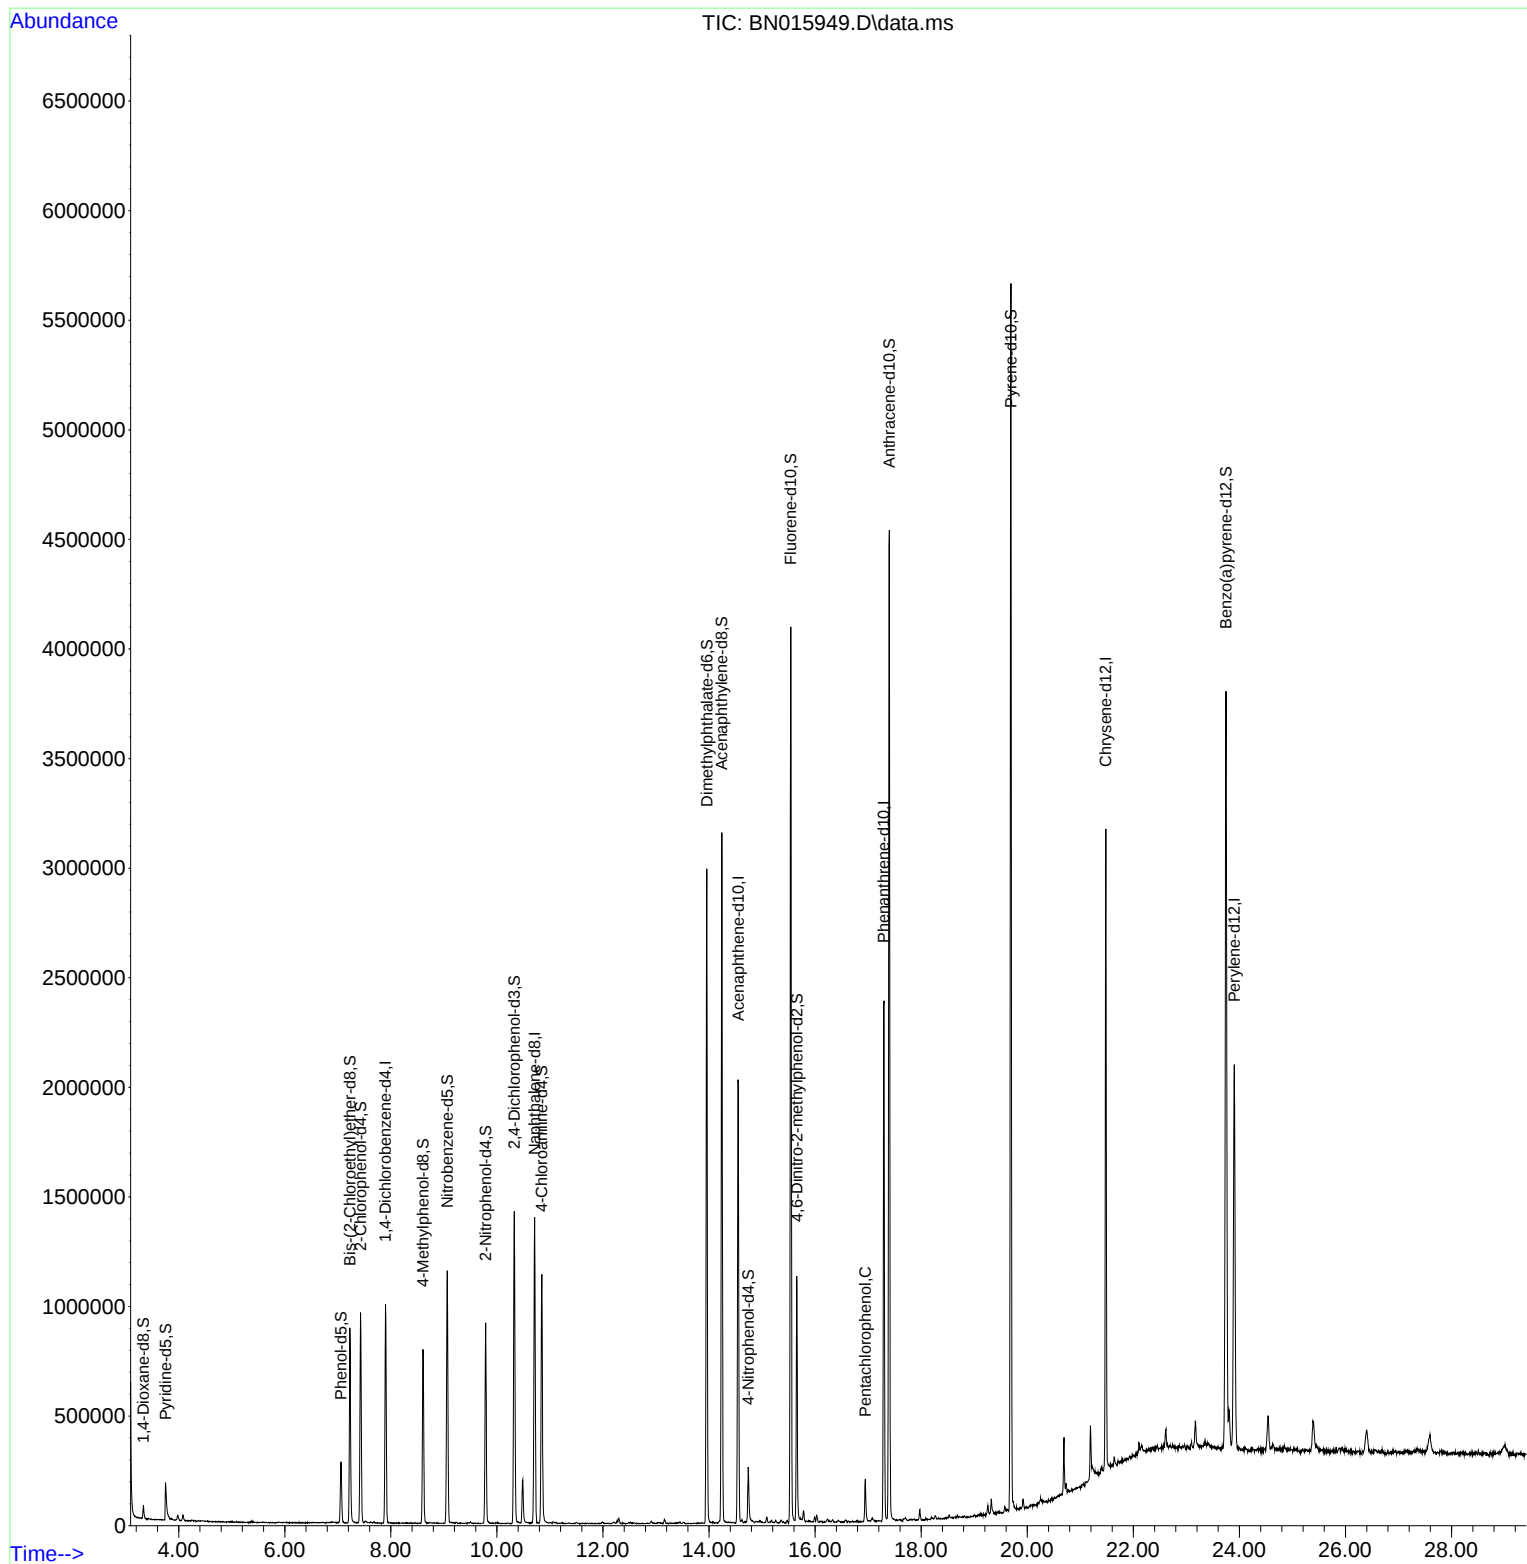

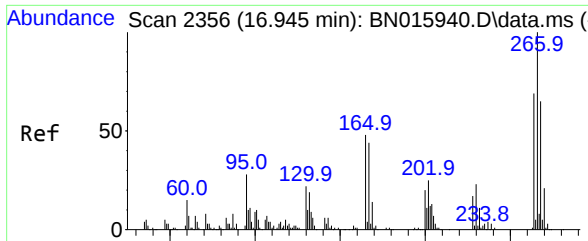

#71
Pentachlorophenol
Concen: 3.362 ng/ul
RT: 16.945 min Scan# 2356
Delta R.T. 0.000 min
Lab File: BN015949.D
Acq: 18 Aug 2021 22:24

Instrument :
BNA_N
ClientSampleId :
DBKA5

Tgt Ion:266 Resp: 33867
Ion Ratio Lower Upper
266 100
264 62.0 53.8 80.6
268 63.0 52.7 79.1

