

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015954.D
 Acq On : 19 Aug 2021 01:27
 Operator : CG/JU
 Sample : M3399-11
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKB3

Quant Time: Aug 19 02:29:50 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 17 09:43:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	248941	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	1053580	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.546	164	665142	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.298	188	1369738	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	1276400	20.000	ng/ul	0.00
88) Perylene-d12	23.904	264	1288187	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	29772	4.659	ng/uL	0.00
4) Pyridine-d5	3.752	84	112087	6.275	ng/ul	0.00
7) Phenol-d5	7.058	99	156210	6.937	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	378458	27.297	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	400667	25.005	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	276341	15.778	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	245068	31.603	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	253614	34.945	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	464394	29.570	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	409005	17.109	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	1814212	37.217	ng/ul	0.00
49) Acenaphthylene-d8	14.240	160	2053203	33.633	ng/ul	0.00
54) 4-Nitrophenol-d4	14.746	143	63064	7.315	ng/ul	0.01
60) Fluorene-d10	15.540	176	1501684	35.317	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	226690	30.989	ng/ul	0.00
73) Anthracene-d10	17.398	188	2491134	38.802	ng/ul	0.00
81) Pyrene-d10	19.692	212	2747521	39.964	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.745	264	2622067	37.646	ng/ul	0.00
Target Compounds						
52) Acenaphthene	14.610	153	100513	2.395	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015954.D
Acq On : 19 Aug 2021 01:27
Operator : CG/JU
Sample : M3399-11
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKB3


Quant Time: Aug 19 02:29:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 17 09:43:53 2021
Response via : Initial Calibration

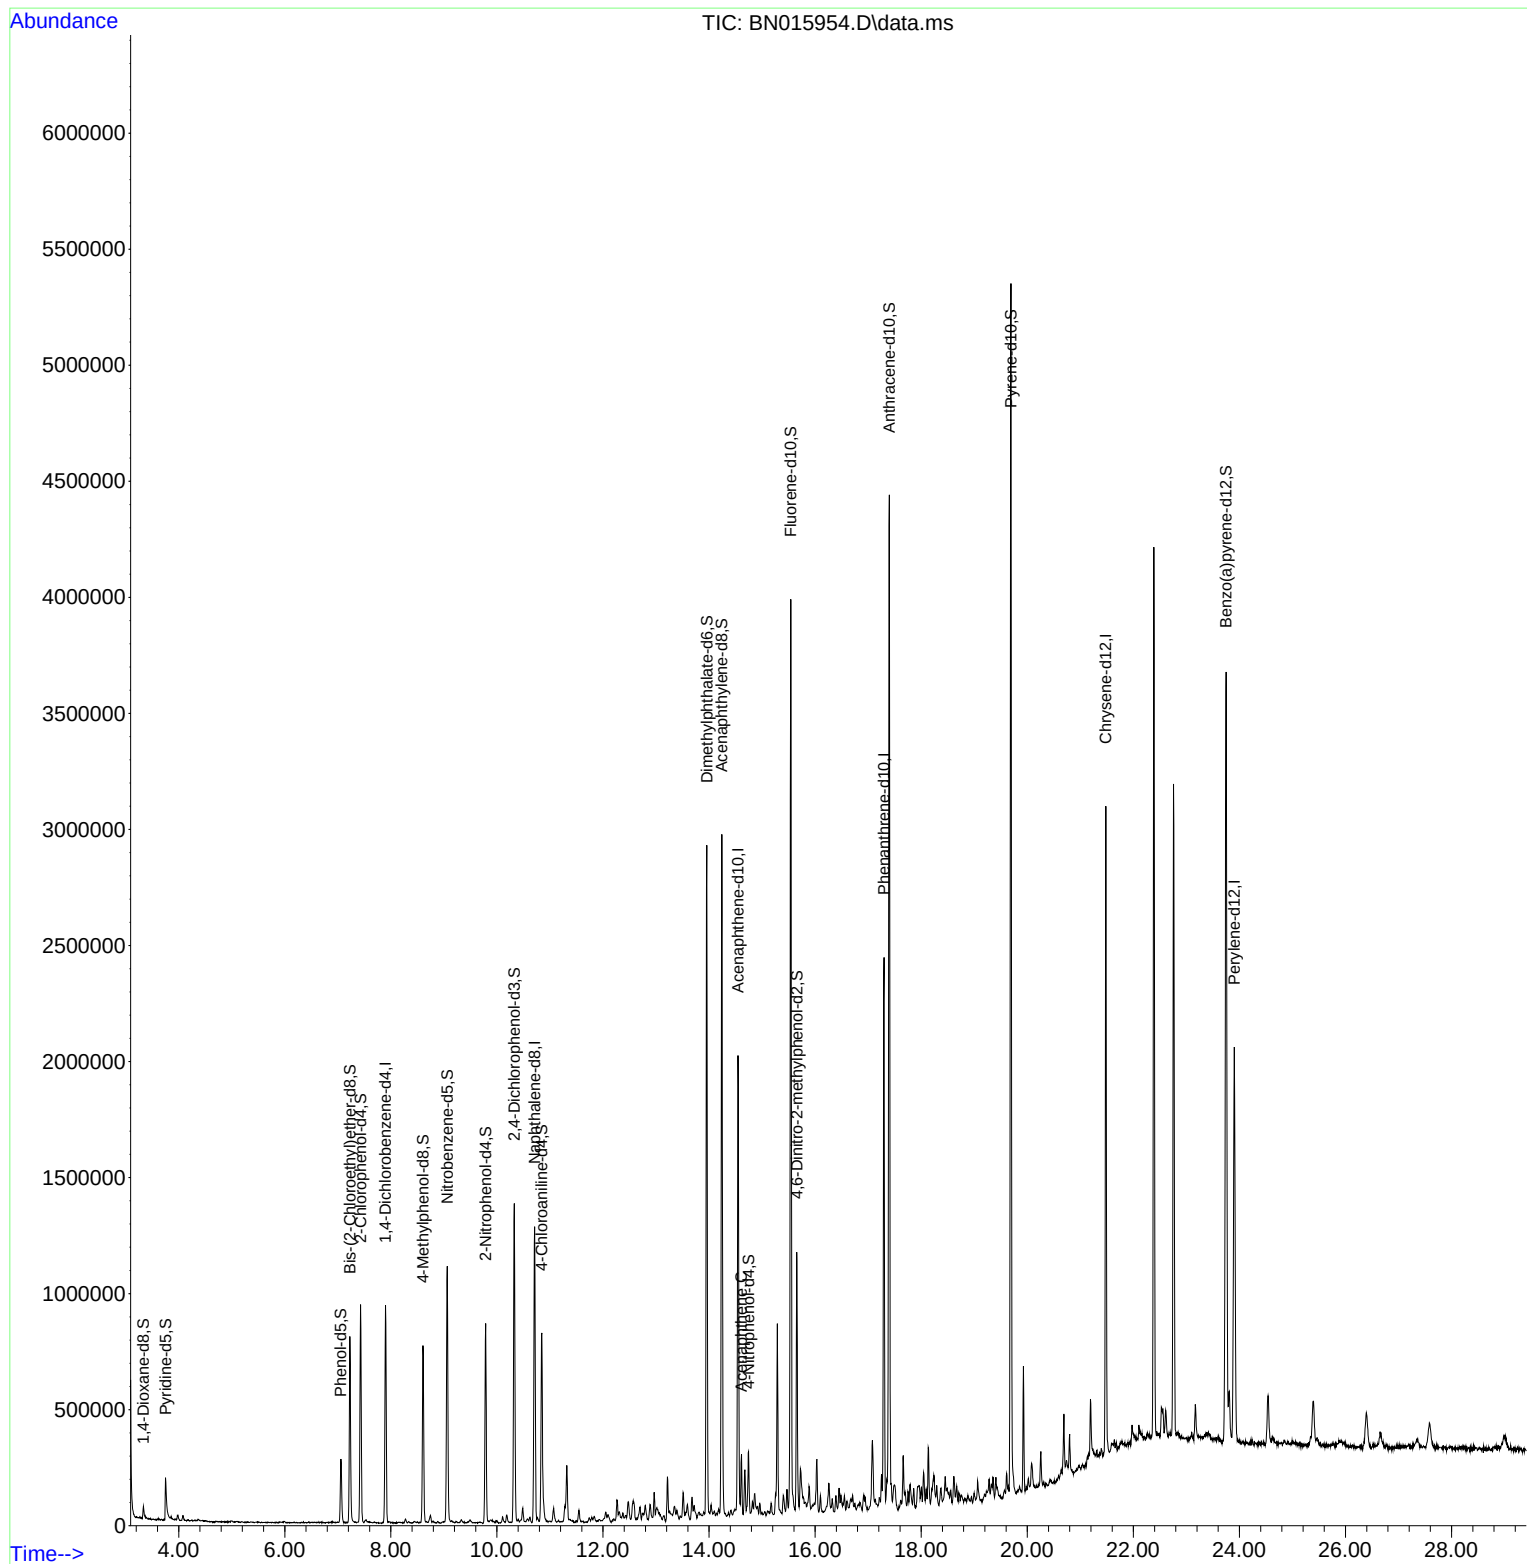

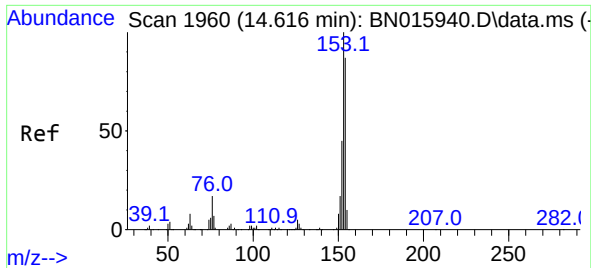

#52
 Acenaphthene
 Concen: 2.395 ng/ul
 RT: 14.610 min Scan# 1959
 Delta R.T. -0.006 min
 Lab File: BN015954.D
 Acq: 19 Aug 2021 01:27

Instrument :
 BNA_N
 ClientSampleId :
 DBKB3

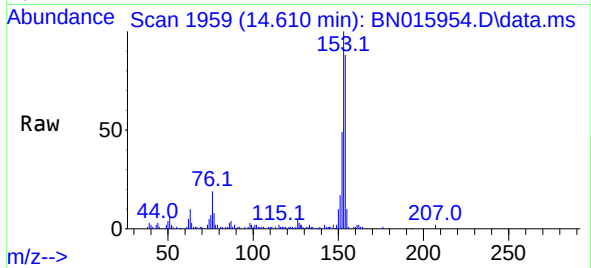

Tgt Ion:153 Resp: 100513
 Ion Ratio Lower Upper
 153 100
 152 49.4 38.6 57.8
 154 88.4 69.3 103.9

