

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015967.D
 Acq On : 19 Aug 2021 10:36
 Operator : CG/JU
 Sample : M3422-13
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKC8

Quant Time: Aug 19 11:31:35 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 17 09:43:53 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	264712	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	1108787	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.545	164	737256	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.298	188	1514237	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	1467142	20.000	ng/ul	0.00
88) Perylene-d12	23.910	264	1448569	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	28138	4.141	ng/uL	0.00
4) Pyridine-d5	3.752	84	121061	6.374	ng/ul	0.00
7) Phenol-d5	7.058	99	157951	6.596	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	410312	27.831	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	413066	24.243	ng/ul	0.00
15) 4-Methylphenol-d8	8.604	113	290306	15.588	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	272489	33.390	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	269984	35.349	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	462637	27.992	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	617110	24.529	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	1769004	32.740	ng/ul	0.00
49) Acenaphthylene-d8	14.239	160	2127765	31.445	ng/ul	0.00
54) 4-Nitrophenol-d4	14.739	143	55589	5.817	ng/ul	0.00
60) Fluorene-d10	15.539	176	1540181	32.679	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	236743	29.275	ng/ul	0.00
73) Anthracene-d10	17.392	188	2738722	38.588	ng/ul	0.00
81) Pyrene-d10	19.692	212	3098702	39.212	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.751	264	2968112	37.896	ng/ul	0.00
Target Compounds						
82) Pyrene	19.722	202	164812	1.656	ng/ul#	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015967.D
Acq On : 19 Aug 2021 10:36
Operator : CG/JU
Sample : M3422-13
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKC8

Quant Time: Aug 19 11:31:35 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 17 09:43:53 2021
Response via : Initial Calibration

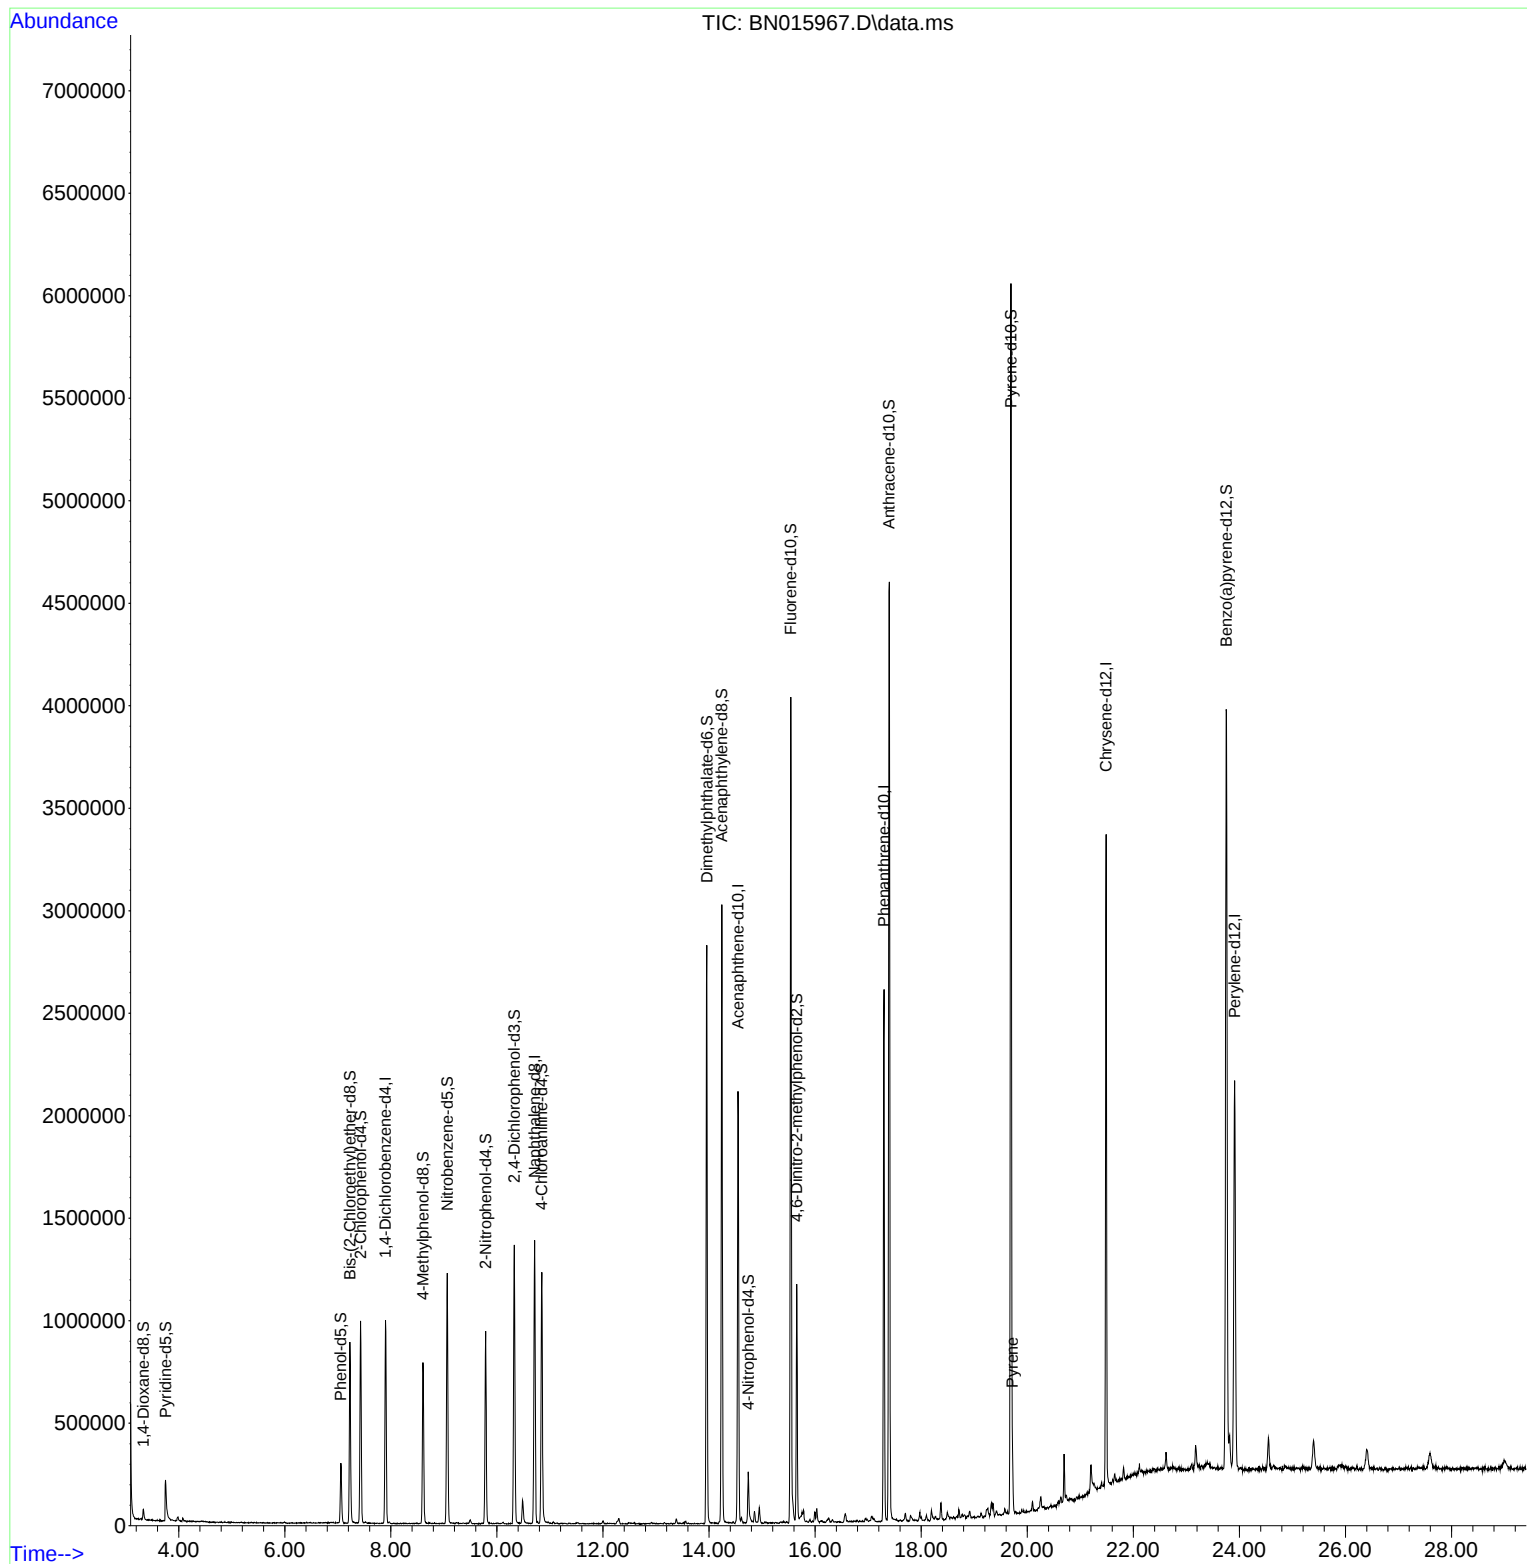

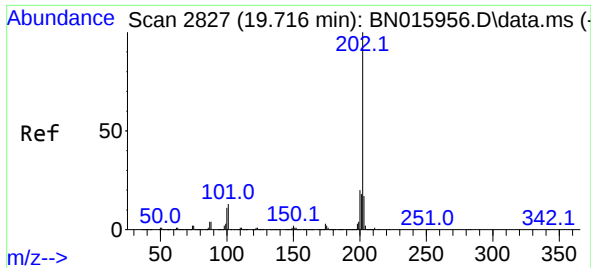

#82

Pyrene

Concen: 1.656 ng/ul

RT: 19.722 min Scan# 2828

Delta R.T. -0.000 min

Lab File: BN015967.D

Acq: 19 Aug 2021 10:36




Tgt Ion:202 Resp: 164812

Ion Ratio Lower Upper

202 100

101 9.9 10.1 15.1#

100 10.3 9.2 13.8

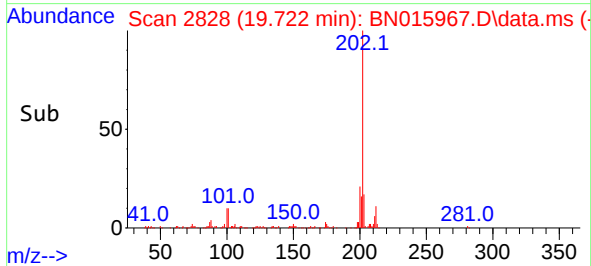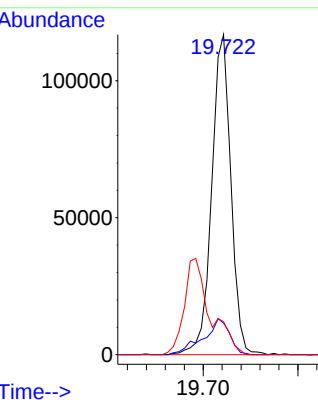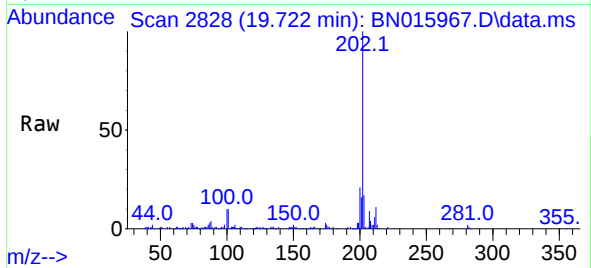

Instrument :

BNA_N

ClientSampleId :

DBKC8