

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015891.D
 Acq On : 17 Aug 2021 09:34
 Operator : CG/JU
 Sample : PB138361BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK361

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015891.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	37	42	50	rVB	85832	128967	1.72%	0.159%
2	3.740	107	111	134	rBV	1061187	1791364	23.83%	2.208%
3	4.081	164	169	175	rVB2	20235	36995	0.49%	0.046%
4	5.093	336	341	348	rVB8	3742	10717	0.14%	0.013%
5	7.052	667	674	686	rBV	1462752	2383152	31.70%	2.937%
6	7.228	697	704	714	rBV	1040001	1772271	23.57%	2.184%
7	7.428	727	738	746	rBV	1483200	2468502	32.83%	3.042%
8	7.899	812	818	828	rVB	1006625	1711067	22.76%	2.109%
9	8.605	929	938	947	rBV	1704481	2878603	38.29%	3.548%
10	9.063	1008	1016	1025	rBV	1396368	2343880	31.17%	2.889%
11	9.787	1132	1139	1151	rVB	1056102	1771140	23.56%	2.183%
12	10.322	1222	1230	1240	rBV	1693851	2896724	38.53%	3.570%
13	10.710	1288	1296	1305	rVB	1398024	2423533	32.23%	2.987%
14	10.846	1311	1319	1330	rBV	1660054	2982645	39.67%	3.676%
15	11.363	1401	1407	1414	rVB7	6878	14379	0.19%	0.018%
16	12.304	1561	1567	1574	rVB2	29814	49993	0.66%	0.062%
17	12.516	1599	1603	1606	rBV5	5367	8999	0.12%	0.011%
18	13.510	1768	1772	1774	rBV5	4670	7522	0.10%	0.009%
19	13.957	1841	1848	1857	rBV	2897807	4196468	55.81%	5.172%
20	14.022	1857	1859	1864	rVB4	6839	9411	0.13%	0.012%
21	14.240	1889	1896	1907	rBV	3337712	4967093	66.06%	6.121%
22	14.551	1941	1949	1958	rVB	2022372	3130954	41.64%	3.859%
23	14.728	1970	1979	1996	rBV	1305083	1984272	26.39%	2.445%
24	15.540	2110	2117	2129	rBV	4077632	6035431	80.27%	7.438%
25	15.651	2130	2136	2148	rBV	1131796	1590311	21.15%	1.960%
26	15.781	2153	2158	2164	rVB2	49848	77743	1.03%	0.096%
27	16.322	2247	2250	2255	rBV3	15514	20629	0.27%	0.025%
28	16.592	2291	2296	2299	rBV6	4410	8300	0.11%	0.010%
29	16.975	2358	2361	2366	rBV6	5932	10842	0.14%	0.013%
30	17.081	2372	2379	2386	rBV7	11254	22738	0.30%	0.028%
31	17.298	2409	2416	2423	rBV	2545878	3638816	48.40%	4.484%
32	17.398	2426	2433	2442	rBV	4374788	6436867	85.61%	7.933%
33	18.516	2614	2623	2627	rBV7	19329	40093	0.53%	0.049%
34	18.810	2671	2673	2678	rBV5	7065	8206	0.11%	0.010%
35	19.322	2756	2760	2765	rVV	48286	71017	0.94%	0.088%
36	19.386	2768	2771	2775	rVB2	46267	57080	0.76%	0.070%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015891.D
 Acq On : 17 Aug 2021 09:34
 Operator : CG/JU
 Sample : PB138361BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK361

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

37	19.575	2799	2803	2807	rVB	43618	54221	0.72%	0.067%
38	19.628	2807	2812	2816	rBV3	81763	100903	1.34%	0.124%
39	19.692	2816	2823	2830	rVV2	5252267	7518631	100.00%	9.266%
40	19.745	2830	2832	2836	rVB4	36082	39211	0.52%	0.048%
41	20.692	2987	2993	2997	rBV2	165650	272533	3.62%	0.336%
42	21.204	3077	3080	3081	rBV2	49442	53671	0.71%	0.066%
43	21.480	3122	3127	3135	rBV	2980560	3945482	52.48%	4.862%
44	23.180	3412	3416	3423	rVB4	104461	162495	2.16%	0.200%
45	23.751	3504	3513	3520	rBV2	3418285	7198684	95.74%	8.872%
46	23.904	3531	3539	3549	rVB2	1811143	3810133	50.68%	4.696%




Sum of corrected areas: 81142688

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015891.D
Acq On : 17 Aug 2021 09:34
Operator : CG/JU
Sample : PB138361BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK361

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

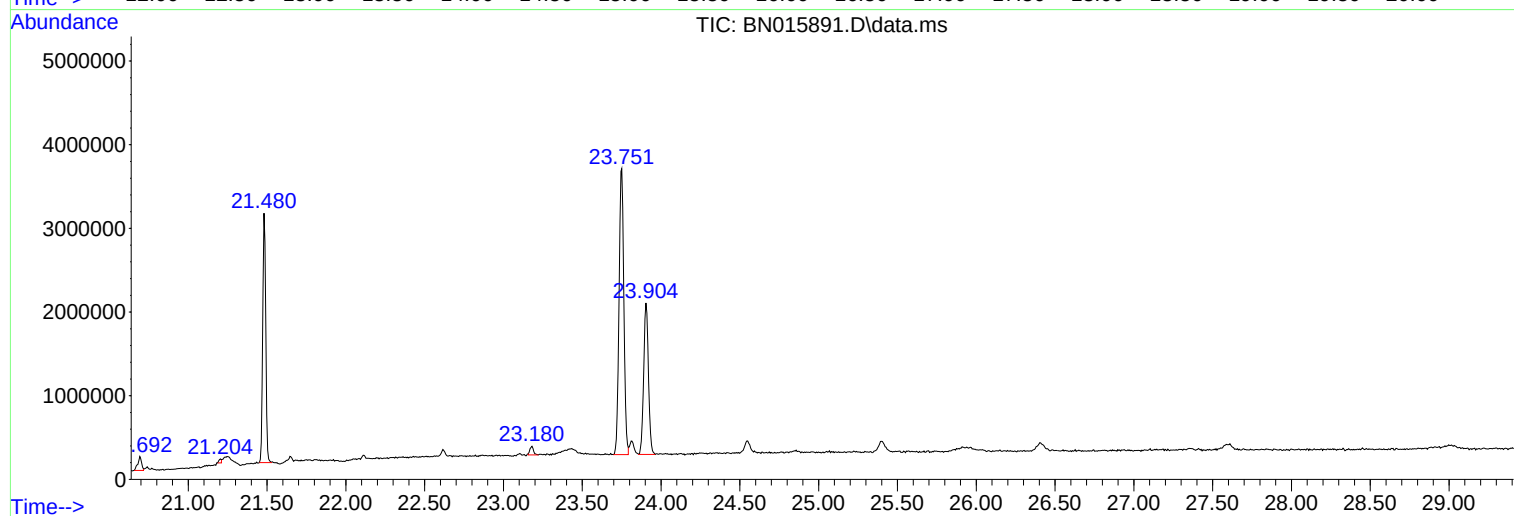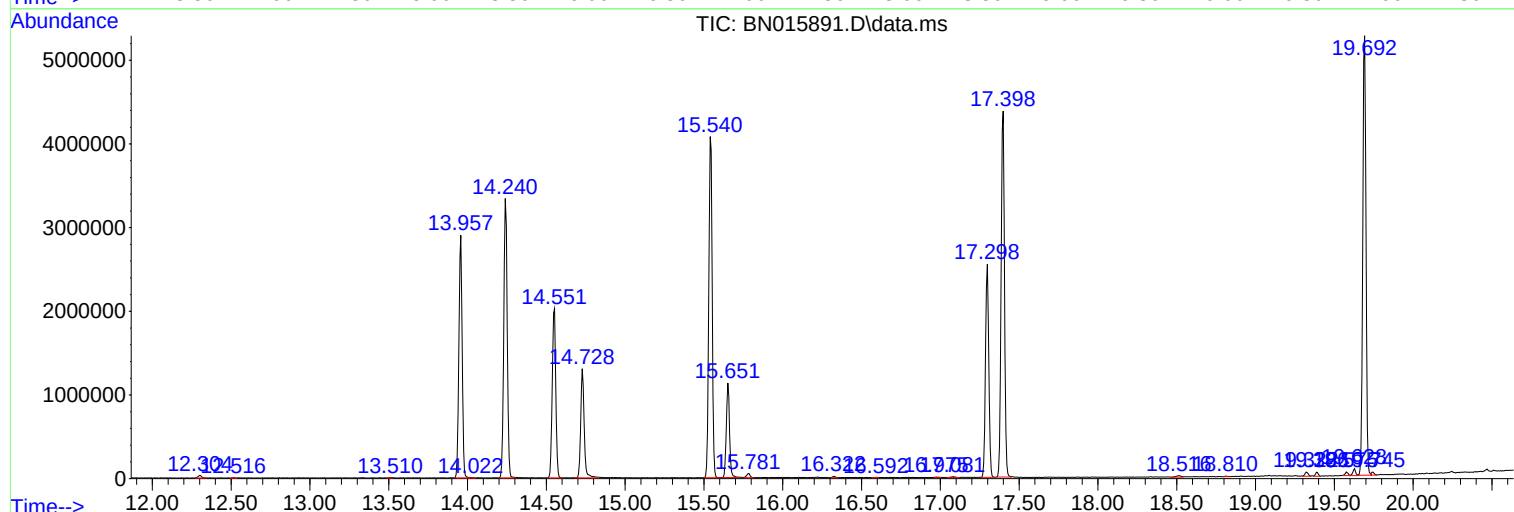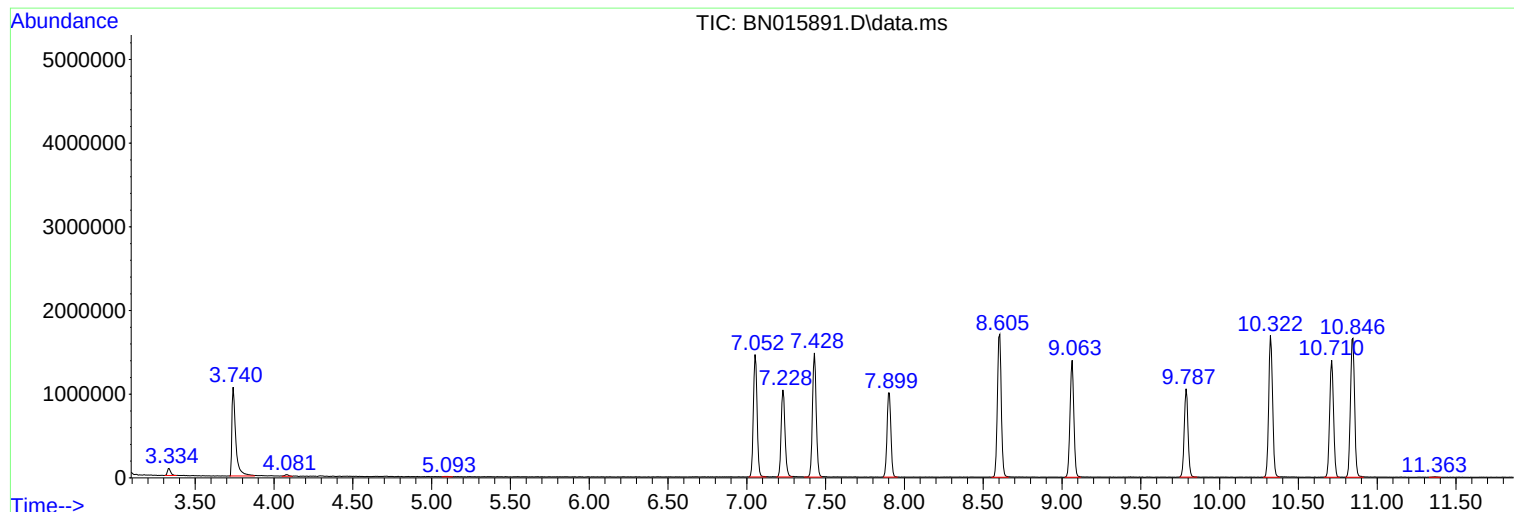

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015891.D
Acq On : 17 Aug 2021 09:34
Operator : CG/JU
Sample : PB138361BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK361

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015891.D
Acq On : 17 Aug 2021 09:34
Operator : CG/JU
Sample : PB138361BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK361

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
