

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015893.D
 Acq On : 17 Aug 2021 10:47
 Operator : CG/JU
 Sample : PB138389BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK389

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015893.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	37	42	50	rVB	84141	125768	1.67%	0.156%
2	3.740	107	111	131	rBV	1032456	1703076	22.67%	2.118%
3	4.081	165	169	173	rVB4	20530	28894	0.38%	0.036%
4	4.299	203	206	208	rBV3	7676	9491	0.13%	0.012%
5	7.052	667	674	684	rBV	1391760	2284702	30.41%	2.841%
6	7.228	698	704	717	rBV	990669	1687718	22.47%	2.099%
7	7.428	731	738	752	rVB	1431579	2365434	31.49%	2.942%
8	7.904	812	819	828	rVB	950860	1653211	22.01%	2.056%
9	8.604	930	938	947	rBV	1646001	2756316	36.69%	3.428%
10	9.063	1008	1016	1027	rBV	1303367	2235801	29.76%	2.781%
11	9.787	1131	1139	1149	rBV	1016398	1705546	22.70%	2.121%
12	10.322	1221	1230	1241	rBV	1621119	2808837	37.39%	3.493%
13	10.710	1289	1296	1305	rVB	1343753	2317363	30.85%	2.882%
14	10.846	1311	1319	1329	rBV	1625629	2842767	37.84%	3.535%
15	11.363	1403	1407	1408	rBV3	6371	8617	0.11%	0.011%
16	12.298	1561	1566	1571	rBV2	30612	47626	0.63%	0.059%
17	13.528	1771	1775	1780	rVB6	5668	9796	0.13%	0.012%
18	13.957	1841	1848	1859	rBV	2826879	4092073	54.47%	5.089%
19	14.239	1889	1896	1904	rBV	3233742	4850732	64.57%	6.032%
20	14.545	1941	1948	1958	rBV	1944800	3072571	40.90%	3.821%
21	14.728	1971	1979	1993	rBV	1312221	1941583	25.84%	2.415%
22	14.839	1995	1998	2001	rVB3	6544	8423	0.11%	0.010%
23	15.539	2110	2117	2126	rBV	4039252	5948550	79.18%	7.398%
24	15.651	2130	2136	2149	rVV	1108623	1584039	21.09%	1.970%
25	15.781	2153	2158	2167	rVB	50310	81550	1.09%	0.101%
26	16.328	2247	2251	2255	rBV4	15752	23475	0.31%	0.029%
27	16.975	2357	2361	2366	rBV8	5445	8032	0.11%	0.010%
28	17.086	2374	2380	2385	rBV5	8737	14749	0.20%	0.018%
29	17.298	2409	2416	2422	rBV	2435402	3593880	47.84%	4.469%
30	17.398	2425	2433	2444	rBV2	4143327	6331141	84.28%	7.874%
31	18.222	2567	2573	2575	rVB7	6135	9467	0.13%	0.012%
32	18.263	2576	2580	2582	rBV5	6123	8053	0.11%	0.010%
33	18.516	2617	2623	2624	rBV4	23007	34102	0.45%	0.042%
34	19.322	2754	2760	2767	rBV2	54190	78956	1.05%	0.098%
35	19.386	2767	2771	2776	rVB4	53631	63866	0.85%	0.079%
36	19.580	2798	2804	2808	rBV	43830	65390	0.87%	0.081%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015893.D
 Acq On : 17 Aug 2021 10:47
 Operator : CG/JU
 Sample : PB138389BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK389

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

37	19.627	2808	2812	2816	rVV2	84488	101917	1.36%	0.127%
38	19.692	2816	2823	2829	rVV	5437541	7512476	100.00%	9.343%
39	19.745	2829	2832	2836	rVB5	34778	41647	0.55%	0.052%
40	20.239	2913	2916	2919	rBV5	17989	22636	0.30%	0.028%
41	20.469	2950	2955	2959	rBV6	32124	48452	0.64%	0.060%
42	20.692	2987	2993	2998	rBV2	164408	274215	3.65%	0.341%
43	20.739	2998	3001	3004	rVV4	24640	29385	0.39%	0.037%
44	21.204	3077	3080	3083	rBV5	34408	51143	0.68%	0.064%
45	21.480	3122	3127	3135	rBV	2925278	3948689	52.56%	4.911%
46	22.110	3232	3234	3240	rVB5	51397	67562	0.90%	0.084%
47	22.615	3318	3320	3327	rVB4	90601	113434	1.51%	0.141%
48	23.180	3412	3416	3421	rVB4	112317	179901	2.39%	0.224%
49	23.751	3505	3513	3520	rBV2	3559955	7116661	94.73%	8.850%
50	23.815	3521	3524	3531	rVB4	189445	326650	4.35%	0.406%
51	23.904	3532	3539	3549	rVB2	1852118	3835710	51.06%	4.770%
52	24.551	3644	3649	3655	rVB3	167689	337961	4.50%	0.420%




Sum of corrected areas: 80410034

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015893.D
Acq On : 17 Aug 2021 10:47
Operator : CG/JU
Sample : PB138389BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK389

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

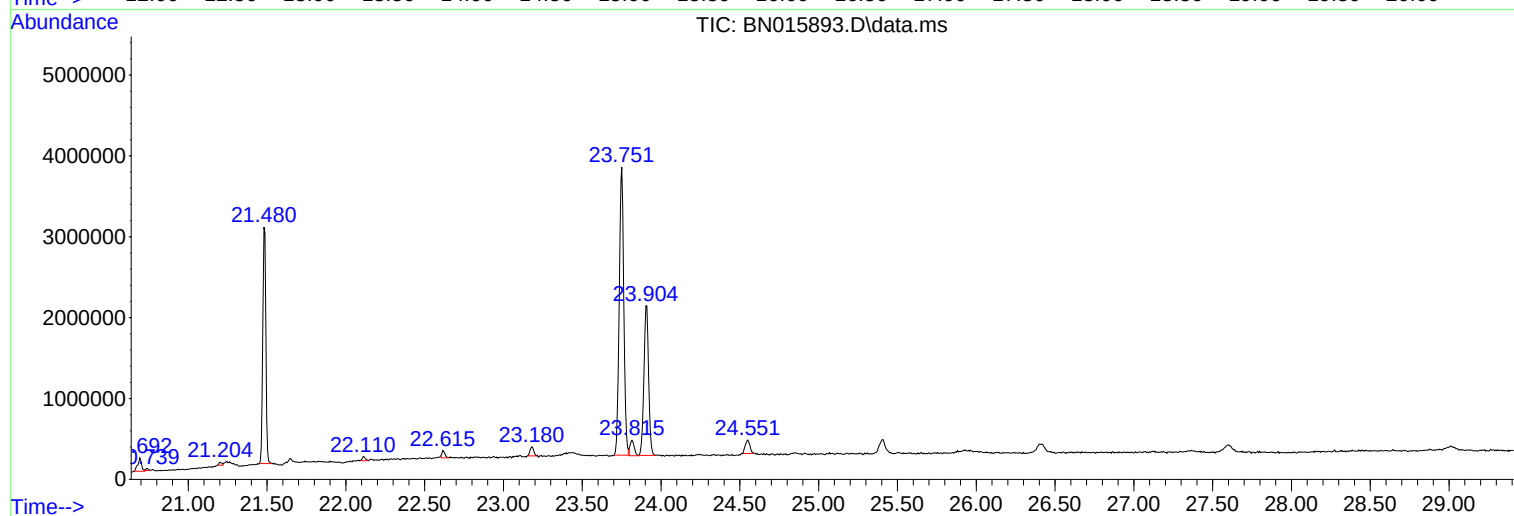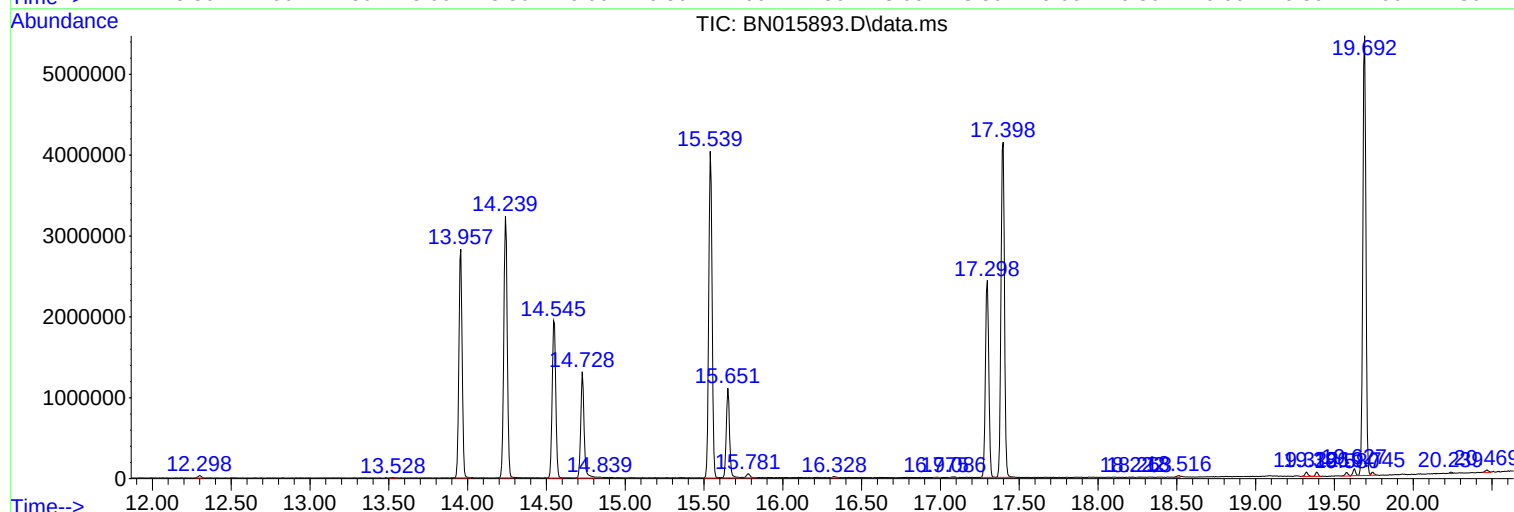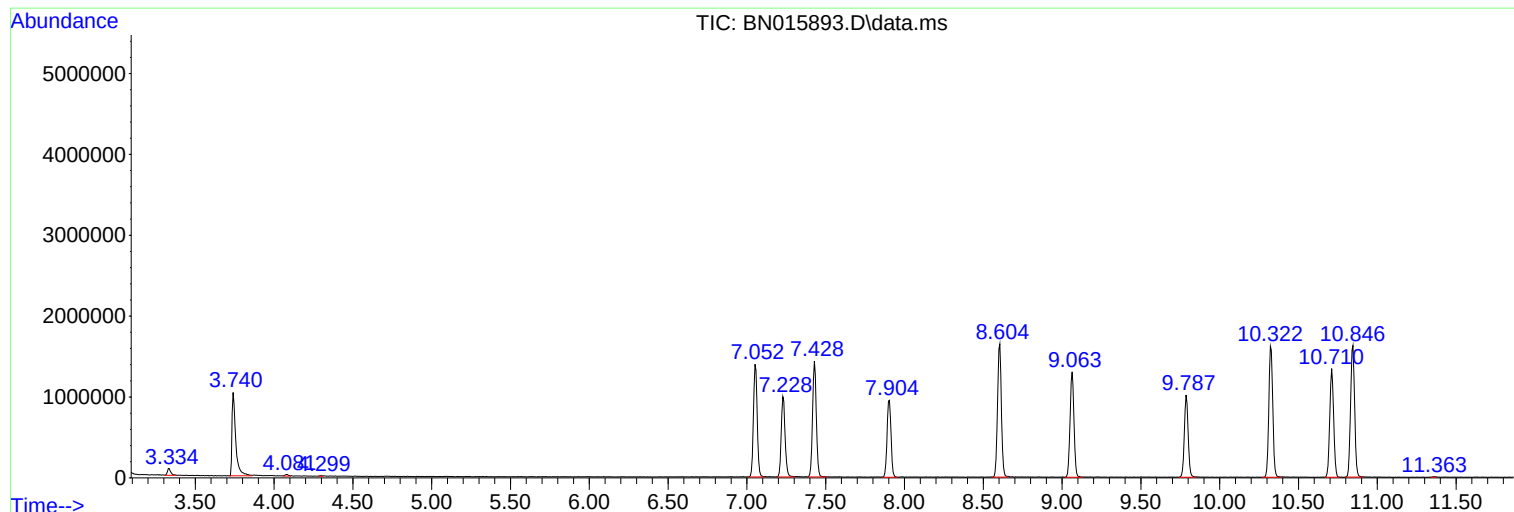

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015893.D
Acq On : 17 Aug 2021 10:47
Operator : CG/JU
Sample : PB138389BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK389

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015893.D
Acq On : 17 Aug 2021 10:47
Operator : CG/JU
Sample : PB138389BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK389

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
