

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015910.D
 Acq On : 17 Aug 2021 21:45
 Operator : CG/JU
 Sample : M3364-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBK92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015910.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	38	42	50	rVB	75804	110143	1.39%	0.150%
2	3.752	111	113	124	rBV	161225	300016	3.79%	0.409%
3	3.981	149	152	158	rVB	21964	34661	0.44%	0.047%
4	4.081	165	169	173	rVB2	15551	22212	0.28%	0.030%
5	7.064	670	676	683	rBV	291764	482286	6.09%	0.657%
6	7.228	697	704	717	rBV	852617	1488689	18.81%	2.029%
7	7.434	731	739	746	rBV	965328	1631922	20.62%	2.224%
8	7.528	751	755	758	rBV4	7007	11686	0.15%	0.016%
9	7.905	811	819	827	rBV	984778	1681874	21.25%	2.292%
10	7.963	827	829	835	rVB5	6871	9261	0.12%	0.013%
11	8.611	932	939	951	rVB	786480	1316759	16.64%	1.795%
12	9.063	1009	1016	1026	rBV	1187553	2035915	25.73%	2.775%
13	9.234	1039	1045	1049	rBV7	5444	10133	0.13%	0.014%
14	9.787	1131	1139	1149	rBV	927388	1654447	20.91%	2.255%
15	10.010	1174	1177	1182	rBV4	6158	8636	0.11%	0.012%
16	10.328	1224	1231	1240	rBV	1405787	2466115	31.16%	3.361%
17	10.487	1252	1258	1269	rBV	157825	273594	3.46%	0.373%
18	10.710	1288	1296	1306	rVB	1339388	2409936	30.45%	3.284%
19	10.846	1311	1319	1332	rBV	1094252	1989016	25.14%	2.711%
20	11.369	1401	1408	1411	rBV7	4383	9568	0.12%	0.013%
21	12.204	1544	1550	1554	rBV5	11255	19113	0.24%	0.026%
22	12.299	1561	1566	1574	rVB2	24553	44093	0.56%	0.060%
23	13.163	1709	1713	1718	rBV4	8364	12366	0.16%	0.017%
24	13.446	1758	1761	1763	rBV2	5146	8205	0.10%	0.011%
25	13.522	1766	1774	1776	rBV7	7498	15107	0.19%	0.021%
26	13.957	1842	1848	1857	rBV	2934825	4293200	54.25%	5.851%
27	14.245	1885	1897	1909	rBV	2970681	4636186	58.59%	6.319%
28	14.504	1938	1941	1942	rBV3	12490	9956	0.13%	0.014%
29	14.551	1942	1949	1956	rVV	2025007	3126230	39.51%	4.261%
30	14.616	1957	1960	1964	rVB3	14502	19916	0.25%	0.027%
31	14.745	1970	1982	1993	rBV	268979	472879	5.98%	0.644%
32	14.963	2014	2019	2024	rBV6	18472	25418	0.32%	0.035%
33	15.293	2069	2075	2080	rBV	104759	147146	1.86%	0.201%
34	15.369	2083	2088	2091	rVB4	7570	14195	0.18%	0.019%
35	15.545	2111	2118	2130	rBV	3853864	5897888	74.53%	8.038%
36	15.657	2130	2137	2147	rBV	1237658	1796908	22.71%	2.449%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015910.D
 Acq On : 17 Aug 2021 21:45
 Operator : CG/JU
 Sample : M3364-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBK92

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

37	15.781	2154	2158	2165	rVB2	56376	87951	1.11%	0.120%
38	15.904	2172	2179	2182	rBV5	9530	21145	0.27%	0.029%
39	15.992	2190	2194	2198	rVB5	11910	15113	0.19%	0.021%
40	16.110	2206	2214	2215	rBV6	6581	12229	0.15%	0.017%
41	16.222	2228	2233	2234	rBV5	12085	12332	0.16%	0.017%
42	16.269	2240	2241	2247	rVB5	8635	9767	0.12%	0.013%
43	16.328	2247	2251	2255	rVB6	19350	29787	0.38%	0.041%
44	16.439	2266	2270	2273	rBV6	7891	11999	0.15%	0.016%
45	16.481	2275	2277	2283	rVB6	7970	12849	0.16%	0.018%
46	16.792	2325	2330	2336	rVB9	12809	26694	0.34%	0.036%
47	16.975	2358	2361	2366	rBV7	9707	17436	0.22%	0.024%
48	17.063	2371	2376	2378	rBV6	13446	21179	0.27%	0.029%
49	17.081	2378	2379	2383	rVB5	9138	9759	0.12%	0.013%
50	17.298	2409	2416	2425	rBV	2527355	3664218	46.30%	4.994%
51	17.398	2427	2433	2444	rVB2	4543346	6778907	85.67%	9.239%
52	17.669	2476	2479	2484	rVB6	10380	14327	0.18%	0.020%
53	17.975	2528	2531	2536	rVB7	27644	34712	0.44%	0.047%
54	18.198	2563	2569	2575	rBV6	37727	70799	0.89%	0.096%
55	18.269	2577	2581	2585	rVB	19398	29500	0.37%	0.040%
56	18.522	2621	2624	2630	rVV8	15119	29736	0.38%	0.041%
57	18.569	2630	2632	2636	rVB5	9499	10577	0.13%	0.014%
58	19.092	2717	2721	2725	rBV7	13851	21440	0.27%	0.029%
59	19.257	2744	2749	2753	rBV2	40796	63768	0.81%	0.087%
60	19.322	2757	2760	2768	rVB	65593	106738	1.35%	0.145%
61	19.410	2773	2775	2777	rBV3	10302	8027	0.10%	0.011%
62	19.581	2800	2804	2807	rBV3	24141	35067	0.44%	0.048%
63	19.692	2817	2823	2830	rBV	5457407	7913253	100.00%	10.785%
64	20.692	2989	2993	2997	rBV	237583	299464	3.78%	0.408%
65	21.198	3075	3079	3083	rBV3	187610	287255	3.63%	0.391%
66	21.486	3122	3128	3138	rBV	2778602	3823875	48.32%	5.211%
67	23.174	3412	3415	3422	rVB4	116734	193011	2.44%	0.263%
68	23.757	3505	3514	3520	rBV	3582371	7463721	94.32%	10.172%
69	23.910	3533	3540	3549	rVB2	1762112	3751776	47.41%	5.113%


Sum of corrected areas: 73374086

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015910.D
Acq On : 17 Aug 2021 21:45
Operator : CG/JU
Sample : M3364-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBK92

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

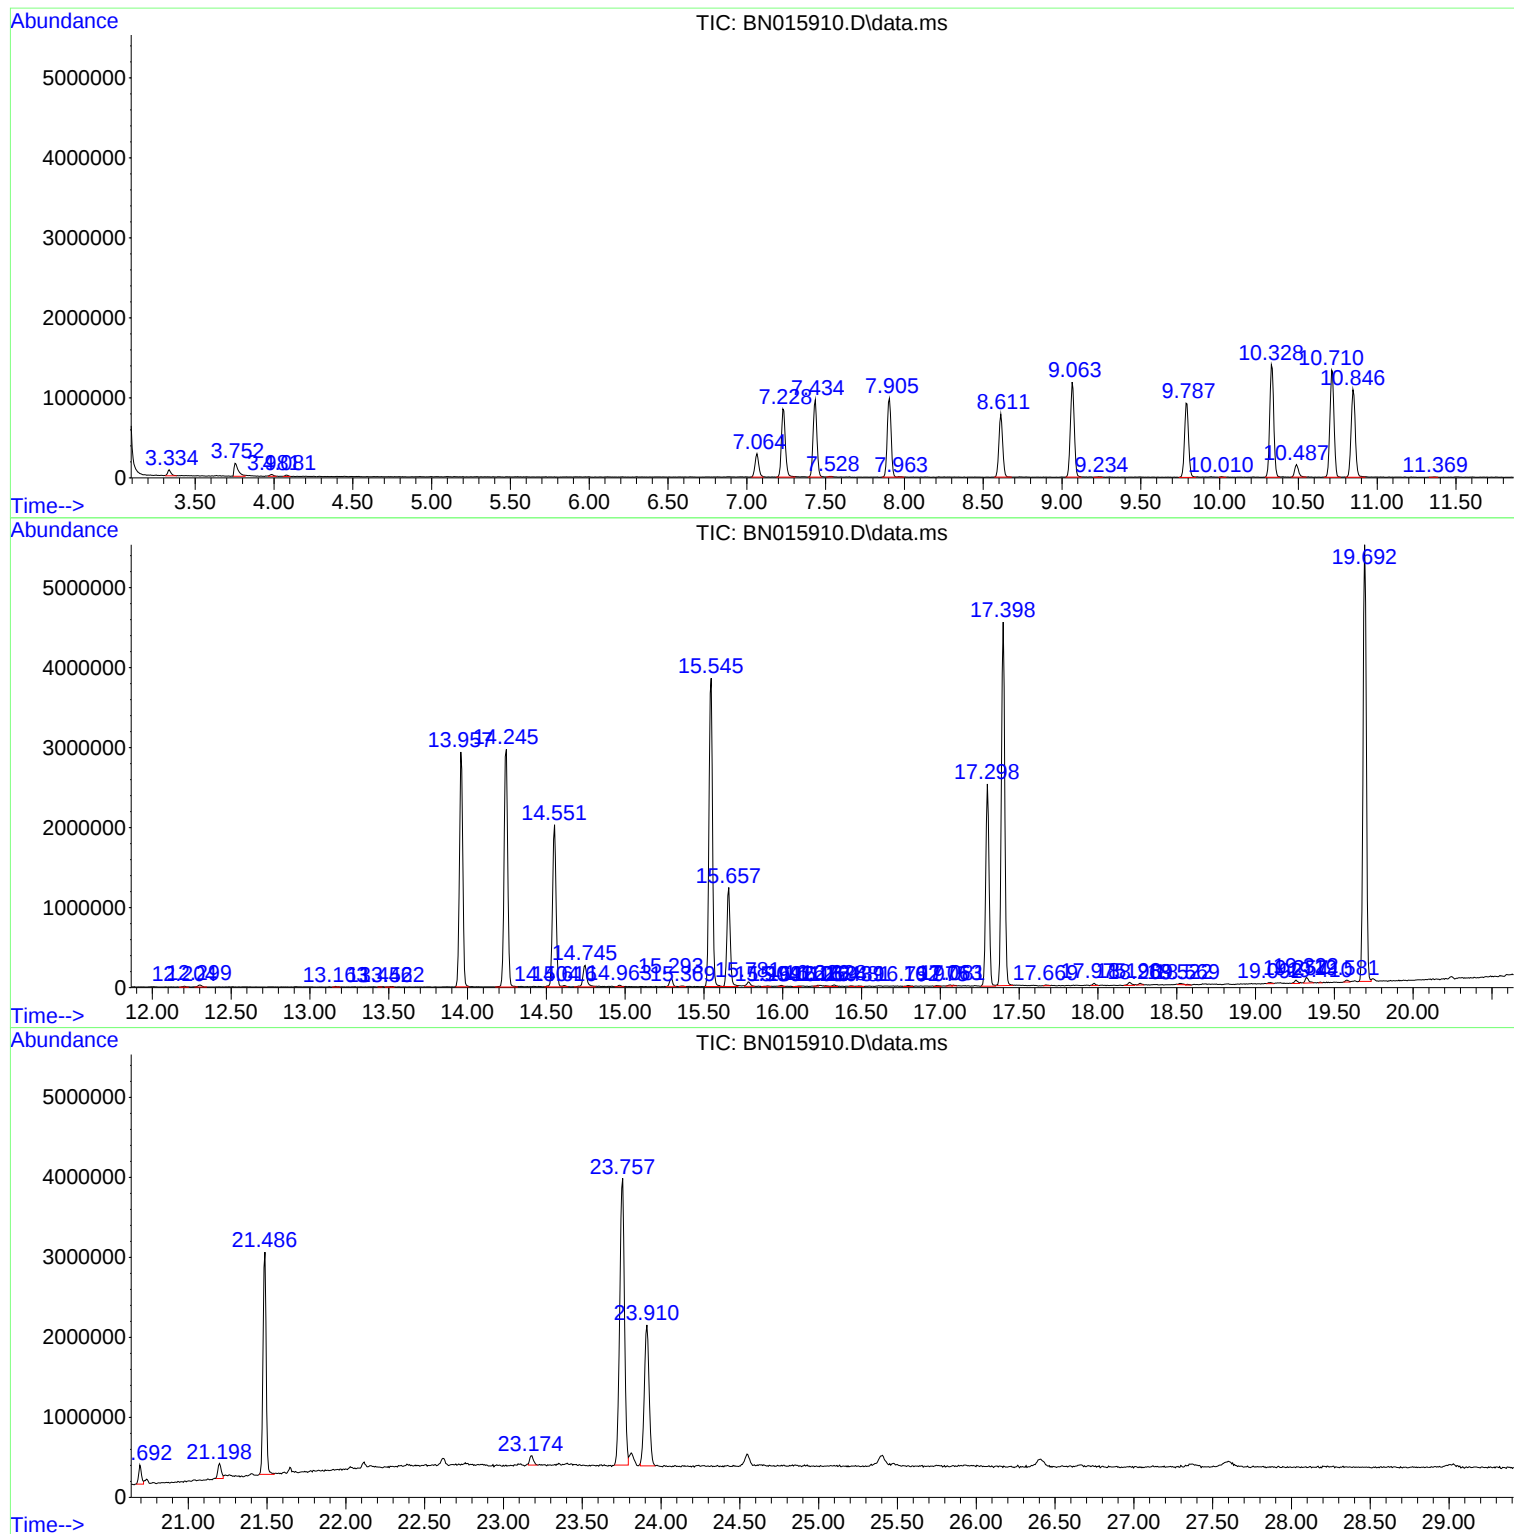

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015910.D
Acq On : 17 Aug 2021 21:45
Operator : CG/JU
Sample : M3364-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBK92










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.487	2.27 ng/ul	273594	Naphthalene-d8	10.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	91
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83
4			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	80
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	78

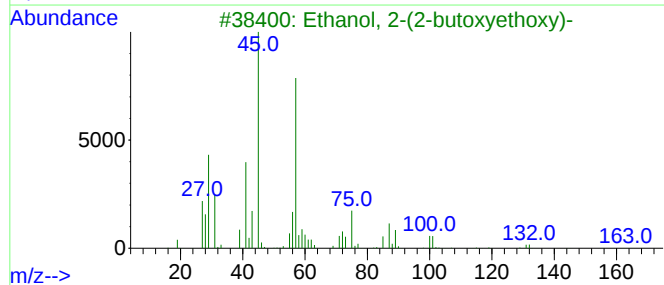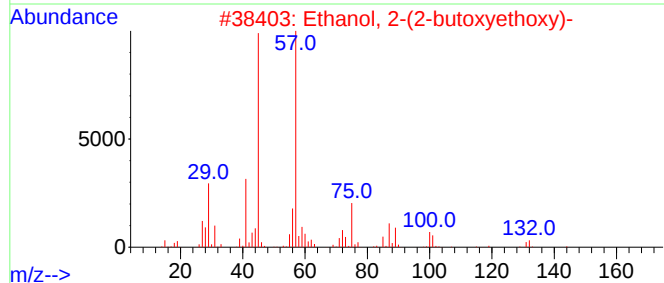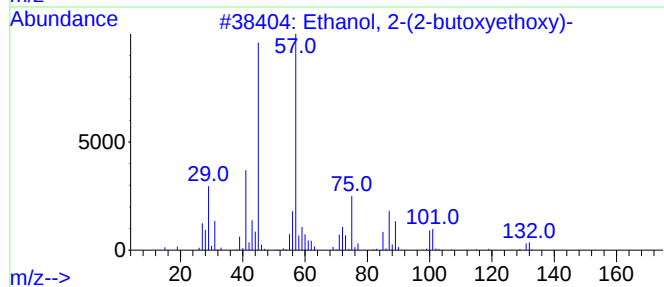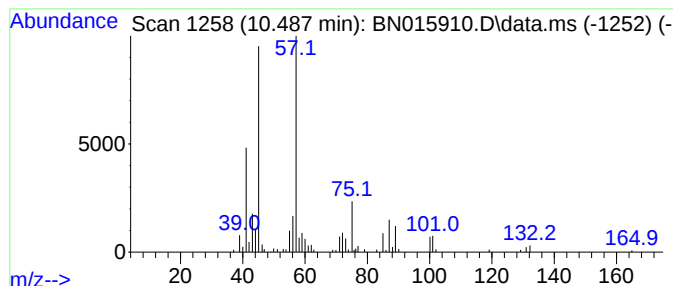

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015910.D
Acq On : 17 Aug 2021 21:45
Operator : CG/JU
Sample : M3364-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBK92

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.487	2.3	ng/u1	273594	2	10.710	2409940	20.0