

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015914.D
 Acq On : 18 Aug 2021 00:48
 Operator : CG/JU
 Sample : M3432-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015914.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.570	80	82	85	rVB4	6503	6091	0.16%	0.033%
2	3.740	110	111	114	rBV3	3812	4540	0.12%	0.025%
3	4.081	166	169	173	rVB3	13957	22498	0.60%	0.123%
4	4.164	180	183	185	rVB4	5168	6642	0.18%	0.036%
5	4.599	255	257	262	rBV4	3057	3769	0.10%	0.021%
6	4.723	274	278	281	rVB3	2511	4257	0.11%	0.023%
7	5.181	350	356	358	rBV5	3294	5430	0.15%	0.030%
8	6.917	647	651	652	rVB3	3580	3830	0.10%	0.021%
9	7.493	746	749	752	rBV3	2761	3760	0.10%	0.021%
10	7.905	809	819	826	rBV	938143	1611970	43.11%	8.832%
11	8.105	848	853	855	rBV4	2854	4425	0.12%	0.024%
12	8.316	887	889	894	rVB3	2950	4192	0.11%	0.023%
13	9.140	1027	1029	1033	rVB5	2878	3921	0.10%	0.021%
14	9.322	1055	1060	1063	rBV6	3019	4817	0.13%	0.026%
15	9.499	1088	1090	1095	rVB4	3411	4402	0.12%	0.024%
16	10.152	1197	1201	1203	rBV5	2661	4492	0.12%	0.025%
17	10.646	1281	1285	1286	rBV4	3056	4315	0.12%	0.024%
18	10.710	1288	1296	1306	rVV	1345000	2311753	61.83%	12.666%
19	12.646	1622	1625	1630	rVB5	3467	5197	0.14%	0.028%
20	13.287	1728	1734	1738	rBV7	3292	6910	0.18%	0.038%
21	14.551	1940	1949	1958	rBV	1961956	2996196	80.13%	16.416%
22	14.875	1999	2004	2005	rBV3	3431	3854	0.10%	0.021%
23	15.428	2094	2098	2103	rVB4	2799	3994	0.11%	0.022%
24	15.593	2123	2126	2130	rVB4	3514	4170	0.11%	0.023%
25	15.751	2149	2153	2154	rBV2	3282	4990	0.13%	0.027%
26	16.193	2226	2228	2233	rVB5	3171	4554	0.12%	0.025%
27	16.863	2340	2342	2344	rBV2	4305	3824	0.10%	0.021%
28	17.087	2374	2380	2384	rVB3	11131	13558	0.36%	0.074%
29	17.222	2402	2403	2408	rBV5	4365	6218	0.17%	0.034%
30	17.298	2408	2416	2429	rVV	2345442	3499974	93.61%	19.176%
31	17.392	2429	2432	2437	rVB	12886	23759	0.64%	0.130%
32	17.598	2465	2467	2470	rVB3	4626	5059	0.14%	0.028%
33	17.628	2470	2472	2474	rBV3	4223	3970	0.11%	0.022%
34	17.687	2479	2482	2483	rBV2	4761	4030	0.11%	0.022%
35	18.034	2537	2541	2542	rVB4	4691	4368	0.12%	0.024%
36	18.275	2580	2582	2585	rBV3	4497	5373	0.14%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015914.D
 Acq On : 18 Aug 2021 00:48
 Operator : CG/JU
 Sample : M3432-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

37	18.963	2696	2699	2700	rBV3	4450	4455	0.12%	0.024%
38	19.034	2709	2711	2714	rBV4	4937	6640	0.18%	0.036%
39	19.087	2717	2720	2722	rBV4	5237	5580	0.15%	0.031%
40	19.110	2722	2724	2730	rBV5	4013	8962	0.24%	0.049%
41	19.234	2743	2745	2749	rBV4	3236	4369	0.12%	0.024%
42	19.304	2754	2757	2758	rBV3	4298	4602	0.12%	0.025%
43	19.575	2801	2803	2804	rBV2	6780	4106	0.11%	0.022%
44	19.757	2832	2834	2836	rBV3	5889	6567	0.18%	0.036%
45	19.916	2859	2861	2862	rVB2	8062	3943	0.11%	0.022%
46	20.692	2989	2993	3000	rBV	174267	224348	6.00%	1.229%
47	21.480	3122	3127	3133	rBV	2833539	3739031	100.00%	20.486%
48	23.904	3532	3539	3549	rVB2	1704172	3623894	96.92%	19.855%




Sum of corrected areas: 18251599

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015914.D
Acq On : 18 Aug 2021 00:48
Operator : CG/JU
Sample : M3432-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

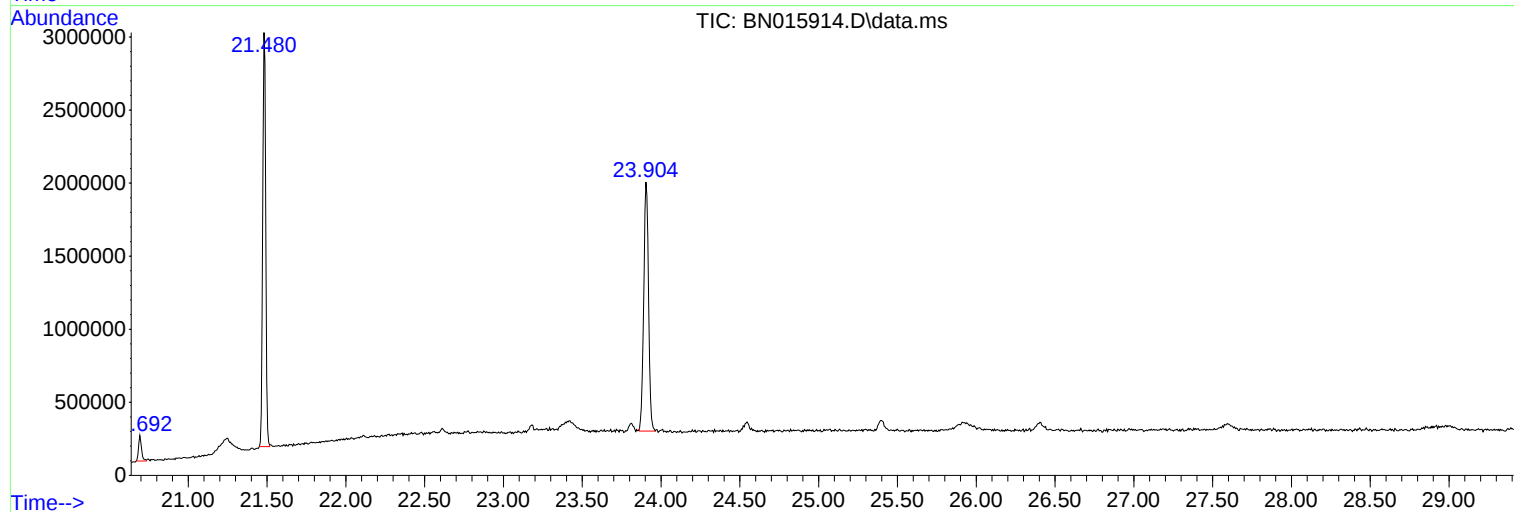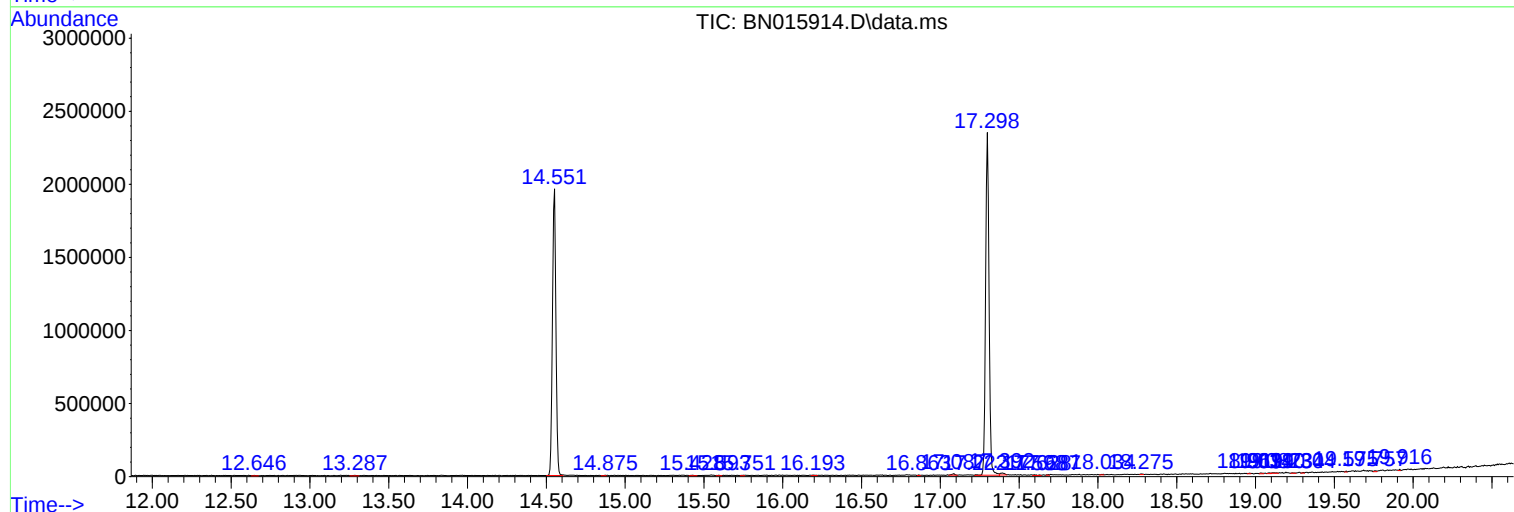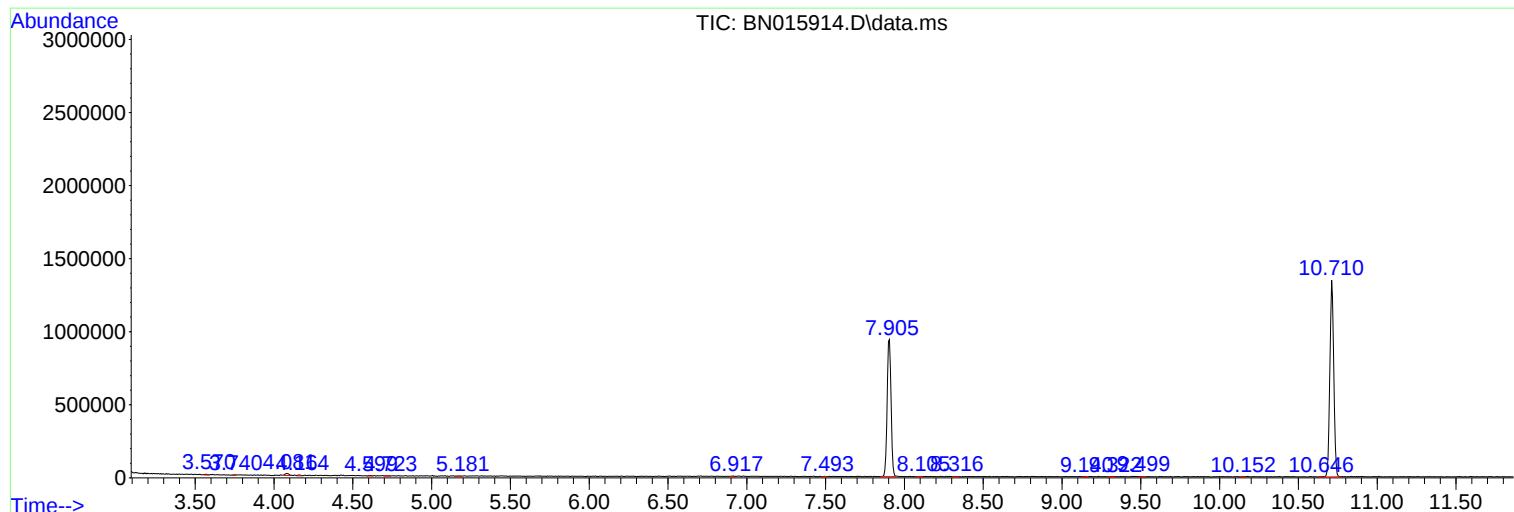

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015914.D
Acq On : 18 Aug 2021 00:48
Operator : CG/JU
Sample : M3432-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015914.D
Acq On : 18 Aug 2021 00:48
Operator : CG/JU
Sample : M3432-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
