

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015928.D
 Acq On : 18 Aug 2021 09:34
 Operator : CG/JU
 Sample : PB138421BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK421

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015928.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	37	42	50	rVB	78392	125027	1.25%	0.128%
2	3.740	108	111	129	rBV	1155839	1937228	19.38%	1.981%
3	4.075	165	168	173	rVB2	16798	25635	0.26%	0.026%
4	7.057	668	675	684	rBV	1612615	2663748	26.65%	2.723%
5	7.228	697	704	714	rBV	1148025	1873012	18.74%	1.915%
6	7.428	731	738	748	rVB	1591254	2646760	26.48%	2.706%
7	7.899	809	818	826	rBV	1100192	1829945	18.31%	1.871%
8	8.604	932	938	947	rBV	1988571	3368652	33.70%	3.444%
9	9.063	1008	1016	1024	rBV	1576631	2679916	26.81%	2.740%
10	9.787	1130	1139	1152	rBV	1338832	2256026	22.57%	2.306%
11	10.328	1223	1231	1243	rBV	2020912	3450250	34.51%	3.527%
12	10.710	1287	1296	1306	rBV	1471091	2637671	26.39%	2.697%
13	10.846	1311	1319	1328	rBV	2025028	3564523	35.66%	3.644%
14	12.298	1560	1566	1572	rVB2	38717	61627	0.62%	0.063%
15	12.481	1595	1597	1600	rBV3	7876	11517	0.12%	0.012%
16	13.522	1768	1774	1779	rVB6	7871	10468	0.10%	0.011%
17	13.957	1841	1848	1857	rBV	3776416	5444892	54.47%	5.567%
18	14.239	1888	1896	1904	rBV	4050027	6189962	61.92%	6.328%
19	14.545	1941	1948	1962	rVB	2231420	3475073	34.76%	3.553%
20	14.739	1973	1981	1997	rBV	1929265	2832408	28.33%	2.896%
21	15.539	2110	2117	2129	rBV	5274671	7703442	77.06%	7.876%
22	15.651	2129	2136	2150	rVV	1299253	1926092	19.27%	1.969%
23	15.781	2152	2158	2165	rVB2	62891	106241	1.06%	0.109%
24	16.322	2246	2250	2256	rVB7	14542	23322	0.23%	0.024%
25	16.975	2358	2361	2364	rBV4	8161	11767	0.12%	0.012%
26	17.080	2376	2379	2381	rBV2	12468	13778	0.14%	0.014%
27	17.298	2409	2416	2423	rBV	2704622	3995590	39.97%	4.085%
28	17.398	2423	2433	2445	rVV	5776318	8552321	85.55%	8.743%
29	19.257	2744	2749	2753	rVB4	40218	62627	0.63%	0.064%
30	19.327	2755	2761	2769	rBV	71223	116394	1.16%	0.119%
31	19.574	2800	2803	2809	rBV	27338	46962	0.47%	0.048%
32	19.692	2816	2823	2833	rBV	7301985	9996509	100.00%	10.220%
33	20.474	2952	2956	2958	rBV5	12271	15734	0.16%	0.016%
34	20.692	2989	2993	3000	rBV2	138348	195858	1.96%	0.200%
35	21.486	3122	3128	3133	rBV	3249761	4291056	42.93%	4.387%
36	23.757	3505	3514	3521	rBV	4610224	9575590	95.79%	9.790%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015928.D
Acq On : 18 Aug 2021 09:34
Operator : CG/JU
Sample : PB138421BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK421

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Title : SVOA CALIBRATION

37	23.910	3532	3540	3548	rVB	2007725	4096959	40.98%	4.188%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 97814582

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015928.D
Acq On : 18 Aug 2021 09:34
Operator : CG/JU
Sample : PB138421BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK421

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

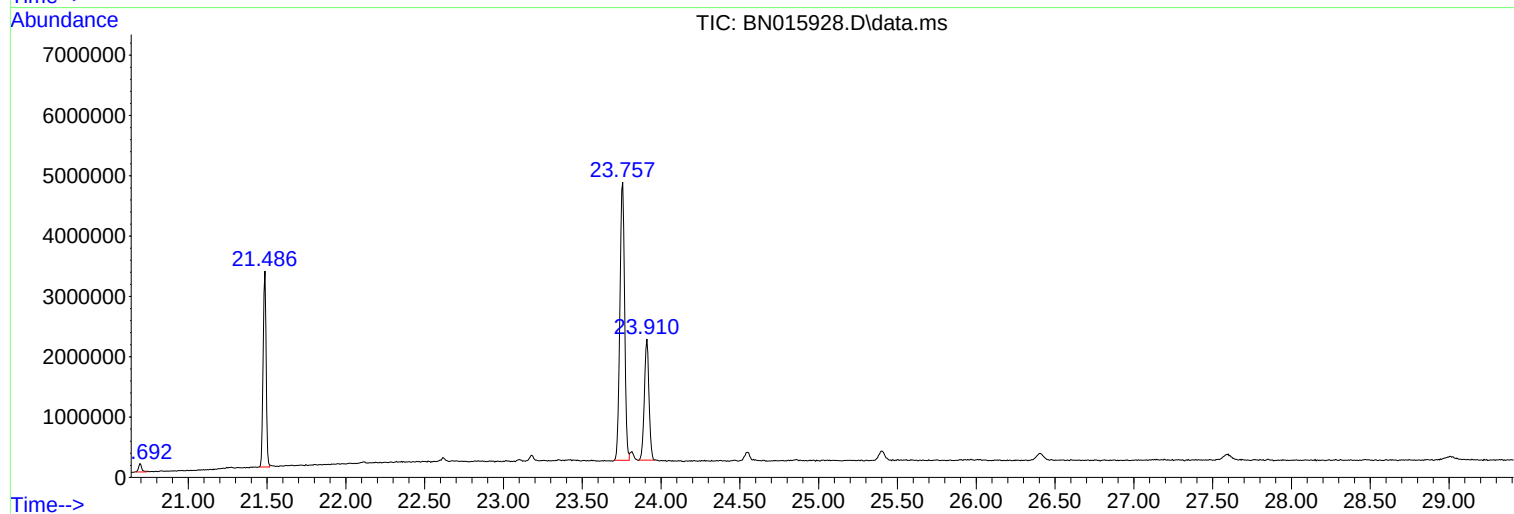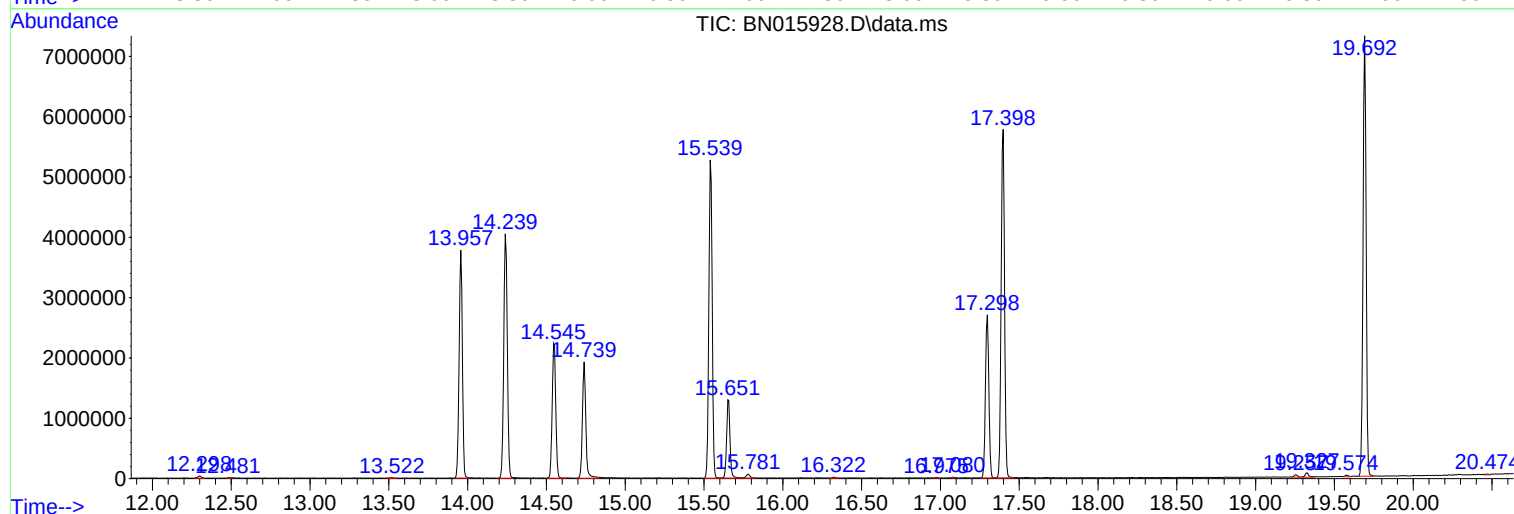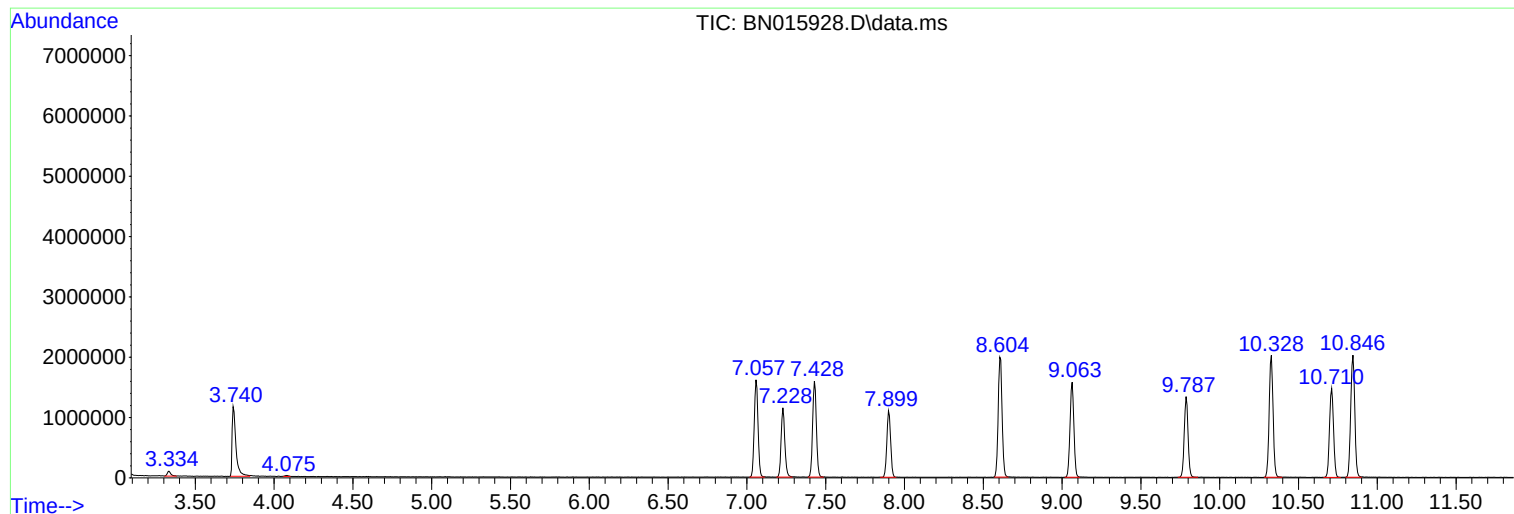

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015928.D
Acq On : 18 Aug 2021 09:34
Operator : CG/JU
Sample : PB138421BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK421

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015928.D
Acq On : 18 Aug 2021 09:34
Operator : CG/JU
Sample : PB138421BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK421

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
