

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015933.D
 Acq On : 18 Aug 2021 12:36
 Operator : CG/JU
 Sample : M3364-20
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015933.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	37	42	51	rVB	81455	131267	1.69%	0.166%
2	3.752	109	113	121	rBV	205806	343289	4.41%	0.433%
3	3.987	148	153	162	rVB3	25700	53992	0.69%	0.068%
4	4.081	165	169	177	rVB2	21299	36119	0.46%	0.046%
5	4.252	192	198	203	rVB8	8590	17209	0.22%	0.022%
6	7.057	668	675	683	rBV	323413	540509	6.94%	0.681%
7	7.228	697	704	713	rBV	888446	1516927	19.47%	1.913%
8	7.428	731	738	749	rBV	1023647	1718455	22.06%	2.167%
9	7.899	811	818	826	rBV	1094045	1900119	24.39%	2.396%
10	7.969	826	830	836	rVB2	23167	37359	0.48%	0.047%
11	8.604	931	938	947	rBV	852284	1477924	18.97%	1.863%
12	9.063	1009	1016	1026	rBV	1222977	2059700	26.44%	2.597%
13	9.263	1043	1050	1057	rVB6	14629	37361	0.48%	0.047%
14	9.787	1131	1139	1148	rBV	957432	1673048	21.48%	2.109%
15	9.922	1157	1162	1167	rBV5	13223	27987	0.36%	0.035%
16	10.010	1171	1177	1178	rVV4	9940	17208	0.22%	0.022%
17	10.110	1187	1194	1201	rBV6	21793	43866	0.56%	0.055%
18	10.328	1224	1231	1245	rBV	1458327	2541273	32.62%	3.204%
19	10.481	1251	1257	1267	rBV	427089	738499	9.48%	0.931%
20	10.710	1288	1296	1303	rBV	1518744	2652017	34.04%	3.344%
21	10.769	1303	1306	1311	rVB5	21460	28617	0.37%	0.036%
22	10.846	1311	1319	1327	rBV	1315201	2376802	30.51%	2.997%
23	10.957	1334	1338	1342	rBV5	14663	22165	0.28%	0.028%
24	11.063	1352	1356	1361	rBV6	10143	18388	0.24%	0.023%
25	11.375	1402	1409	1415	rBV10	11807	26249	0.34%	0.033%
26	11.498	1423	1430	1434	rBV8	14525	31169	0.40%	0.039%
27	12.269	1556	1561	1562	rBV2	22563	30025	0.39%	0.038%
28	12.298	1564	1566	1572	rVB2	22261	29870	0.38%	0.038%
29	12.569	1607	1612	1617	rVB5	16074	30277	0.39%	0.038%
30	12.881	1662	1665	1673	rBV9	20306	46921	0.60%	0.059%
31	13.063	1691	1696	1702	rVV6	22093	40878	0.52%	0.052%
32	13.151	1705	1711	1720	rVB10	18804	46456	0.60%	0.059%
33	13.392	1746	1752	1758	rVV	144241	228642	2.94%	0.288%
34	13.457	1759	1763	1768	rVB6	12166	20487	0.26%	0.026%
35	13.598	1783	1787	1794	rVB6	30596	63885	0.82%	0.081%
36	13.687	1797	1802	1805	rBV5	11296	15519	0.20%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015933.D
 Acq On : 18 Aug 2021 12:36
 Operator : CG/JU
 Sample : M3364-20
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKC7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

37	13.957	1841	1848	1859	rBV	2976443	4335813	55.66%	5.467%
38	14.092	1869	1871	1876	rBV5	16817	30778	0.40%	0.039%
39	14.139	1876	1879	1885	rVB7	15458	24670	0.32%	0.031%
40	14.239	1889	1896	1908	rVB	3099181	4743884	60.90%	5.981%
41	14.504	1936	1941	1942	rVV4	24800	28469	0.37%	0.036%
42	14.545	1942	1948	1955	rVV	2221573	3482301	44.70%	4.391%
43	14.610	1955	1959	1964	rVB	144823	212407	2.73%	0.268%
44	14.663	1964	1968	1972	rBV6	13298	17032	0.22%	0.021%
45	14.739	1973	1981	1990	rBV	291953	480251	6.17%	0.606%
46	14.863	1996	2002	2007	rBV	48484	80596	1.03%	0.102%
47	15.169	2050	2054	2064	rVB	18856	47958	0.62%	0.060%
48	15.263	2064	2070	2072	rBV6	14850	27040	0.35%	0.034%
49	15.345	2079	2084	2088	rBV7	10853	21474	0.28%	0.027%
50	15.539	2110	2117	2131	rVV	3923625	6067727	77.89%	7.650%
51	15.651	2131	2136	2144	rVV	1088347	1639106	21.04%	2.067%
52	15.716	2145	2147	2149	rVV3	26966	32726	0.42%	0.041%
53	15.757	2151	2154	2155	rVV2	43742	57534	0.74%	0.073%
54	15.781	2156	2158	2165	rVB3	65641	89197	1.15%	0.112%
55	15.851	2165	2170	2174	rBV6	25795	48501	0.62%	0.061%
56	15.992	2190	2194	2197	rVV5	54259	92094	1.18%	0.116%
57	16.028	2197	2200	2208	rVB2	105066	184872	2.37%	0.233%
58	16.228	2230	2234	2237	rBV6	15090	19989	0.26%	0.025%
59	16.298	2243	2246	2249	rVB3	25648	35238	0.45%	0.044%
60	16.392	2257	2262	2267	rBV4	45738	85808	1.10%	0.108%
61	16.445	2267	2271	2278	rVV9	28634	60636	0.78%	0.076%
62	16.504	2278	2281	2284	rVV5	12073	18584	0.24%	0.023%
63	16.557	2286	2290	2295	rVV7	43055	88896	1.14%	0.112%
64	16.598	2295	2297	2302	rVB3	35038	47389	0.61%	0.060%
65	16.669	2304	2309	2312	rBV7	17942	35932	0.46%	0.045%
66	16.839	2334	2338	2340	rBV5	12671	16506	0.21%	0.021%
67	17.080	2373	2379	2383	rBV6	19620	36432	0.47%	0.046%
68	17.192	2393	2398	2400	rVV3	41118	61759	0.79%	0.078%
69	17.216	2400	2402	2405	rVV3	29225	34808	0.45%	0.044%
70	17.251	2405	2408	2410	rVV3	49248	56829	0.73%	0.072%
71	17.298	2410	2416	2422	rVV	2680185	3885876	49.88%	4.899%
72	17.398	2426	2433	2443	rVV2	4429842	6711237	86.15%	8.462%
73	17.669	2475	2479	2481	rBV5	13347	21725	0.28%	0.027%
74	17.698	2481	2484	2490	rVB8	33919	50739	0.65%	0.064%
75	17.975	2524	2531	2534	rVV4	82708	154874	1.99%	0.195%
76	18.004	2534	2536	2540	rVB2	45286	56694	0.73%	0.071%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015933.D
 Acq On : 18 Aug 2021 12:36
 Operator : CG/JU
 Sample : M3364-20
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKC7

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

77	18.098	2548	2552	2556	rBV6	45935	68206	0.88%	0.086%
78	18.133	2556	2558	2563	rVB	48630	61613	0.79%	0.078%
79	18.198	2565	2569	2575	rBV7	65145	109914	1.41%	0.139%
80	18.269	2578	2581	2585	rVB4	23036	31429	0.40%	0.040%
81	18.369	2593	2598	2603	rBV3	66115	117962	1.51%	0.149%
82	18.451	2608	2612	2617	rBV	47866	75579	0.97%	0.095%
83	18.492	2617	2619	2621	rBV3	20789	25002	0.32%	0.032%
84	18.563	2627	2631	2634	rBV6	23759	36522	0.47%	0.046%
85	18.669	2645	2649	2653	rVB5	45124	65270	0.84%	0.082%
86	18.769	2663	2666	2672	rBV7	36835	52387	0.67%	0.066%
87	18.886	2683	2686	2691	rVB5	36285	37417	0.48%	0.047%
88	18.998	2702	2705	2710	rVB7	41912	49347	0.63%	0.062%
89	19.257	2745	2749	2756	rBV9	37714	80180	1.03%	0.101%
90	19.322	2756	2760	2763	rBV	62493	88181	1.13%	0.111%
91	19.569	2800	2802	2807	rVB3	43870	64642	0.83%	0.082%
92	19.692	2816	2823	2834	rBV2	5523250	7789830	100.00%	9.822%
93	20.098	2888	2892	2897	rVB	95048	135234	1.74%	0.171%
94	20.157	2898	2902	2906	rBV	101582	143252	1.84%	0.181%
95	20.692	2989	2993	2997	rBV	235550	298228	3.83%	0.376%
96	20.769	3003	3006	3009	rBV2	57601	73337	0.94%	0.092%
97	21.198	3075	3079	3085	rBV2	205481	360692	4.63%	0.455%
98	21.486	3122	3128	3134	rBV	3188117	4159177	53.39%	5.244%
99	23.757	3505	3514	3522	rBV2	3637856	7422971	95.29%	9.359%
100	23.910	3532	3540	3550	rVB2	1951901	4121115	52.90%	5.196%


Sum of corrected areas: 79312346

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015933.D
Acq On : 18 Aug 2021 12:36
Operator : CG/JU
Sample : M3364-20
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

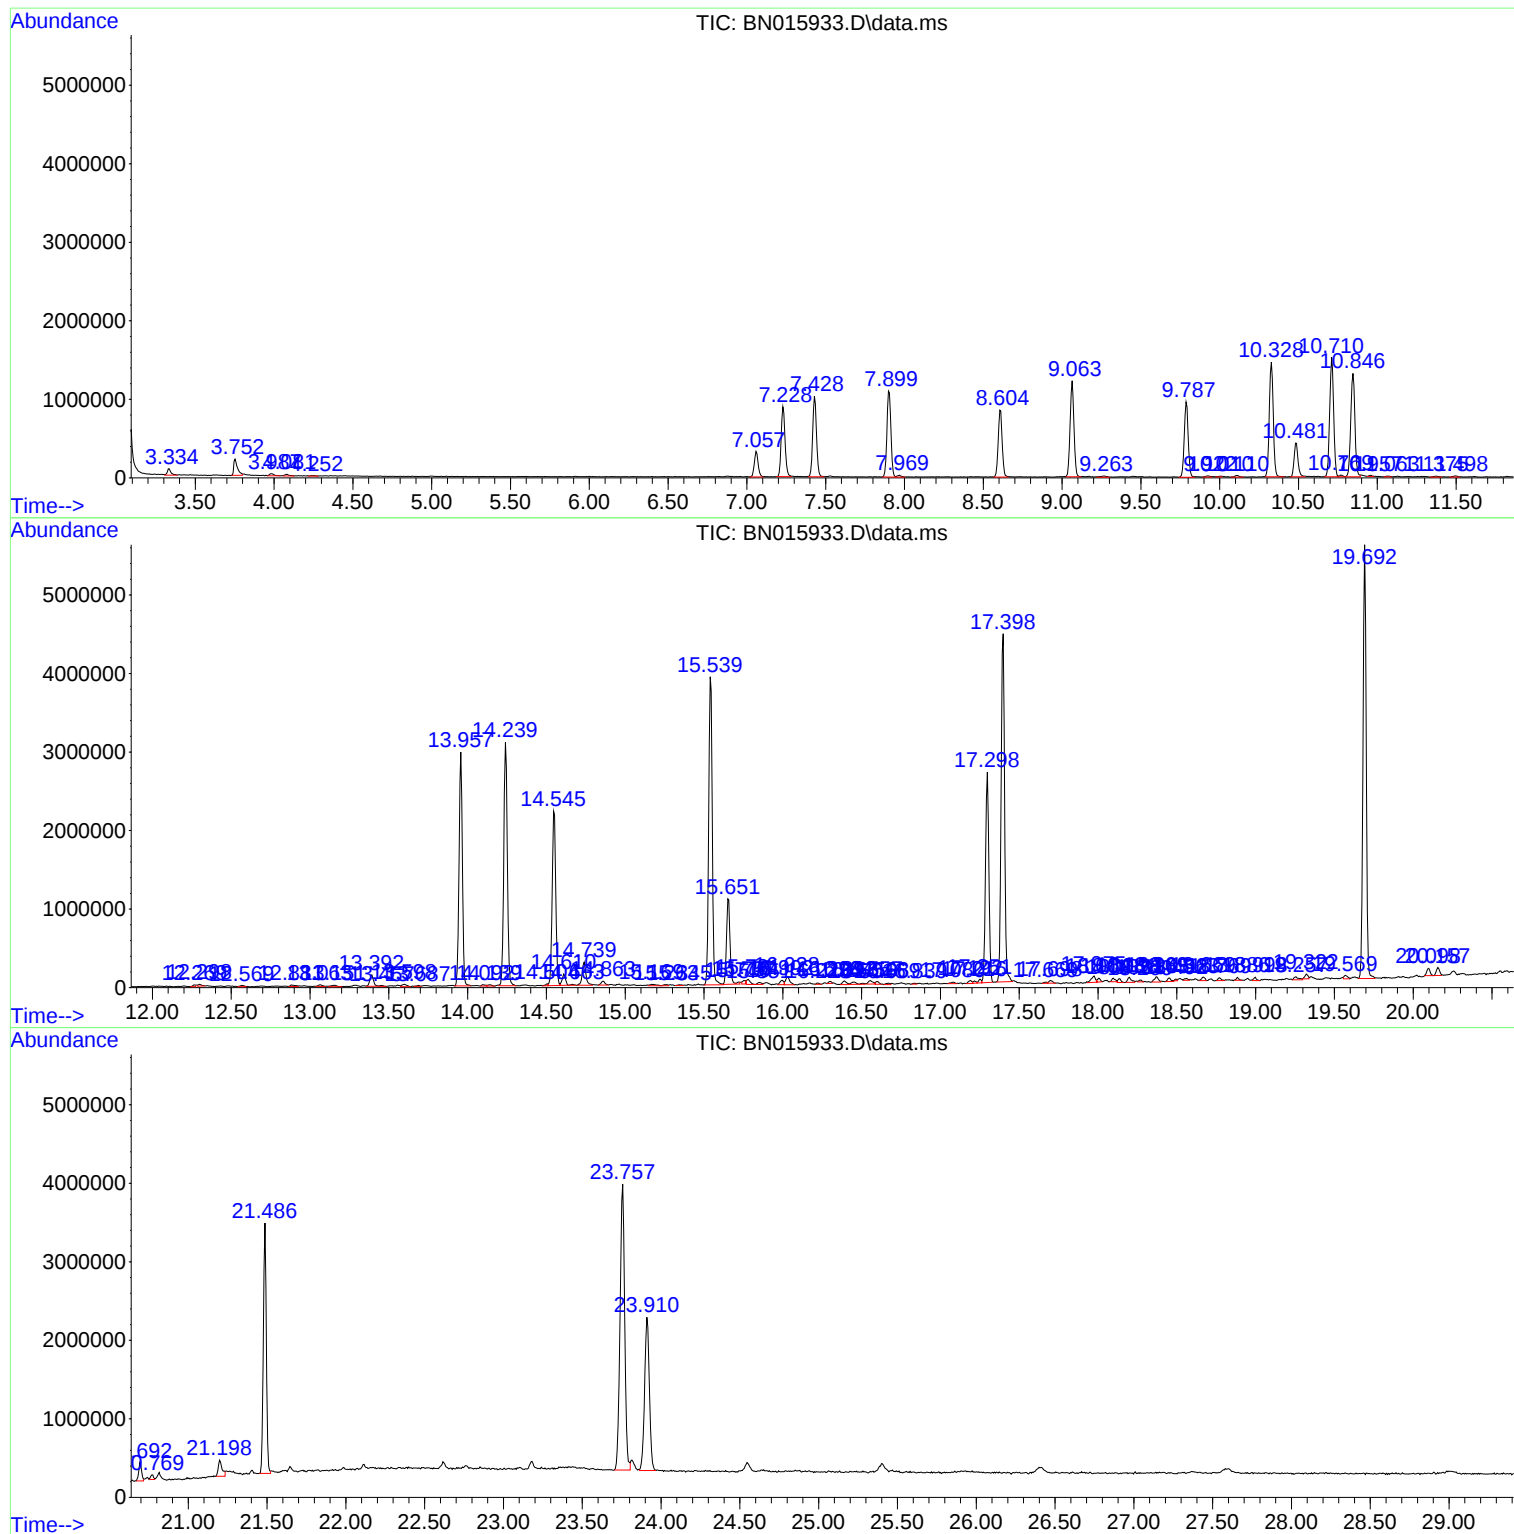

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015933.D
Acq On : 18 Aug 2021 12:36
Operator : CG/JU
Sample : M3364-20
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKC7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.481	5.57 ng/ul	738499	Naphthalene-d8	10.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83
3			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83
4			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	72
5			Ethanol, 2-[2-(2-methylpropoxy)e...	162	C8H18O3	018912-80-6	72

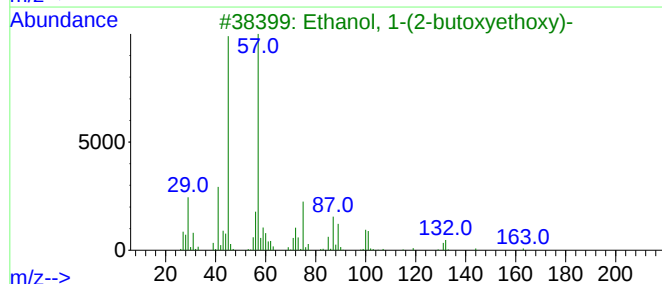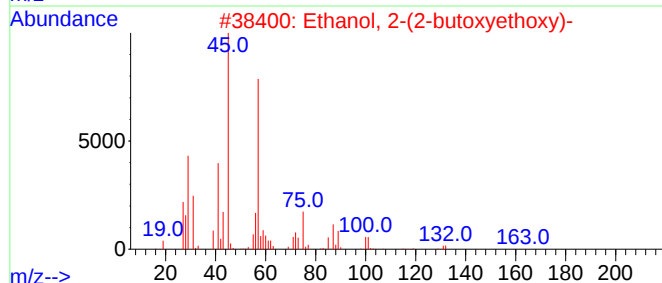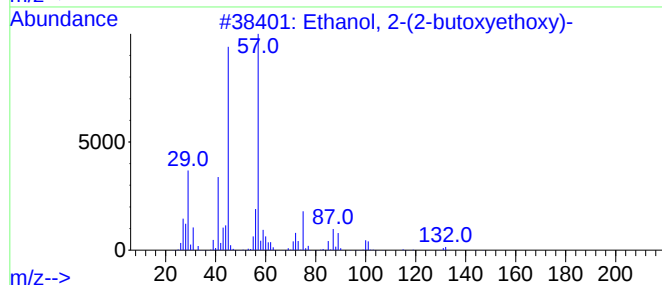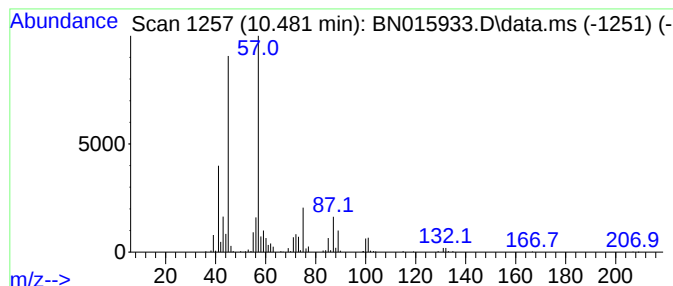

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015933.D
Acq On : 18 Aug 2021 12:36
Operator : CG/JU
Sample : M3364-20
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.481	5.6	ng/u1	738499	2	10.710	2652020	20.0