

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015937.D
 Acq On : 18 Aug 2021 15:03
 Operator : CG/JU
 Sample : M3362-01
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JMXD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015937.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	39	42	51	rVB4	25174	46141	1.26%	0.115%
2	3.675	96	100	105	rBV7	6213	9419	0.26%	0.023%
3	3.752	111	113	124	rBV	142776	261834	7.18%	0.651%
4	3.987	147	153	158	rBV3	29610	55602	1.52%	0.138%
5	4.075	165	168	172	rVB2	10502	16764	0.46%	0.042%
6	4.158	179	182	185	rBV3	3812	6973	0.19%	0.017%
7	4.452	227	232	237	rVB7	6601	12490	0.34%	0.031%
8	4.993	320	324	329	rBV3	12407	16810	0.46%	0.042%
9	5.628	430	432	436	rBV4	5455	7069	0.19%	0.018%
10	5.987	491	493	498	rVB5	5467	8476	0.23%	0.021%
11	7.057	667	675	685	rBV	430500	740532	20.30%	1.840%
12	7.228	698	704	714	rBV	312258	524457	14.38%	1.303%
13	7.428	732	738	749	rVB	443441	748608	20.52%	1.860%
14	7.528	751	755	760	rBV5	9489	16005	0.44%	0.040%
15	7.904	812	819	826	rBV	910332	1546901	42.40%	3.843%
16	7.957	827	828	833	rVV5	5512	6706	0.18%	0.017%
17	8.134	855	858	862	rVV6	4905	6398	0.18%	0.016%
18	8.269	876	881	885	rVB6	5586	8872	0.24%	0.022%
19	8.604	930	938	947	rBV	524562	905785	24.83%	2.250%
20	8.728	955	959	965	rVB4	11855	18967	0.52%	0.047%
21	9.063	1006	1016	1026	rBV	431343	732533	20.08%	1.820%
22	9.169	1030	1034	1040	rBV7	4921	10970	0.30%	0.027%
23	9.481	1085	1087	1090	rBV4	4388	5997	0.16%	0.015%
24	9.787	1131	1139	1146	rBV	319970	557232	15.27%	1.384%
25	10.328	1224	1231	1239	rBV	531956	894693	24.53%	2.223%
26	10.481	1251	1257	1272	rBV	193788	374667	10.27%	0.931%
27	10.710	1286	1296	1304	rBV	1227360	2203571	60.40%	5.475%
28	10.846	1312	1319	1329	rBV	521224	917899	25.16%	2.280%
29	11.504	1429	1431	1434	rVV3	4821	6361	0.17%	0.016%
30	11.751	1467	1473	1476	rVV4	6790	9866	0.27%	0.025%
31	12.304	1562	1567	1571	rVB6	9349	13965	0.38%	0.035%
32	12.910	1665	1670	1675	rBV5	6707	13526	0.37%	0.034%
33	13.098	1697	1702	1704	rVV5	9235	13900	0.38%	0.035%
34	13.163	1708	1713	1717	rVB6	9902	16422	0.45%	0.041%
35	13.381	1747	1750	1753	rBV3	5713	6053	0.17%	0.015%
36	13.445	1757	1761	1762	rBV3	5858	6786	0.19%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015937.D
 Acq On : 18 Aug 2021 15:03
 Operator : CG/JU
 Sample : M3362-01
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JMXD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

37	13.875	1831	1834	1837	rVV4	8759	12129	0.33%	0.030%
38	13.957	1841	1848	1858	rVV	949306	1406241	38.55%	3.494%
39	14.039	1858	1862	1864	rVV4	8521	10893	0.30%	0.027%
40	14.098	1870	1872	1875	rBV4	4735	6299	0.17%	0.016%
41	14.239	1890	1896	1906	rVB	1028105	1581211	43.34%	3.928%
42	14.451	1927	1932	1937	rBV6	5833	9031	0.25%	0.022%
43	14.551	1941	1949	1955	rBV	1875667	2942143	80.65%	7.310%
44	14.610	1955	1959	1965	rVB	153503	236675	6.49%	0.588%
45	14.739	1974	1981	1996	rBV	276285	503007	13.79%	1.250%
46	14.963	2013	2019	2027	rBV10	19100	36141	0.99%	0.090%
47	15.539	2109	2117	2123	rBV	1381771	2040314	55.93%	5.069%
48	15.592	2123	2126	2131	rVV	64361	96870	2.66%	0.241%
49	15.651	2131	2136	2146	rVV	242280	357834	9.81%	0.889%
50	15.763	2152	2155	2156	rBV2	16204	18276	0.50%	0.045%
51	15.810	2160	2163	2167	rVV3	28102	37942	1.04%	0.094%
52	15.845	2167	2169	2172	rVB4	9048	9995	0.27%	0.025%
53	15.898	2172	2178	2183	rBV7	11550	22581	0.62%	0.056%
54	15.981	2190	2192	2193	rBV2	7348	6238	0.17%	0.015%
55	15.992	2193	2194	2197	rVB2	9067	6011	0.16%	0.015%
56	16.292	2240	2245	2249	rVB2	35755	50786	1.39%	0.126%
57	16.328	2249	2251	2255	rVV5	5303	6924	0.19%	0.017%
58	16.392	2258	2262	2266	rBV5	13307	22428	0.61%	0.056%
59	16.439	2269	2270	2273	rVB3	8863	7601	0.21%	0.019%
60	16.551	2286	2289	2291	rBV4	5000	6230	0.17%	0.015%
61	16.604	2293	2298	2301	rVV5	9573	16879	0.46%	0.042%
62	16.645	2301	2305	2311	rVV9	7483	16064	0.44%	0.040%
63	16.869	2341	2343	2346	rVB3	7841	9570	0.26%	0.024%
64	16.904	2346	2349	2350	rBV3	6344	5999	0.16%	0.015%
65	17.057	2372	2375	2377	rVV4	7052	10278	0.28%	0.026%
66	17.080	2377	2379	2381	rVV2	9986	11197	0.31%	0.028%
67	17.116	2381	2385	2390	rVB2	38542	57212	1.57%	0.142%
68	17.298	2408	2416	2420	rBV	2272110	3392137	92.98%	8.428%
69	17.339	2420	2423	2427	rVV	306484	435678	11.94%	1.082%
70	17.392	2427	2432	2442	rVV	1468036	2289773	62.77%	5.689%
71	17.486	2445	2448	2453	rVB6	23702	32504	0.89%	0.081%
72	17.586	2461	2465	2467	rVB5	5847	7384	0.20%	0.018%
73	17.669	2477	2479	2481	rBV3	7580	7074	0.19%	0.018%
74	17.716	2484	2487	2488	rBV3	6960	8164	0.22%	0.020%
75	17.810	2501	2503	2506	rBV5	6107	8728	0.24%	0.022%
76	17.975	2525	2531	2538	rBV2	54181	82666	2.27%	0.205%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015937.D
 Acq On : 18 Aug 2021 15:03
 Operator : CG/JU
 Sample : M3362-01
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JMXD6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

77	18.045	2540	2543	2548	rVB7	5837	10444	0.29%	0.026%
78	18.139	2556	2559	2562	rBV5	7429	6184	0.17%	0.015%
79	18.169	2562	2564	2565	rBV2	16400	12904	0.35%	0.032%
80	18.222	2570	2573	2578	rVB3	16495	23716	0.65%	0.059%
81	18.269	2578	2581	2583	rVB4	8000	8118	0.22%	0.020%
82	18.369	2593	2598	2603	rBV3	33592	61663	1.69%	0.153%
83	18.498	2619	2620	2623	rBV3	6815	9068	0.25%	0.023%
84	18.663	2645	2648	2649	rBV3	7490	7635	0.21%	0.019%
85	18.974	2695	2701	2702	rBV6	10618	20291	0.56%	0.050%
86	19.092	2719	2721	2724	rVV4	7524	6066	0.17%	0.015%
87	19.145	2727	2730	2735	rVB7	23704	34049	0.93%	0.085%
88	19.251	2743	2748	2752	rBV8	14252	24572	0.67%	0.061%
89	19.357	2762	2766	2771	rVB	135442	188142	5.16%	0.467%
90	19.692	2817	2823	2833	rBV	1967708	2821741	77.35%	7.010%
91	19.921	2859	2862	2868	rVB	40863	46309	1.27%	0.115%
92	20.139	2894	2899	2905	rBV2	254947	341638	9.36%	0.849%
93	20.216	2910	2912	2915	rVB2	21873	19583	0.54%	0.049%
94	20.316	2926	2929	2932	rBV5	27373	33983	0.93%	0.084%
95	20.698	2990	2994	2998	rBV	187594	241906	6.63%	0.601%
96	21.198	3076	3079	3085	rBV4	81855	135208	3.71%	0.336%
97	21.486	3122	3128	3133	rBV	2810983	3648070	100.00%	9.063%
98	23.174	3413	3415	3421	rVB3	105359	173296	4.75%	0.431%
99	23.751	3506	3513	3520	rBV	1016245	2228117	61.08%	5.536%
100	23.910	3533	3540	3552	rVB2	1680343	3573535	97.96%	8.878%

Sum of corrected areas: 40250595




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015937.D
Acq On : 18 Aug 2021 15:03
Operator : CG/JU
Sample : M3362-01
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JMXD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

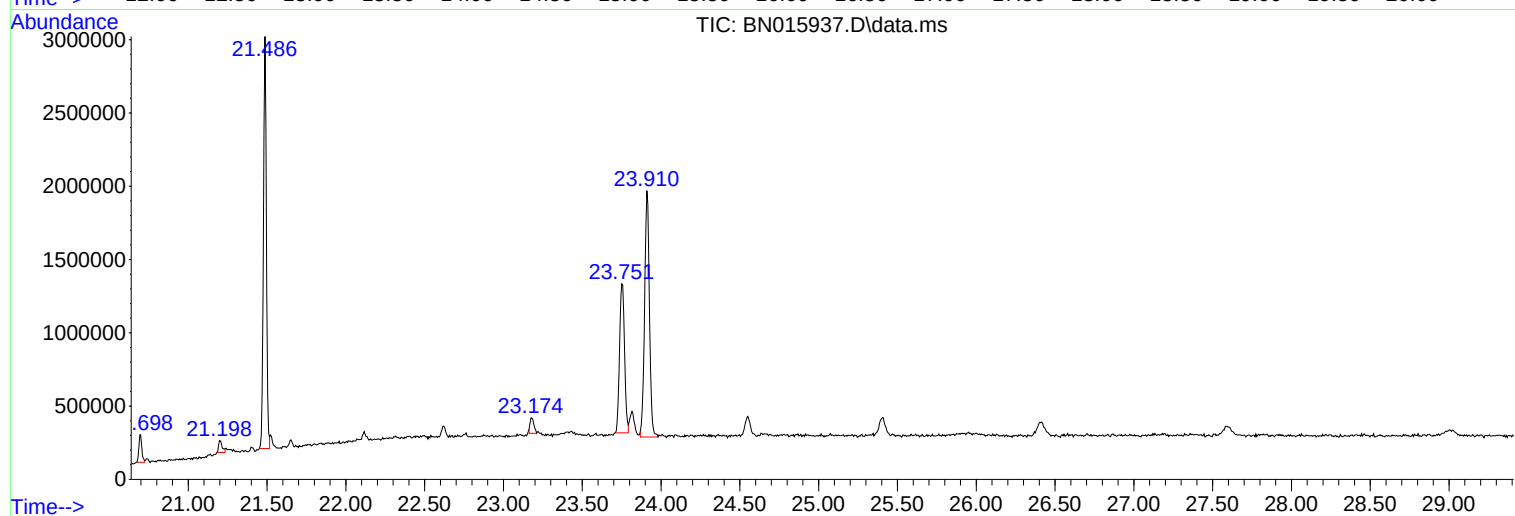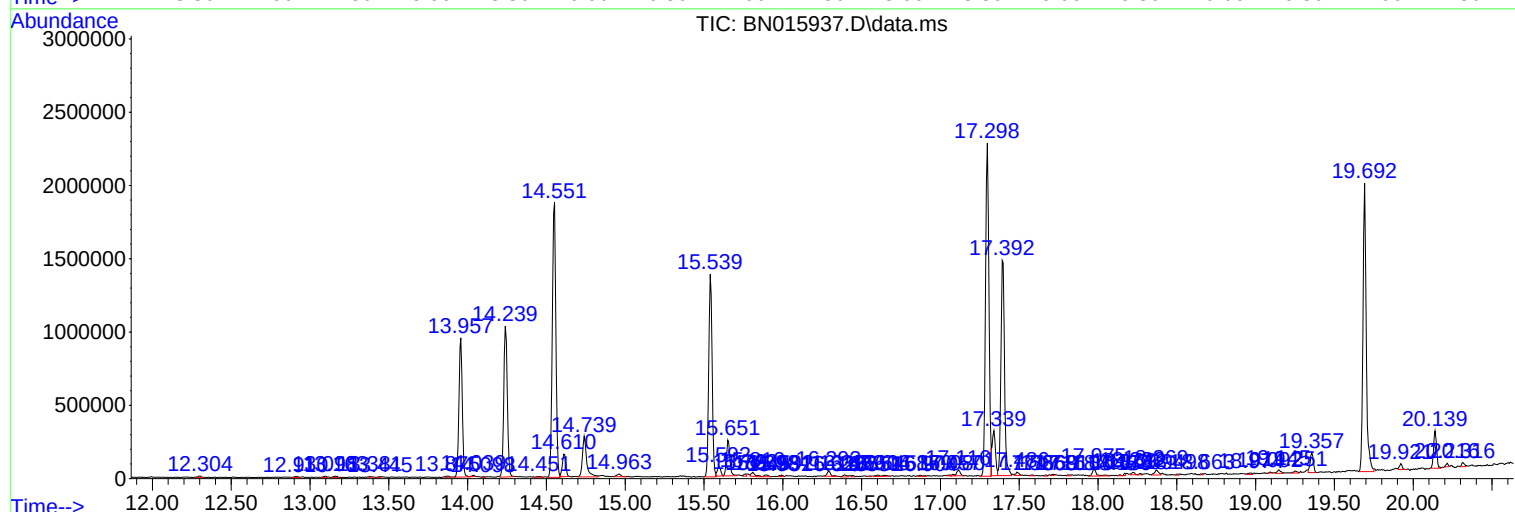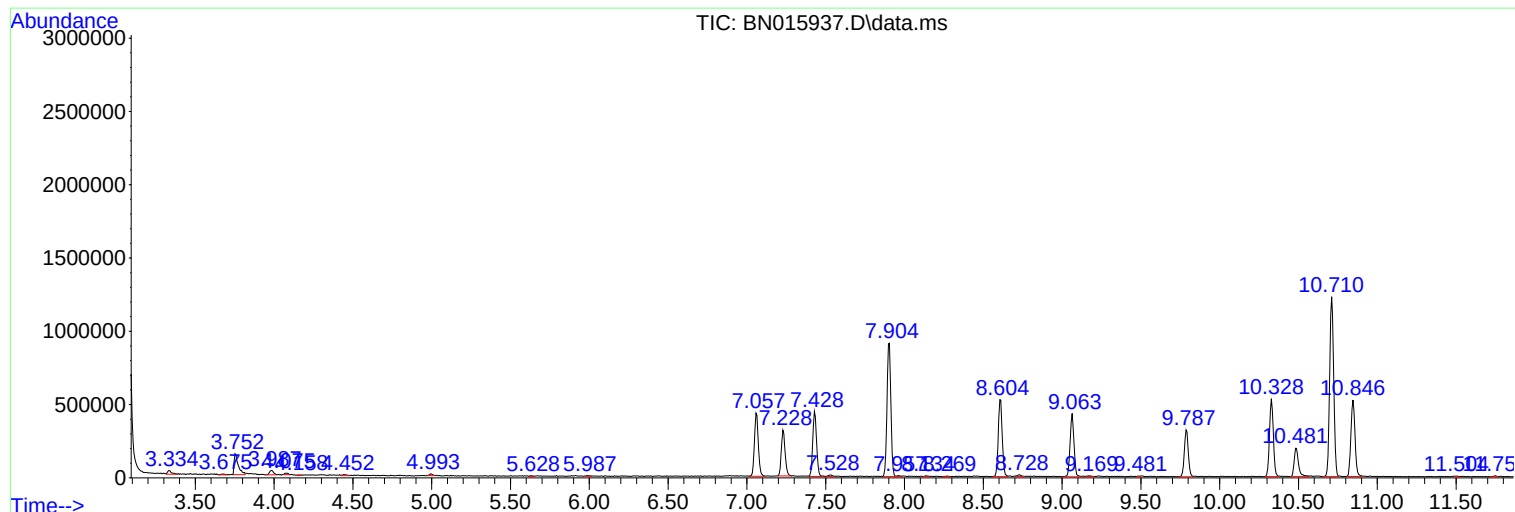

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015937.D
Acq On : 18 Aug 2021 15:03
Operator : CG/JU
Sample : M3362-01
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JMXD6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.481	3.40 ng/ul	374667	Naphthalene-d8	10.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	86
4			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83

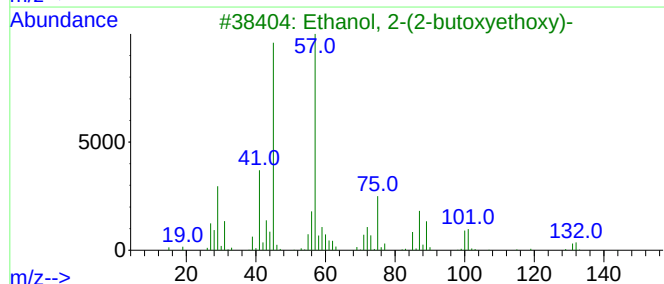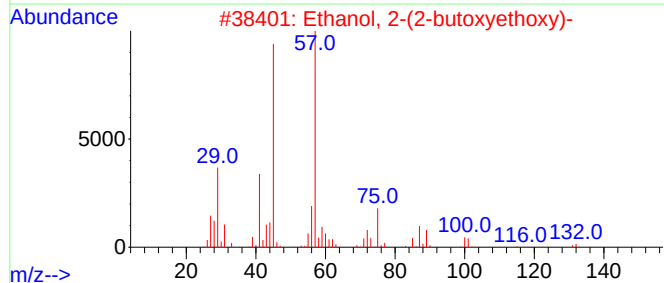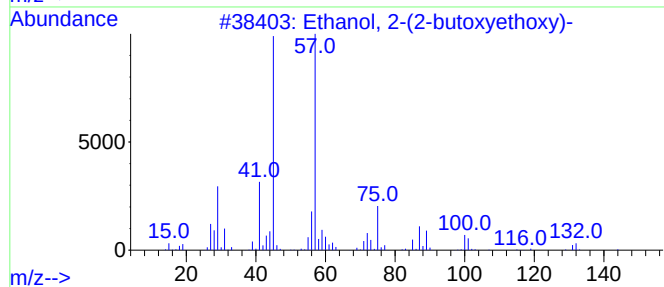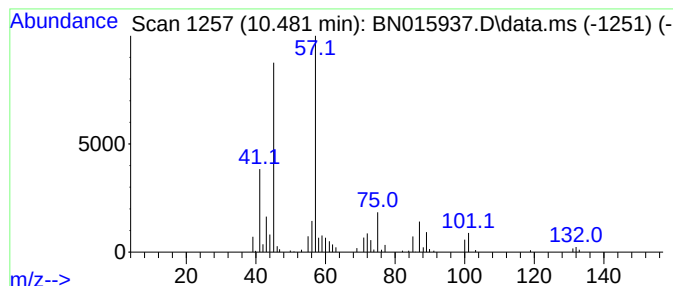

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015937.D
Acq On : 18 Aug 2021 15:03
Operator : CG/JU
Sample : M3362-01
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JMXD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.481	3.4	ng/u1	374667	2	10.710	2203570	20.0