

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015941.D
 Acq On : 18 Aug 2021 17:30
 Operator : CG/JU
 Sample : PB138486BL
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK486

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015941.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	38	42	49	rBV2	63765	95200	1.39%	0.134%
2	3.746	109	112	126	rBV	862379	1460271	21.39%	2.059%
3	4.081	166	169	174	rVB	15297	20970	0.31%	0.030%
4	7.057	668	675	686	rBV	1183254	1971177	28.87%	2.779%
5	7.228	698	704	716	rBV	833046	1416004	20.74%	1.996%
6	7.428	731	738	747	rBV	1168385	1983124	29.04%	2.796%
7	7.899	809	818	826	rBV	894092	1522481	22.30%	2.146%
8	8.610	931	939	947	rBV	1436257	2413601	35.35%	3.403%
9	8.734	954	960	964	rVB7	3783	8813	0.13%	0.012%
10	9.063	1008	1016	1027	rVV	1121918	1925926	28.21%	2.715%
11	9.787	1131	1139	1149	rBV	924679	1594106	23.35%	2.247%
12	10.328	1223	1231	1244	rBV	1404485	2468664	36.15%	3.480%
13	10.710	1289	1296	1304	rBV	1257367	2150476	31.49%	3.032%
14	10.845	1311	1319	1328	rBV	1408043	2492802	36.51%	3.514%
15	12.304	1562	1567	1573	rVB	24688	43933	0.64%	0.062%
16	13.957	1842	1848	1858	rBV	2663360	3742045	54.80%	5.276%
17	14.239	1888	1896	1904	rBV	2700641	4237339	62.06%	5.974%
18	14.551	1941	1949	1957	rBV	1844601	2882588	42.22%	4.064%
19	14.739	1974	1981	2004	rBV	1177757	1837153	26.91%	2.590%
20	15.539	2110	2117	2125	rBV	3583764	5259519	77.03%	7.415%
21	15.651	2131	2136	2144	rBV	837472	1219487	17.86%	1.719%
22	15.780	2152	2158	2163	rVB4	43193	70313	1.03%	0.099%
23	16.116	2210	2215	2219	rBV4	5228	8489	0.12%	0.012%
24	16.322	2246	2250	2257	rBV9	8350	14217	0.21%	0.020%
25	17.080	2375	2379	2385	rBV5	10090	17749	0.26%	0.025%
26	17.298	2409	2416	2425	rBV	2247513	3337753	48.88%	4.706%
27	17.398	2425	2433	2444	rVV	3983116	5988099	87.70%	8.442%
28	17.545	2455	2458	2463	rVB6	6972	9563	0.14%	0.013%
29	18.810	2669	2673	2676	rBV5	5127	6875	0.10%	0.010%
30	19.257	2745	2749	2756	rBV9	25883	44024	0.64%	0.062%
31	19.327	2756	2761	2768	rVV	47777	70073	1.03%	0.099%
32	19.516	2790	2793	2794	rBV2	7400	8951	0.13%	0.013%
33	19.580	2801	2804	2808	rVB	18360	24403	0.36%	0.034%
34	19.692	2816	2823	2838	rVV	4940402	6828222	100.00%	9.626%
35	20.692	2989	2993	3001	rBV	174631	242044	3.54%	0.341%
36	21.404	3111	3114	3118	rVB2	56040	69347	1.02%	0.098%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015941.D
Acq On : 18 Aug 2021 17:30
Operator : CG/JU
Sample : PB138486BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK486

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Title : SVOA CALIBRATION

37	21.486	3122	3128	3136	rVV	2696182	3553134	52.04%	5.009%
38	23.751	3505	3513	3521	rBV	3127346	6509869	95.34%	9.178%
39	23.909	3532	3540	3549	rVB2	1593280	3383636	49.55%	4.770%


Sum of corrected areas: 70932440

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015941.D
Acq On : 18 Aug 2021 17:30
Operator : CG/JU
Sample : PB138486BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK486

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

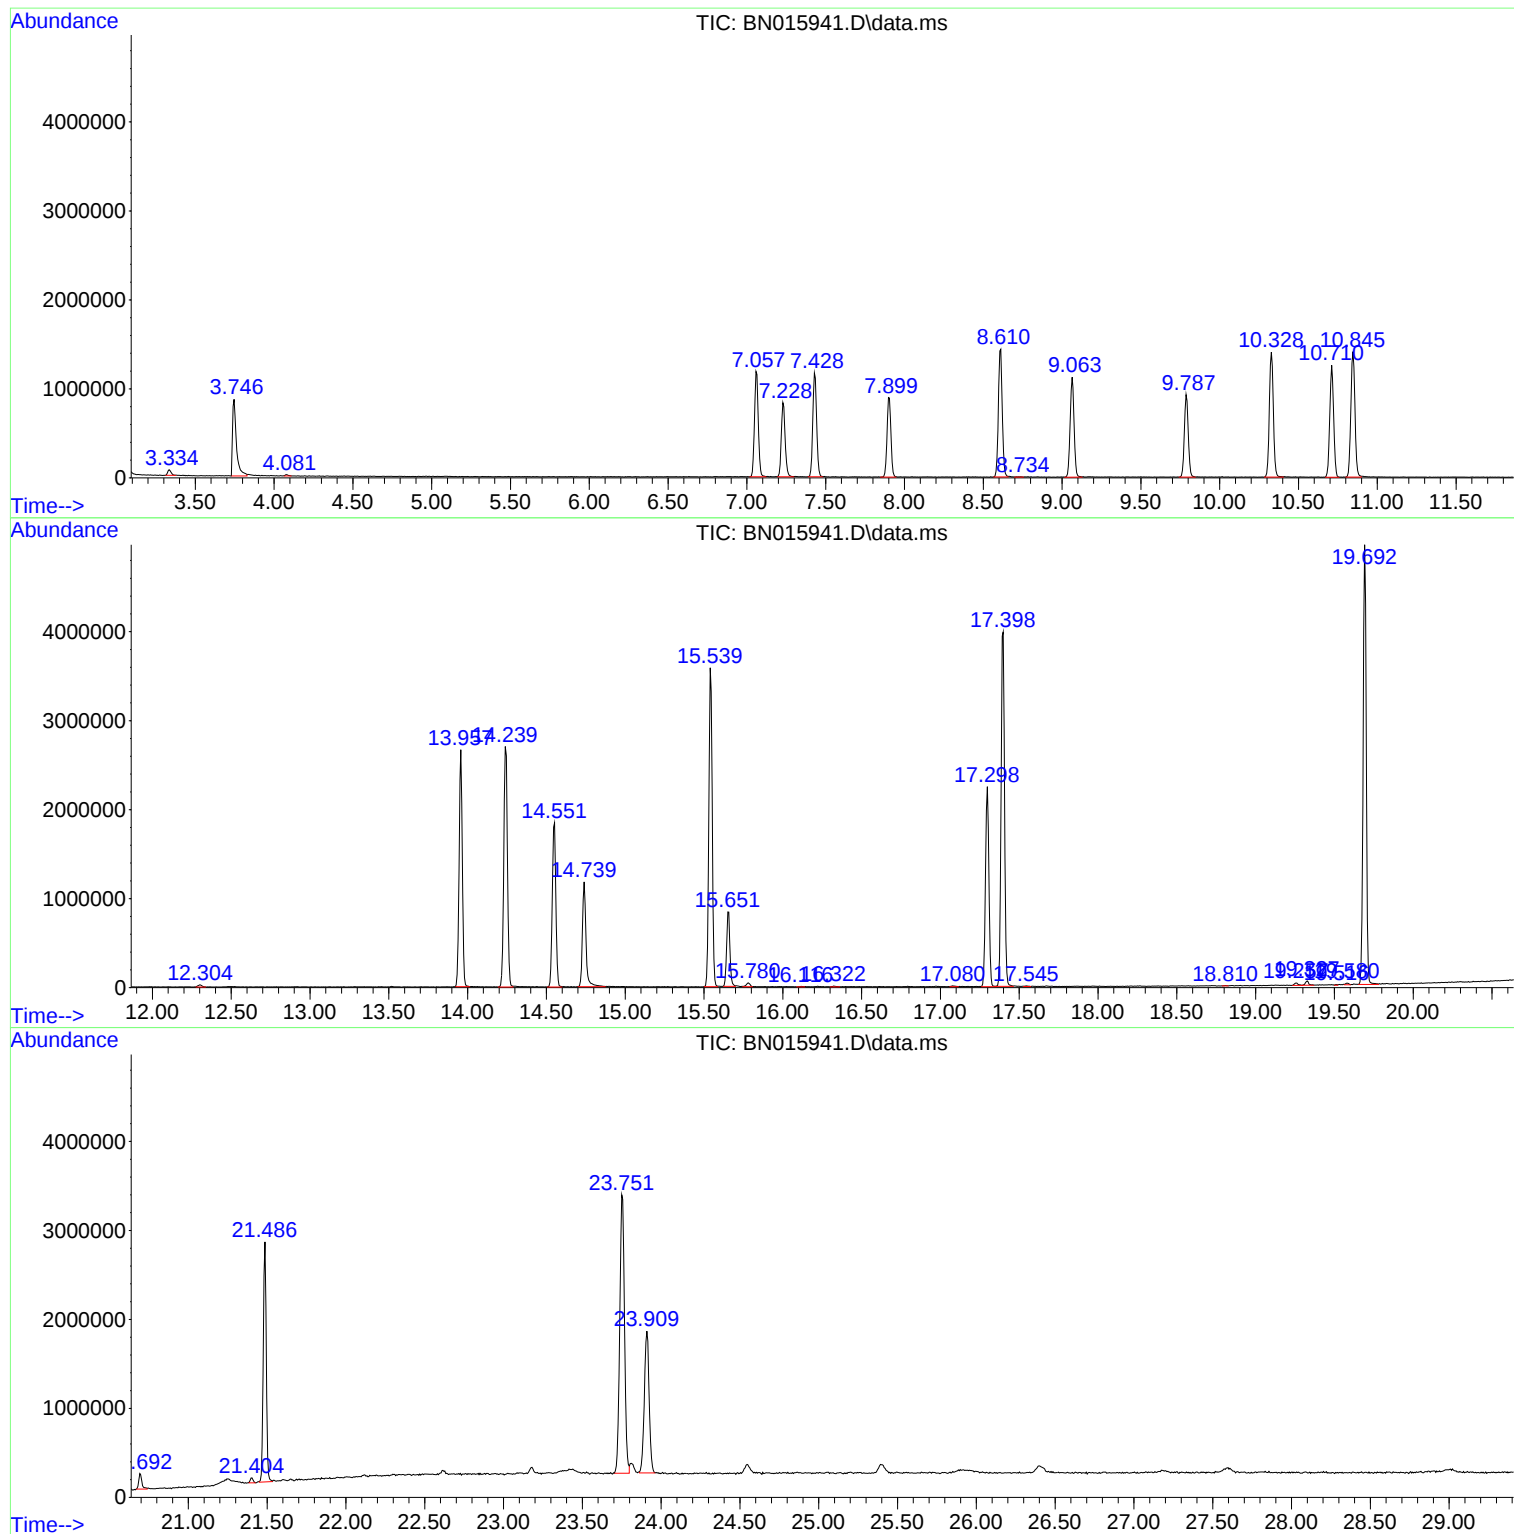

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015941.D
Acq On : 18 Aug 2021 17:30
Operator : CG/JU
Sample : PB138486BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK486

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015941.D
Acq On : 18 Aug 2021 17:30
Operator : CG/JU
Sample : PB138486BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK486

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
