

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015942.D
 Acq On : 18 Aug 2021 18:07
 Operator : CG/JU
 Sample : PB138519BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK519

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015942.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	36	42	49	rVB	66287	104417	1.59%	0.147%
2	3.746	108	112	133	rBV	892848	1563264	23.74%	2.202%
3	4.075	165	168	177	rVB	32539	54202	0.82%	0.076%
4	6.293	541	545	549	rBV4	4634	8905	0.14%	0.013%
5	7.058	668	675	685	rBV	1196447	2010283	30.53%	2.831%
6	7.228	698	704	718	rBV	845934	1444017	21.93%	2.034%
7	7.428	731	738	748	rVB	1220914	2055846	31.22%	2.895%
8	7.899	810	818	829	rBV	881246	1496337	22.72%	2.107%
9	8.605	932	938	950	rBV	1452075	2478137	37.63%	3.490%
10	9.063	1009	1016	1024	rBV	1180416	1980420	30.07%	2.789%
11	9.787	1131	1139	1148	rBV	941863	1657811	25.18%	2.335%
12	10.328	1223	1231	1239	rBV	1471275	2533072	38.47%	3.568%
13	10.710	1288	1296	1306	rBV	1237664	2150220	32.65%	3.028%
14	10.846	1312	1319	1331	rBV	1459908	2555720	38.81%	3.599%
15	12.304	1561	1567	1572	rVB	24183	41058	0.62%	0.058%
16	13.522	1770	1774	1779	rVB6	6295	8844	0.13%	0.012%
17	13.957	1841	1848	1859	rBV	2554974	3703790	56.25%	5.216%
18	14.240	1889	1896	1905	rBV	2791997	4276020	64.94%	6.022%
19	14.551	1942	1949	1956	rBV	1911371	2866352	43.53%	4.037%
20	14.740	1974	1981	1996	rBV	1118021	1766357	26.82%	2.488%
21	14.951	2015	2017	2022	rVB4	4416	6855	0.10%	0.010%
22	15.540	2109	2117	2130	rBV	3502391	5316314	80.73%	7.487%
23	15.657	2130	2137	2148	rVV	791285	1156923	17.57%	1.629%
24	15.781	2153	2158	2165	rVB2	47827	73958	1.12%	0.104%
25	16.328	2247	2251	2256	rVB5	9243	12141	0.18%	0.017%
26	16.981	2359	2362	2364	rVB4	5926	6587	0.10%	0.009%
27	17.081	2375	2379	2386	rBV6	8324	16645	0.25%	0.023%
28	17.298	2408	2416	2424	rBV	2344331	3438910	52.22%	4.843%
29	17.398	2424	2433	2449	rVB	3878746	5792165	87.96%	8.158%
30	17.539	2455	2457	2462	rBV5	6023	9609	0.15%	0.014%
31	18.263	2576	2580	2582	rBV5	6408	7480	0.11%	0.011%
32	18.522	2620	2624	2629	rBV6	14297	23015	0.35%	0.032%
33	18.739	2656	2661	2664	rBV7	6890	10225	0.16%	0.014%
34	18.810	2666	2673	2674	rBV6	6982	11786	0.18%	0.017%
35	19.257	2744	2749	2753	rVB3	27920	41051	0.62%	0.058%
36	19.322	2755	2760	2765	rBV2	46328	66056	1.00%	0.093%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015942.D
 Acq On : 18 Aug 2021 18:07
 Operator : CG/JU
 Sample : PB138519BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK519

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

37	19.580	2800	2804	2807	rBV	20311	28855	0.44%	0.041%
38	19.692	2816	2823	2829	rBV	4821569	6585023	100.00%	9.274%
39	20.033	2877	2881	2885	rBV7	10528	18598	0.28%	0.026%
40	20.228	2912	2914	2917	rBV4	8353	8268	0.13%	0.012%
41	20.692	2989	2993	3001	rBV	172616	229793	3.49%	0.324%
42	21.486	3122	3128	3137	rBV	2711161	3659857	55.58%	5.154%
43	23.751	3505	3513	3522	rBV2	3136117	6262811	95.11%	8.820%
44	23.910	3532	3540	3550	rVB2	1632674	3465293	52.62%	4.880%




Sum of corrected areas: 71003290

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015942.D
Acq On : 18 Aug 2021 18:07
Operator : CG/JU
Sample : PB138519BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK519

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

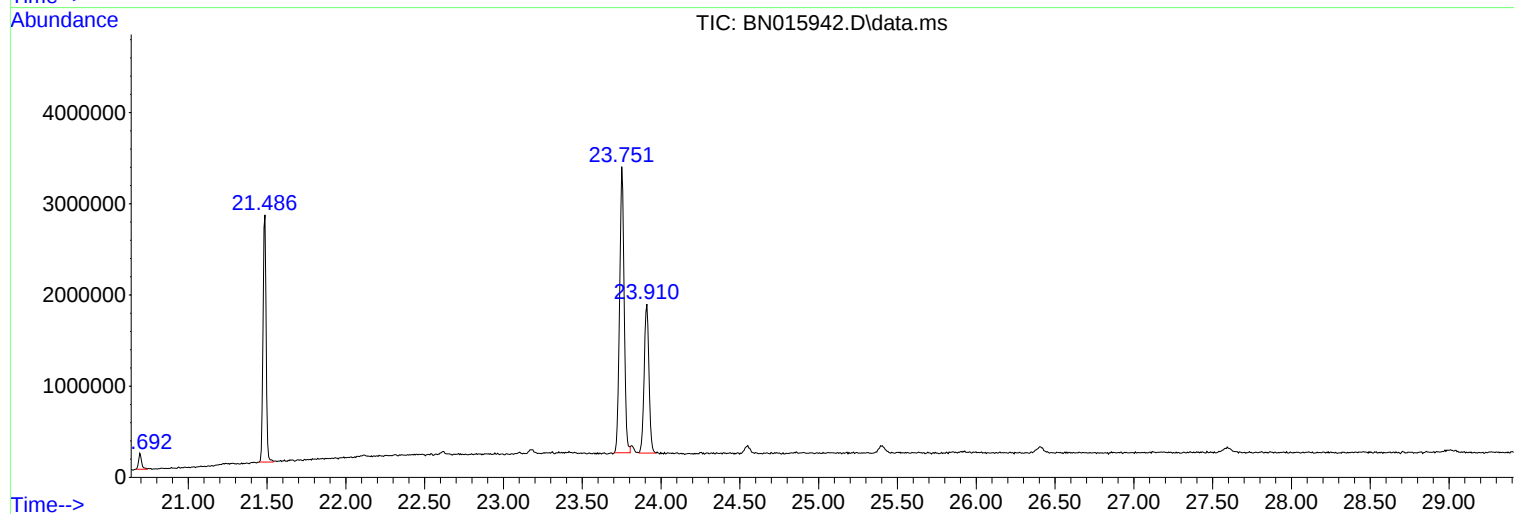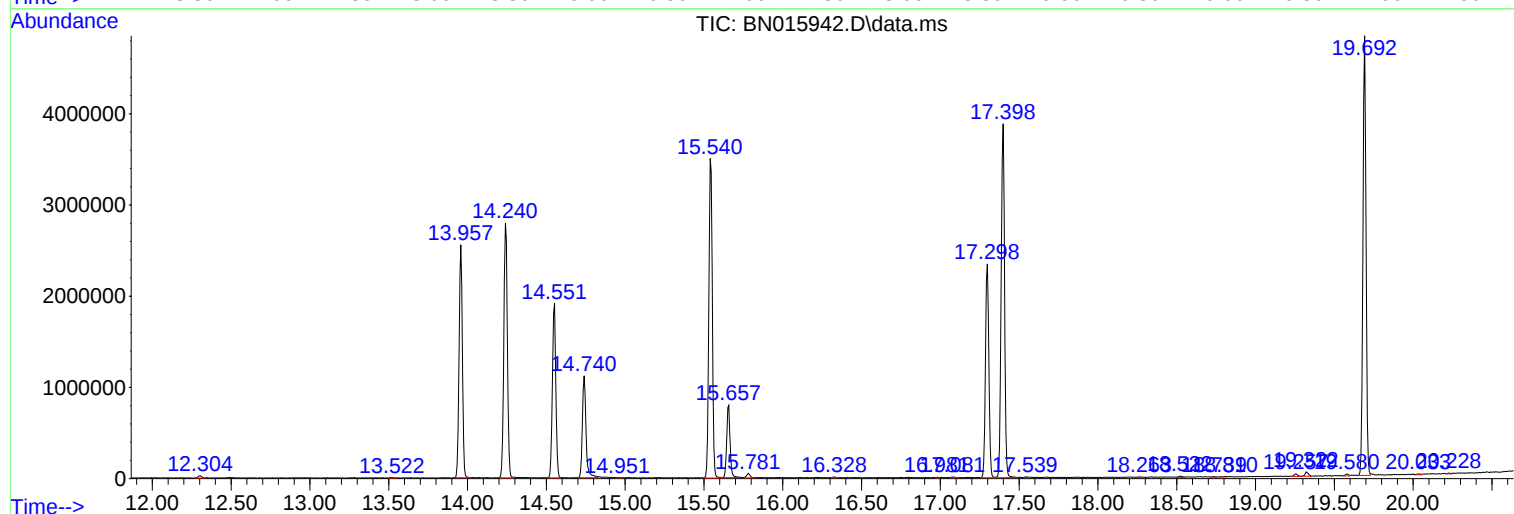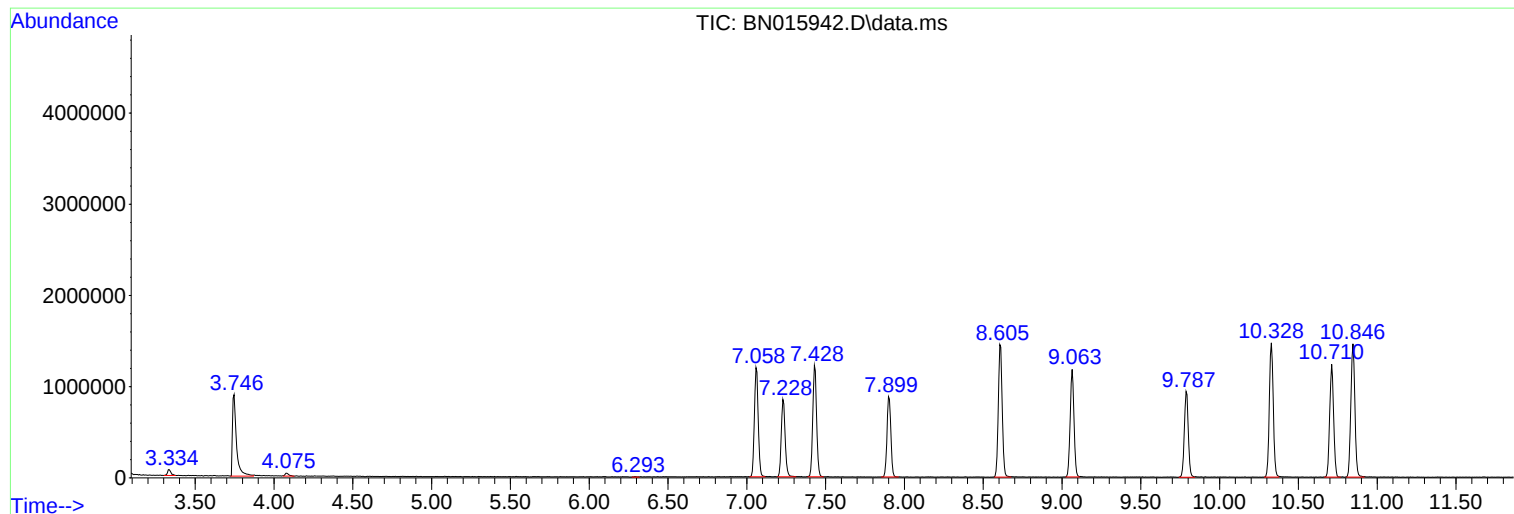

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015942.D
Acq On : 18 Aug 2021 18:07
Operator : CG/JU
Sample : PB138519BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK519

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015942.D
Acq On : 18 Aug 2021 18:07
Operator : CG/JU
Sample : PB138519BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK519

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
