

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015946.D
 Acq On : 18 Aug 2021 20:34
 Operator : CG/JU
 Sample : M3399-09
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015946.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	38	42	50	rVB	47938	72983	1.04%	0.108%
2	3.752	110	113	125	rBV	214467	382946	5.46%	0.565%
3	3.981	149	152	156	rVB4	18067	27286	0.39%	0.040%
4	4.081	165	169	175	rVB2	28314	44453	0.63%	0.066%
5	4.446	228	231	235	rBV6	7263	9727	0.14%	0.014%
6	5.981	487	492	500	rVB10	7758	20396	0.29%	0.030%
7	7.058	668	675	685	rBV2	252209	488776	6.97%	0.721%
8	7.228	698	704	717	rBV	764985	1290811	18.40%	1.904%
9	7.428	731	738	746	rBV	840382	1441255	20.55%	2.126%
10	7.528	752	755	762	rVB9	11797	17314	0.25%	0.026%
11	7.899	810	818	826	rBV	968260	1645401	23.46%	2.427%
12	7.969	826	830	835	rVB6	4288	7564	0.11%	0.011%
13	8.428	903	908	910	rBV6	4340	8490	0.12%	0.013%
14	8.605	930	938	946	rBV	757743	1266184	18.05%	1.868%
15	9.063	1007	1016	1024	rBV	1021823	1757781	25.06%	2.593%
16	9.234	1040	1045	1049	rBV6	6904	13633	0.19%	0.020%
17	9.499	1085	1090	1094	rBV4	8998	16047	0.23%	0.024%
18	9.787	1130	1139	1147	rBV	803395	1377368	19.64%	2.032%
19	9.922	1157	1162	1171	rVV5	25472	54019	0.77%	0.080%
20	10.010	1173	1177	1182	rVB6	5393	8701	0.12%	0.013%
21	10.210	1204	1211	1217	rBV10	9106	21495	0.31%	0.032%
22	10.328	1224	1231	1241	rBV	1359042	2342137	33.40%	3.455%
23	10.487	1252	1258	1264	rBV3	53777	98281	1.40%	0.145%
24	10.710	1288	1296	1306	rBV	1349033	2382921	33.98%	3.515%
25	10.846	1311	1319	1329	rBV	1147338	2066281	29.46%	3.048%
26	12.304	1562	1567	1571	rBV4	20877	34309	0.49%	0.051%
27	12.481	1593	1597	1600	rBV5	6501	11765	0.17%	0.017%
28	12.516	1600	1603	1606	rVB5	7767	10902	0.16%	0.016%
29	12.904	1663	1669	1675	rBV9	6287	16135	0.23%	0.024%
30	12.969	1678	1680	1684	rVB4	7389	8963	0.13%	0.013%
31	13.175	1712	1715	1718	rVB3	10547	12601	0.18%	0.019%
32	13.387	1748	1751	1755	rVB6	11906	13751	0.20%	0.020%
33	13.516	1769	1773	1774	rBV4	7706	10395	0.15%	0.015%
34	13.534	1774	1776	1778	rVV3	8328	8612	0.12%	0.013%
35	13.957	1840	1848	1857	rBV	2752349	3952778	56.36%	5.831%
36	14.022	1857	1859	1865	rVB7	6497	9399	0.13%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015946.D
 Acq On : 18 Aug 2021 20:34
 Operator : CG/JU
 Sample : M3399-09
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKB1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

37	14.240	1886	1896	1909	rBV	2873175	4505186	64.24%	6.645%
38	14.387	1919	1921	1927	rVB6	9764	11700	0.17%	0.017%
39	14.451	1930	1932	1937	rVB7	16196	22347	0.32%	0.033%
40	14.545	1939	1948	1957	rBV	1991191	3253987	46.40%	4.800%
41	14.740	1976	1981	1992	rVV	211374	354747	5.06%	0.523%
42	14.822	1994	1995	2001	rVB6	11343	11676	0.17%	0.017%
43	14.893	2005	2007	2012	rVB5	8398	11275	0.16%	0.017%
44	14.957	2015	2018	2024	rBV8	11640	22563	0.32%	0.033%
45	15.287	2070	2074	2076	rBV5	9280	8992	0.13%	0.013%
46	15.540	2110	2117	2125	rBV	3745210	5557569	79.24%	8.198%
47	15.651	2130	2136	2146	rBV	893334	1330403	18.97%	1.962%
48	15.781	2155	2158	2163	rVB2	47751	74770	1.07%	0.110%
49	16.104	2209	2213	2215	rBV5	11104	13678	0.20%	0.020%
50	16.234	2230	2235	2239	rBV2	32933	61860	0.88%	0.091%
51	16.334	2249	2252	2258	rVB	33948	56656	0.81%	0.084%
52	16.604	2294	2298	2303	rVB7	22981	39800	0.57%	0.059%
53	16.916	2349	2351	2353	rBV3	10129	8270	0.12%	0.012%
54	16.939	2353	2355	2357	rBV3	12672	12739	0.18%	0.019%
55	17.298	2410	2416	2426	rVV	2254922	3530020	50.33%	5.207%
56	17.398	2426	2433	2445	rVB	3909130	6139956	87.55%	9.057%
57	17.916	2519	2521	2523	rBV3	11408	9524	0.14%	0.014%
58	17.969	2528	2530	2535	rVB6	30060	33968	0.48%	0.050%
59	18.198	2565	2569	2573	rBV5	66979	111782	1.59%	0.165%
60	19.257	2746	2749	2753	rVB6	33404	47293	0.67%	0.070%
61	19.322	2757	2760	2763	rVV	66187	101246	1.44%	0.149%
62	19.357	2763	2766	2772	rVB	84269	116040	1.65%	0.171%
63	19.575	2801	2803	2807	rBV3	31217	36065	0.51%	0.053%
64	19.692	2817	2823	2836	rVB	4769612	7013378	100.00%	10.345%
65	20.692	2989	2993	2997	rBV	245728	304087	4.34%	0.449%
66	20.733	2998	3000	3004	rVB3	94580	104185	1.49%	0.154%
67	21.198	3076	3079	3087	rBV	233550	354547	5.06%	0.523%
68	21.480	3122	3127	3133	rBV	2685271	3634055	51.82%	5.360%
69	21.645	3153	3155	3160	rVB2	122114	117613	1.68%	0.173%
70	23.751	3505	3513	3520	rBV2	2977970	6283052	89.59%	9.268%
71	23.910	3532	3540	3548	rVB2	1653046	3546410	50.57%	5.231%


Sum of corrected areas: 67793299

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015946.D
Acq On : 18 Aug 2021 20:34
Operator : CG/JU
Sample : M3399-09
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

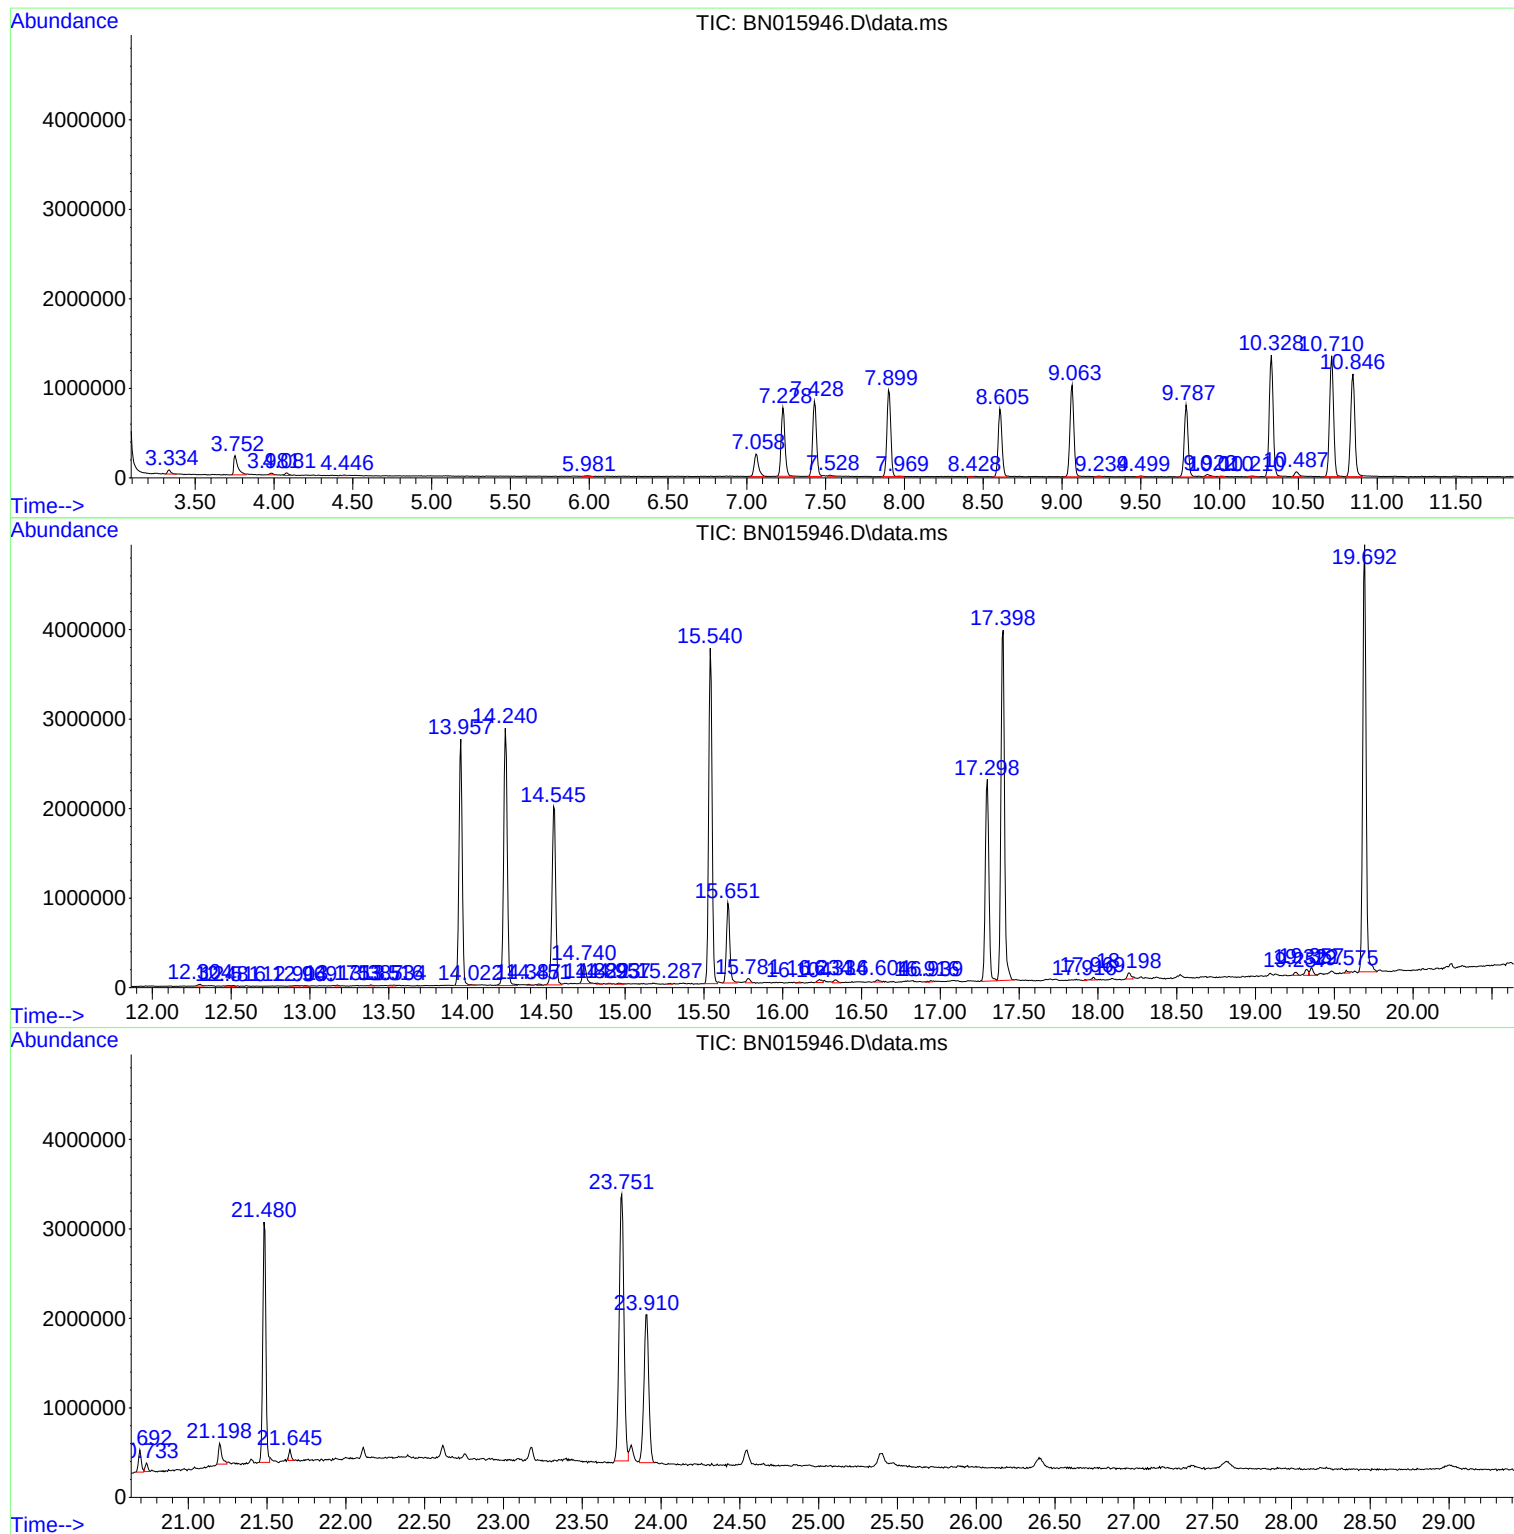

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015946.D
Acq On : 18 Aug 2021 20:34
Operator : CG/JU
Sample : M3399-09
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015946.D
Acq On : 18 Aug 2021 20:34
Operator : CG/JU
Sample : M3399-09
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
