

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015957.D
 Acq On : 19 Aug 2021 04:29
 Operator : CG/JU
 Sample : PB138537BL
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK537

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015957.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	38	42	50	rBV	82213	125619	1.54%	0.144%
2	3.740	108	111	128	rBV	1101511	1866336	22.92%	2.143%
3	3.981	147	152	155	rBV7	5424	9686	0.12%	0.011%
4	4.081	164	169	175	rBV	19182	29898	0.37%	0.034%
5	5.081	336	339	344	rVB5	5859	10512	0.13%	0.012%
6	7.058	668	675	686	rVB	1497447	2479988	30.45%	2.847%
7	7.228	697	704	716	rBV	1030297	1748510	21.47%	2.007%
8	7.428	731	738	748	rBV	1495780	2482478	30.48%	2.850%
9	7.899	811	818	827	rVB	1017201	1705172	20.94%	1.958%
10	8.604	931	938	951	rBV	1811179	3036369	37.28%	3.486%
11	9.063	1008	1016	1025	rBV	1374416	2414044	29.64%	2.771%
12	9.787	1130	1139	1147	rBV	1162415	2008698	24.66%	2.306%
13	10.322	1223	1230	1239	rBV	1720551	3092342	37.97%	3.550%
14	10.710	1286	1296	1304	rBV	1408208	2488156	30.55%	2.856%
15	10.846	1310	1319	1330	rBV	1765275	3178834	39.03%	3.649%
16	12.298	1560	1566	1571	rBV2	31609	49216	0.60%	0.057%
17	12.487	1592	1598	1599	rBV4	7530	11537	0.14%	0.013%
18	13.957	1841	1848	1860	rBV	3107993	4579873	56.23%	5.258%
19	14.239	1888	1896	1903	rBV	3661712	5416808	66.51%	6.219%
20	14.545	1941	1948	1958	rBV	2259746	3404543	41.80%	3.908%
21	14.739	1974	1981	1992	rBV	1376634	2192337	26.92%	2.517%
22	14.839	1997	1998	2003	rVV5	15953	22170	0.27%	0.025%
23	15.363	2083	2087	2091	rVB2	9642	15289	0.19%	0.018%
24	15.539	2110	2117	2126	rBV	4538603	6602698	81.07%	7.580%
25	15.651	2130	2136	2149	rVV	1004010	1464308	17.98%	1.681%
26	15.781	2153	2158	2163	rVB	51173	77634	0.95%	0.089%
27	16.328	2244	2251	2256	rVB9	11659	20319	0.25%	0.023%
28	17.081	2373	2379	2383	rBV2	13202	16477	0.20%	0.019%
29	17.298	2408	2416	2423	rBV	2723717	4032558	49.51%	4.629%
30	17.392	2426	2432	2444	rVB	4641602	7215909	88.60%	8.284%
31	17.551	2453	2459	2462	rBV6	10000	17866	0.22%	0.021%
32	17.663	2473	2478	2483	rBV6	9093	15511	0.19%	0.018%
33	18.275	2578	2582	2586	rVB4	7193	11509	0.14%	0.013%
34	18.592	2631	2636	2638	rVB5	6757	10480	0.13%	0.012%
35	19.251	2745	2748	2752	rBV3	29980	37337	0.46%	0.043%
36	19.322	2755	2760	2765	rBV	57353	83452	1.02%	0.096%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015957.D
 Acq On : 19 Aug 2021 04:29
 Operator : CG/JU
 Sample : PB138537BL
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK537

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

37	19.580	2799	2804	2807	rBV3	20602	32486	0.40%	0.037%
38	19.686	2816	2822	2834	rBV2	5743357	8144336	100.00%	9.350%
39	19.886	2854	2856	2859	rBV3	7451	8645	0.11%	0.010%
40	20.692	2989	2993	2998	rVB	162203	202034	2.48%	0.232%
41	21.398	3110	3113	3117	rVB4	47044	54713	0.67%	0.063%
42	21.480	3122	3127	3133	rBV	3240592	4166276	51.16%	4.783%
43	23.168	3411	3414	3421	rVB5	90557	159444	1.96%	0.183%
44	23.751	3504	3513	3520	rBV2	3597204	7658232	94.03%	8.792%
45	23.904	3531	3539	3550	rVB2	1996898	4094966	50.28%	4.701%
46	24.539	3643	3647	3654	rVB4	137704	288157	3.54%	0.331%
47	25.398	3787	3793	3801	rVB2	132312	323577	3.97%	0.371%




Sum of corrected areas: 87107339

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015957.D
Acq On : 19 Aug 2021 04:29
Operator : CG/JU
Sample : PB138537BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK537

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

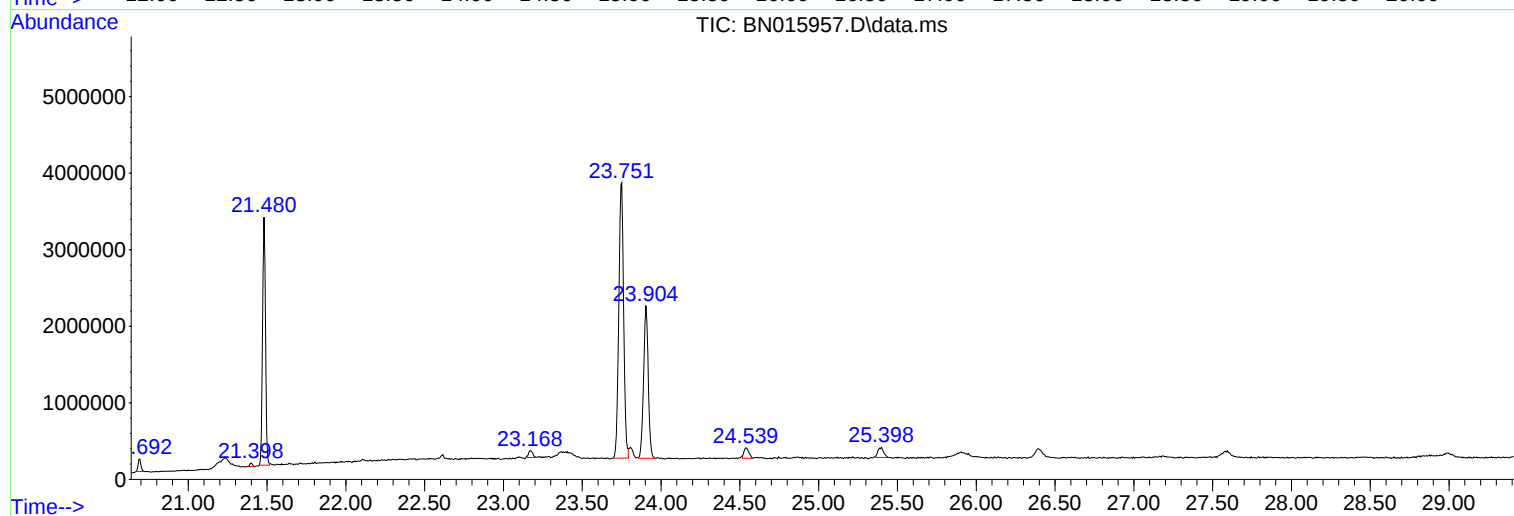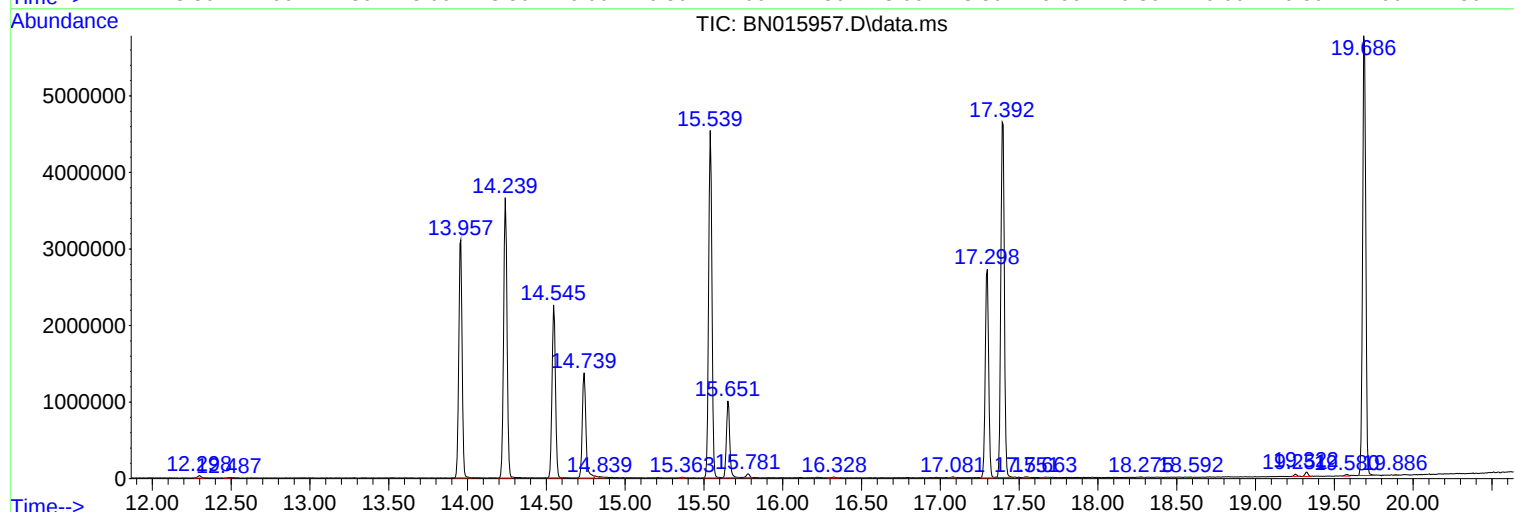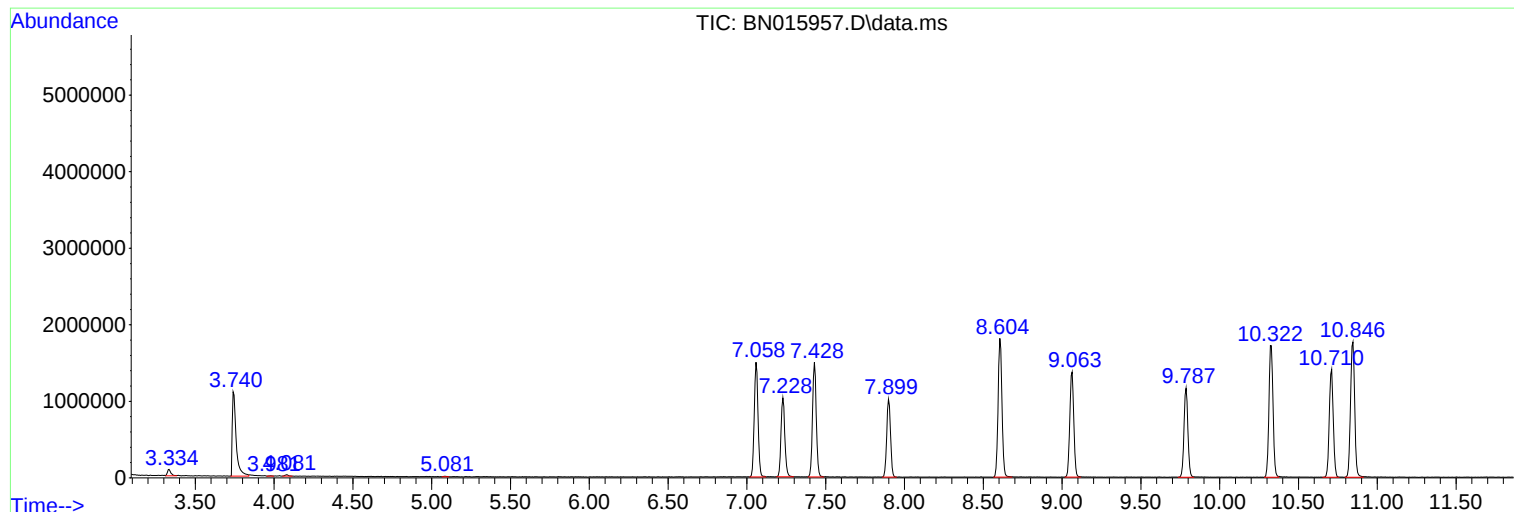

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015957.D
Acq On : 19 Aug 2021 04:29
Operator : CG/JU
Sample : PB138537BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK537

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015957.D
Acq On : 19 Aug 2021 04:29
Operator : CG/JU
Sample : PB138537BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK537

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
