

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015958.D
 Acq On : 19 Aug 2021 05:06
 Operator : CG/JU
 Sample : PB138538BL
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK538

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015958.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	37	42	51	rVB	96718	142573	1.66%	0.157%
2	3.740	108	111	135	rBV	1137817	1961442	22.88%	2.165%
3	4.081	165	169	175	rVB4	20624	35445	0.41%	0.039%
4	7.058	667	675	684	rBV	1537354	2584530	30.15%	2.853%
5	7.228	697	704	714	rBV	1086238	1797381	20.96%	1.984%
6	7.428	730	738	752	rBV	1565311	2605439	30.39%	2.876%
7	7.899	811	818	831	rVB	1018006	1697495	19.80%	1.874%
8	8.605	931	938	953	rBV	1900113	3149283	36.73%	3.476%
9	9.063	1008	1016	1026	rBV	1432295	2484343	28.98%	2.742%
10	9.787	1132	1139	1149	rBV	1228999	2094715	24.43%	2.312%
11	10.322	1223	1230	1245	rBV	1844520	3236246	37.75%	3.572%
12	10.704	1287	1295	1309	rBV	1357841	2472993	28.84%	2.730%
13	10.846	1311	1319	1333	rBV	1864918	3322662	38.76%	3.667%
14	12.298	1560	1566	1571	rVB2	30324	53464	0.62%	0.059%
15	12.510	1599	1602	1605	rVB4	6409	9163	0.11%	0.010%
16	13.510	1770	1772	1778	rBV6	6459	11420	0.13%	0.013%
17	13.957	1840	1848	1858	rBV	3264941	4767253	55.61%	5.262%
18	14.240	1888	1896	1907	rBV	3804590	5673435	66.17%	6.262%
19	14.545	1940	1948	1959	rBV	2206460	3373186	39.34%	3.723%
20	14.739	1972	1981	2002	rBV	1504275	2408697	28.10%	2.659%
21	15.198	2054	2059	2064	rBV6	5305	10030	0.12%	0.011%
22	15.539	2110	2117	2130	rBV	4709543	6928731	80.82%	7.648%
23	15.651	2130	2136	2145	rBV	1041229	1514952	17.67%	1.672%
24	15.781	2153	2158	2164	rVB	61524	85859	1.00%	0.095%
25	16.322	2246	2250	2256	rBV7	11717	19810	0.23%	0.022%
26	17.081	2373	2379	2384	rBV3	12561	18106	0.21%	0.020%
27	17.298	2407	2416	2424	rBV	2594179	4008854	46.76%	4.425%
28	17.392	2424	2432	2444	rVV2	5131264	7632636	89.03%	8.425%
29	17.551	2455	2459	2463	rBV6	6368	10714	0.12%	0.012%
30	17.675	2476	2480	2484	rBV6	7147	9495	0.11%	0.010%
31	19.251	2745	2748	2754	rVB5	36157	43223	0.50%	0.048%
32	19.327	2754	2761	2764	rBV2	55542	82888	0.97%	0.091%
33	19.575	2800	2803	2809	rBV2	25066	34683	0.40%	0.038%
34	19.692	2816	2823	2832	rBV	5980793	8573386	100.00%	9.463%
35	20.692	2989	2993	3002	rBV	170426	219100	2.56%	0.242%
36	21.480	3122	3127	3135	rBV2	3230656	4301160	50.17%	4.748%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015958.D
Acq On : 19 Aug 2021 05:06
Operator : CG/JU
Sample : PB138538BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK538

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Title : SVOA CALIBRATION

37	23.751	3504	3513	3520	rBV	3903705	8285249	96.64%	9.145%
38	23.904	3532	3539	3555	rVB2	1964557	4293394	50.08%	4.739%
39	24.539	3642	3647	3654	rVB4	149525	313005	3.65%	0.345%
40	25.392	3789	3792	3802	rVB2	164797	331217	3.86%	0.366%


Sum of corrected areas: 90597657

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015958.D
Acq On : 19 Aug 2021 05:06
Operator : CG/JU
Sample : PB138538BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK538

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

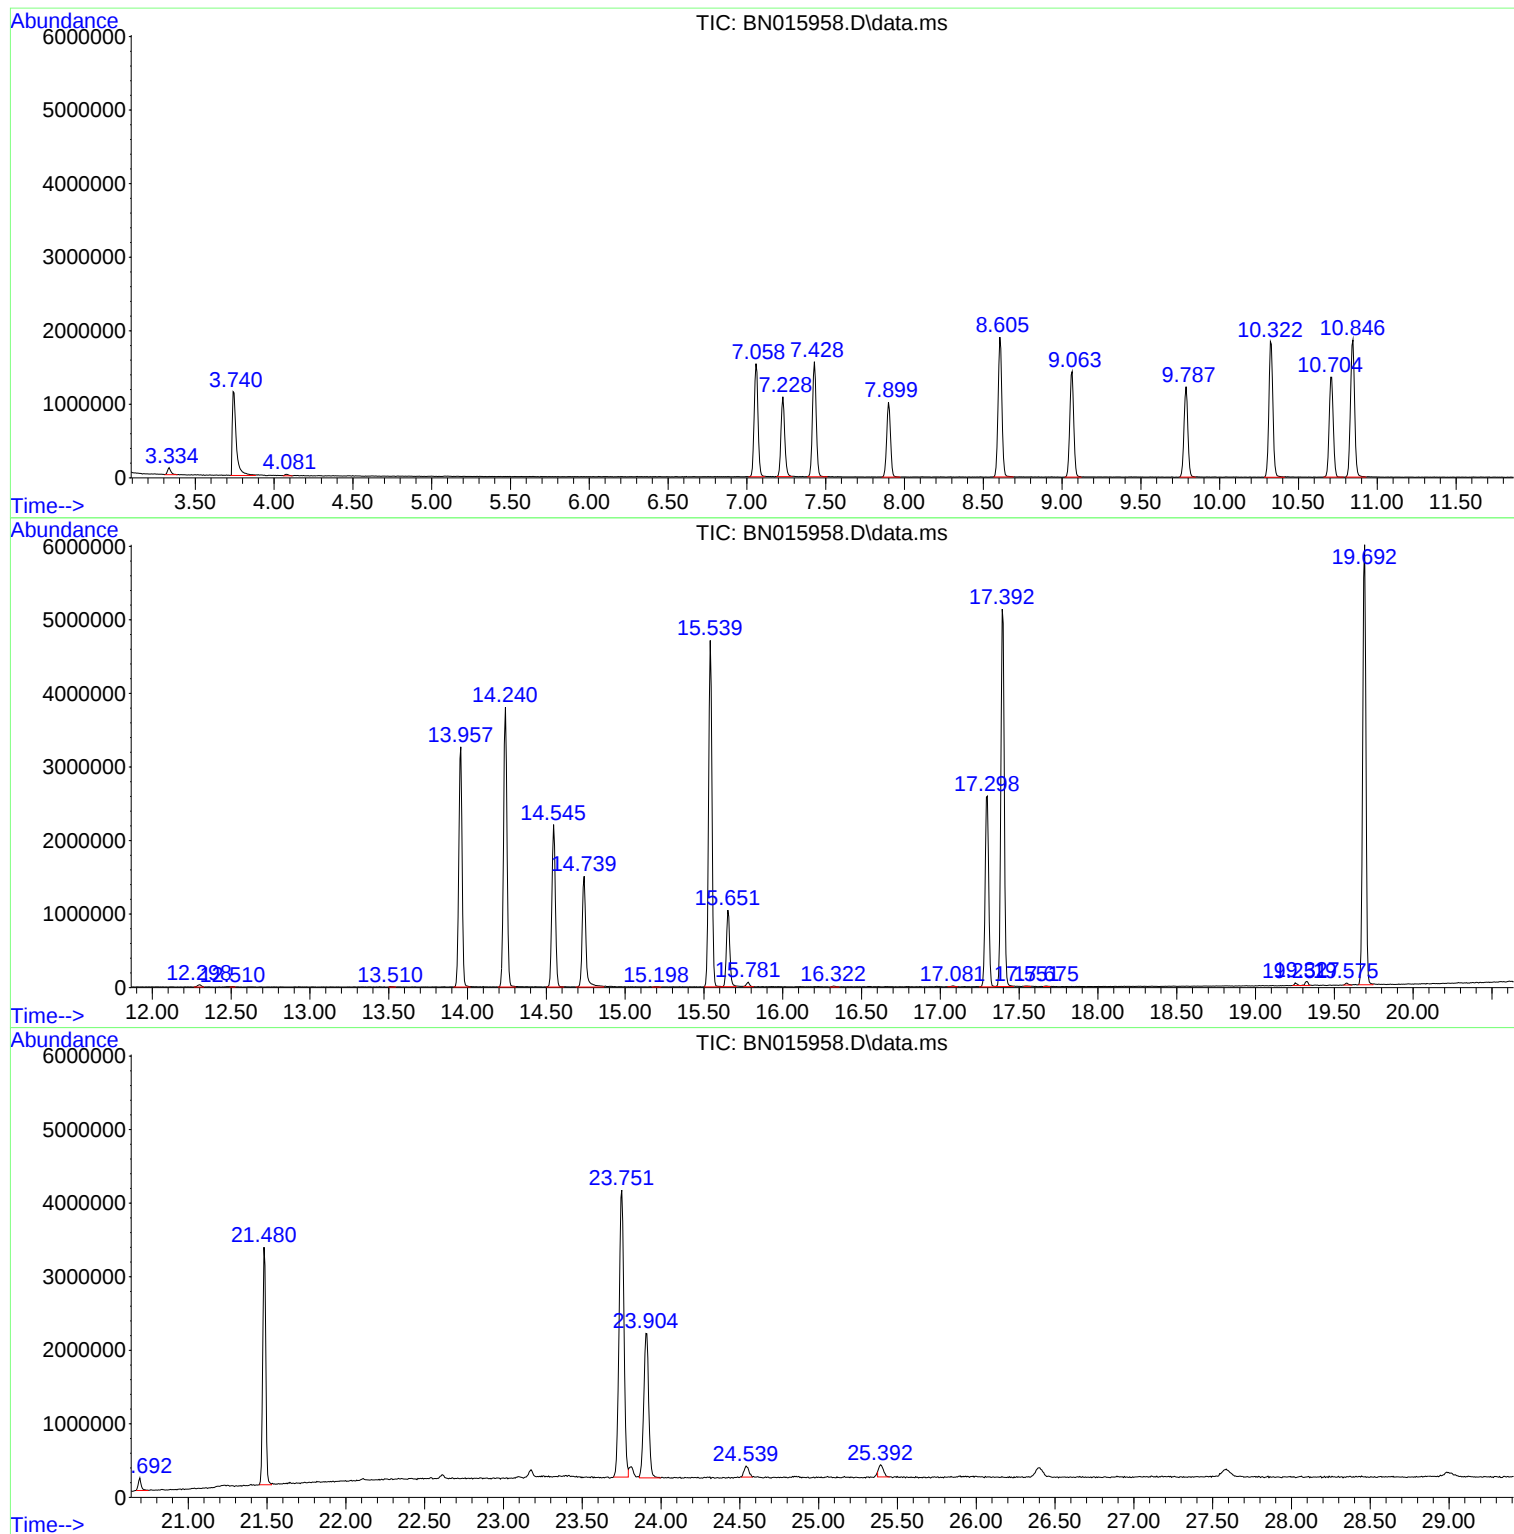

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015958.D
Acq On : 19 Aug 2021 05:06
Operator : CG/JU
Sample : PB138538BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK538

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015958.D
Acq On : 19 Aug 2021 05:06
Operator : CG/JU
Sample : PB138538BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK538

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
