

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015961.D
 Acq On : 19 Aug 2021 06:55
 Operator : CG/JU
 Sample : M3399-19
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015961.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	38	42	48	rVB	57224	80020	1.07%	0.106%
2	3.752	109	113	127	rBV	280884	540010	7.21%	0.716%
3	3.975	149	151	158	rVB4	23806	40244	0.54%	0.053%
4	4.081	164	169	174	rVB3	20672	30340	0.40%	0.040%
5	5.981	488	492	497	rBV4	11162	17654	0.24%	0.023%
6	6.875	641	644	649	rBV5	7310	11178	0.15%	0.015%
7	7.058	668	675	689	rBV	304622	568833	7.59%	0.754%
8	7.228	694	704	717	rBV	839564	1446081	19.30%	1.917%
9	7.428	731	738	746	rBV	965736	1613531	21.53%	2.139%
10	7.528	751	755	759	rVB4	8956	10822	0.14%	0.014%
11	7.899	811	818	825	rBV	1094209	1832946	24.46%	2.429%
12	7.963	825	829	837	rVB5	15167	28057	0.37%	0.037%
13	8.281	875	883	889	rVB6	14154	29435	0.39%	0.039%
14	8.604	931	938	948	rBV	832375	1375726	18.36%	1.823%
15	9.063	1008	1016	1028	rBV	1103290	1965254	26.23%	2.605%
16	9.169	1031	1034	1037	rVV4	7319	10894	0.15%	0.014%
17	9.228	1037	1044	1048	rVV7	16968	27122	0.36%	0.036%
18	9.493	1084	1089	1098	rVB3	24244	47490	0.63%	0.063%
19	9.787	1131	1139	1148	rBV	922256	1580926	21.10%	2.095%
20	10.104	1187	1193	1199	rBV5	8939	19463	0.26%	0.026%
21	10.322	1222	1230	1239	rBV	1413368	2451254	32.71%	3.249%
22	10.481	1252	1257	1265	rBV	110025	207172	2.76%	0.275%
23	10.710	1288	1296	1303	rBV	1454339	2608056	34.81%	3.457%
24	10.840	1308	1318	1326	rBV	1083578	1943662	25.94%	2.576%
25	11.357	1401	1406	1409	rBV6	4815	9160	0.12%	0.012%
26	11.493	1425	1429	1435	rBV7	10838	22348	0.30%	0.030%
27	11.993	1510	1514	1518	rVB7	9128	14186	0.19%	0.019%
28	12.293	1562	1565	1571	rVB3	25611	39945	0.53%	0.053%
29	12.481	1592	1597	1599	rBV5	7283	12059	0.16%	0.016%
30	12.587	1609	1615	1622	rBV8	12285	27953	0.37%	0.037%
31	12.963	1674	1679	1682	rVB5	8490	13282	0.18%	0.018%
32	13.157	1708	1712	1717	rVB8	9853	20585	0.27%	0.027%
33	13.375	1745	1749	1756	rBV7	20366	40902	0.55%	0.054%
34	13.445	1756	1761	1768	rVB9	8779	17888	0.24%	0.024%
35	13.510	1768	1772	1778	rBV8	15102	26688	0.36%	0.035%
36	13.687	1798	1802	1804	rBV5	7435	9971	0.13%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015961.D
 Acq On : 19 Aug 2021 06:55
 Operator : CG/JU
 Sample : M3399-19
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

37	13.869	1829	1833	1838	rVV6	12642	23148	0.31%	0.031%
38	13.951	1841	1847	1857	rVV	2734589	4090937	54.60%	5.422%
39	14.034	1860	1861	1866	rVB5	10496	13757	0.18%	0.018%
40	14.104	1870	1873	1876	rVV4	9585	11780	0.16%	0.016%
41	14.239	1884	1896	1903	rBV	2942929	4564211	60.91%	6.049%
42	14.451	1929	1932	1936	rVV5	11873	19090	0.25%	0.025%
43	14.504	1936	1941	1943	rVV	275870	431397	5.76%	0.572%
44	14.545	1943	1948	1955	rVV	2402962	3805179	50.78%	5.043%
45	14.610	1955	1959	1966	rVV2	103590	184009	2.46%	0.244%
46	14.663	1966	1968	1971	rVV4	10355	12979	0.17%	0.017%
47	14.692	1971	1973	1975	rVV3	10296	10393	0.14%	0.014%
48	14.739	1975	1981	1997	rVB	247220	463732	6.19%	0.615%
49	14.892	2004	2007	2012	rVB6	10670	17406	0.23%	0.023%
50	14.963	2012	2019	2021	rBV7	11969	19808	0.26%	0.026%
51	15.087	2038	2040	2044	rVB5	7800	11292	0.15%	0.015%
52	15.134	2044	2048	2052	rBV6	11623	16612	0.22%	0.022%
53	15.286	2067	2074	2080	rBV2	52467	79110	1.06%	0.105%
54	15.357	2080	2086	2090	rVV9	15353	36191	0.48%	0.048%
55	15.404	2090	2094	2100	rVB9	13209	20214	0.27%	0.027%
56	15.539	2108	2117	2124	rBV	3981730	5836203	77.89%	7.735%
57	15.592	2124	2126	2130	rVB	37934	47077	0.63%	0.062%
58	15.651	2130	2136	2144	rBV	1034972	1505190	20.09%	1.995%
59	15.781	2153	2158	2165	rVB3	50162	91524	1.22%	0.121%
60	15.898	2173	2178	2182	rBV7	9073	16399	0.22%	0.022%
61	15.957	2185	2188	2192	rBV6	14804	17468	0.23%	0.023%
62	15.986	2192	2193	2198	rVB5	10751	9924	0.13%	0.013%
63	16.098	2210	2212	2219	rVB7	11620	22426	0.30%	0.030%
64	16.175	2223	2225	2229	rBV5	8590	10304	0.14%	0.014%
65	16.222	2229	2233	2236	rBV6	12738	18772	0.25%	0.025%
66	16.269	2237	2241	2242	rBV3	10760	12010	0.16%	0.016%
67	16.310	2243	2248	2251	rBV2	51586	83047	1.11%	0.110%
68	16.433	2267	2269	2275	rVB7	9500	14962	0.20%	0.020%
69	16.604	2292	2298	2303	rBV10	13002	25826	0.34%	0.034%
70	16.692	2310	2313	2316	rBV5	10731	12009	0.16%	0.016%
71	16.951	2352	2357	2359	rBV5	12658	21106	0.28%	0.028%
72	17.081	2370	2379	2382	rBV5	21625	61362	0.82%	0.081%
73	17.110	2382	2384	2389	rVB6	20093	25273	0.34%	0.033%
74	17.292	2409	2415	2421	rBV	2702975	4020747	53.66%	5.329%
75	17.392	2426	2432	2444	rVV2	4245642	6591396	87.97%	8.736%
76	17.486	2445	2448	2451	rVV5	20152	36608	0.49%	0.049%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015961.D
 Acq On : 19 Aug 2021 06:55
 Operator : CG/JU
 Sample : M3399-19
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKD1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

77	17.522	2451	2454	2460	rVB	90184	111998	1.49%	0.148%
78	17.686	2478	2482	2484	rVV5	12227	20817	0.28%	0.028%
79	17.728	2486	2489	2496	rVB5	29349	47301	0.63%	0.063%
80	17.798	2498	2501	2502	rBV3	9470	9936	0.13%	0.013%
81	17.969	2525	2530	2535	rBV7	64364	92542	1.24%	0.123%
82	18.086	2548	2550	2554	rVB5	23816	27534	0.37%	0.036%
83	18.192	2564	2568	2576	rBV5	31117	70177	0.94%	0.093%
84	18.263	2578	2580	2584	rBV	19251	26314	0.35%	0.035%
85	18.522	2620	2624	2627	rVV6	20041	33041	0.44%	0.044%
86	18.675	2644	2650	2653	rBV8	15129	26677	0.36%	0.035%
87	18.910	2687	2690	2694	rBV	32216	42353	0.57%	0.056%
88	19.086	2717	2720	2725	rBV2	27721	39899	0.53%	0.053%
89	19.251	2745	2748	2753	rVB3	38450	47612	0.64%	0.063%
90	19.322	2756	2760	2764	rBV	55377	80964	1.08%	0.107%
91	19.580	2799	2804	2807	rBV2	39632	64639	0.86%	0.086%
92	19.686	2816	2822	2834	rBV	5223878	7492775	100.00%	9.931%
93	19.922	2858	2862	2864	rBV5	22924	31673	0.42%	0.042%
94	20.233	2912	2915	2919	rVB7	31370	39821	0.53%	0.053%
95	20.692	2989	2993	2998	rBV	187685	234651	3.13%	0.311%
96	21.198	3075	3079	3085	rBV2	248308	396855	5.30%	0.526%
97	21.398	3110	3113	3116	rVB	100941	108158	1.44%	0.143%
98	21.480	3122	3127	3137	rVB	3241072	4187370	55.89%	5.550%
99	23.751	3505	3513	3520	rBV	3461702	6965078	92.96%	9.231%
100	23.904	3532	3539	3551	rVB2	1973403	4199406	56.05%	5.566%



Sum of corrected areas: 75449606

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015961.D
Acq On : 19 Aug 2021 06:55
Operator : CG/JU
Sample : M3399-19
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

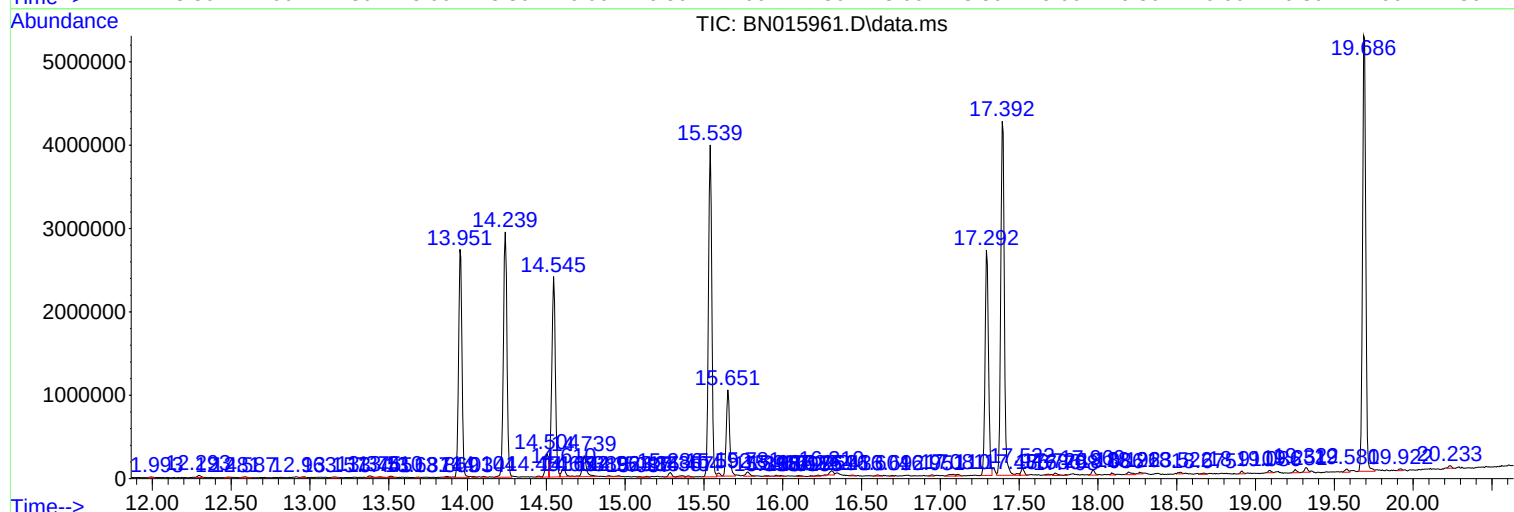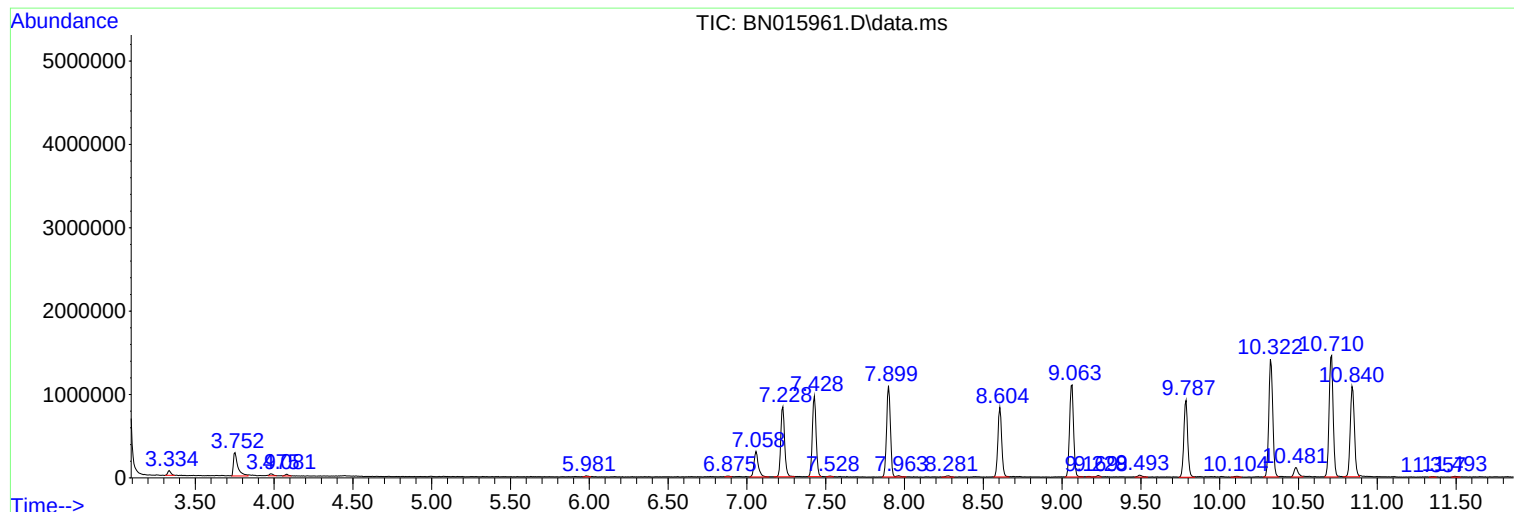

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015961.D
Acq On : 19 Aug 2021 06:55
Operator : CG/JU
Sample : M3399-19
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015961.D
Acq On : 19 Aug 2021 06:55
Operator : CG/JU
Sample : M3399-19
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
