

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015962.D
 Acq On : 19 Aug 2021 07:31
 Operator : CG/JU
 Sample : M3399-20
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015962.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	36	42	49	rBV	56454	93509	1.22%	0.130%
2	3.758	111	114	128	rBV	83626	180014	2.35%	0.250%
3	3.981	149	152	159	rVB4	20265	38304	0.50%	0.053%
4	4.081	164	169	175	rBV2	20384	31623	0.41%	0.044%
5	5.987	489	493	500	rVB6	5535	11718	0.15%	0.016%
6	7.058	669	675	684	rBV2	256138	456792	5.97%	0.635%
7	7.228	697	704	714	rBV	845135	1454755	19.00%	2.022%
8	7.428	731	738	750	rVB	935018	1570887	20.52%	2.184%
9	7.528	750	755	760	rBV6	7121	13210	0.17%	0.018%
10	7.899	810	818	825	rBV	1036386	1737792	22.69%	2.416%
11	7.969	825	830	833	rVB4	8234	12237	0.16%	0.017%
12	8.605	929	938	948	rBV	718814	1192763	15.58%	1.658%
13	9.058	1007	1015	1026	rBV	1123811	1981075	25.87%	2.754%
14	9.493	1084	1089	1093	rVB5	11134	17200	0.22%	0.024%
15	9.787	1131	1139	1150	rBV	894429	1566948	20.46%	2.178%
16	10.322	1223	1230	1244	rBV	1302323	2267190	29.61%	3.152%
17	10.487	1252	1258	1264	rBV5	21688	39037	0.51%	0.054%
18	10.705	1287	1295	1304	rBV	1406148	2515069	32.85%	3.496%
19	10.840	1310	1318	1331	rBV	862611	1553518	20.29%	2.160%
20	12.005	1513	1516	1521	rVB5	6825	9510	0.12%	0.013%
21	12.299	1560	1566	1571	rBV	26748	38975	0.51%	0.054%
22	13.375	1744	1749	1755	rVB8	9427	13953	0.18%	0.019%
23	13.510	1767	1772	1775	rBV6	5616	7865	0.10%	0.011%
24	13.951	1841	1847	1858	rBV	2575720	3756744	49.06%	5.223%
25	14.240	1887	1896	1905	rBV	2879170	4348715	56.79%	6.046%
26	14.451	1929	1932	1936	rVB6	7943	9880	0.13%	0.014%
27	14.546	1940	1948	1956	rBV	2192103	3358203	43.86%	4.669%
28	14.740	1974	1981	1998	rBV	190910	359653	4.70%	0.500%
29	14.957	2014	2018	2020	rBV4	8915	9948	0.13%	0.014%
30	15.287	2071	2074	2079	rVB4	7793	9506	0.12%	0.013%
31	15.540	2110	2117	2129	rBV	3807066	5562731	72.65%	7.733%
32	15.651	2130	2136	2145	rBV	1086478	1552177	20.27%	2.158%
33	15.781	2152	2158	2167	rVB2	44844	78516	1.03%	0.109%
34	15.957	2185	2188	2191	rBV4	6410	9316	0.12%	0.013%
35	15.987	2191	2193	2196	rVB3	6916	8265	0.11%	0.011%
36	16.110	2212	2214	2219	rVB4	6915	9472	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015962.D
 Acq On : 19 Aug 2021 07:31
 Operator : CG/JU
 Sample : M3399-20
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKD2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

37	16.181	2219	2226	2228	rBV7	3927	9064	0.12%	0.013%
38	16.222	2230	2233	2237	rVV6	8803	13744	0.18%	0.019%
39	16.263	2237	2240	2244	rVV5	12588	16897	0.22%	0.023%
40	16.328	2246	2251	2258	rVB7	13058	23504	0.31%	0.033%
41	16.787	2325	2329	2335	rVB6	6436	13178	0.17%	0.018%
42	16.898	2345	2348	2351	rBV4	6057	8060	0.11%	0.011%
43	16.975	2356	2361	2364	rBV6	9309	14059	0.18%	0.020%
44	17.057	2371	2375	2377	rBV5	13116	19047	0.25%	0.026%
45	17.075	2377	2378	2382	rVV3	15335	16529	0.22%	0.023%
46	17.110	2382	2384	2388	rVB5	9895	13030	0.17%	0.018%
47	17.292	2408	2415	2423	rBV	2752861	4020346	52.50%	5.589%
48	17.392	2425	2432	2446	rVV2	4384418	6642249	86.75%	9.234%
49	17.581	2462	2464	2469	rVB6	6281	9913	0.13%	0.014%
50	17.663	2475	2478	2482	rBV4	8152	10649	0.14%	0.015%
51	17.798	2498	2501	2505	rBV5	16797	19705	0.26%	0.027%
52	17.969	2525	2530	2535	rBV7	27753	38401	0.50%	0.053%
53	18.039	2538	2542	2543	rBV4	8748	7902	0.10%	0.011%
54	18.087	2547	2550	2555	rVB5	10557	15239	0.20%	0.021%
55	18.198	2563	2569	2574	rBV9	19875	38849	0.51%	0.054%
56	18.263	2574	2580	2583	rBV5	13040	19510	0.25%	0.027%
57	18.404	2602	2604	2608	rVB5	6744	8617	0.11%	0.012%
58	18.492	2616	2619	2623	rBV4	21358	28188	0.37%	0.039%
59	18.669	2647	2649	2652	rBV4	7098	9457	0.12%	0.013%
60	18.816	2670	2674	2676	rBV5	10172	14608	0.19%	0.020%
61	19.128	2724	2727	2729	rVV4	12912	12646	0.17%	0.018%
62	19.251	2744	2748	2752	rBV5	36460	50170	0.66%	0.070%
63	19.322	2755	2760	2769	rVV	59362	100398	1.31%	0.140%
64	19.581	2801	2804	2808	rVB5	17442	24598	0.32%	0.034%
65	19.686	2816	2822	2830	rBV2	5469553	7657166	100.00%	10.645%
66	20.128	2895	2897	2898	rBV2	11371	9835	0.13%	0.014%
67	20.692	2989	2993	2997	rBV	185558	234487	3.06%	0.326%
68	21.198	3075	3079	3084	rBV2	165101	283113	3.70%	0.394%
69	21.480	3122	3127	3135	rBV	3215765	4272027	55.79%	5.939%
70	23.175	3411	3415	3421	rVB2	124884	198714	2.60%	0.276%
71	23.751	3504	3513	3520	rBV	3542930	7231086	94.44%	10.053%
72	23.904	3531	3539	3549	rVB2	2058914	4215705	55.06%	5.861%
73	24.539	3643	3647	3654	rVB4	175657	340205	4.44%	0.473%
74	25.392	3787	3792	3802	rVB4	159662	394028	5.15%	0.548%

Sum of corrected areas: 71931993

Instrument :

BNA_N

ClientSampleId :




DBKD2

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015962.D
Acq On : 19 Aug 2021 07:31
Operator : CG/JU
Sample : M3399-20
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

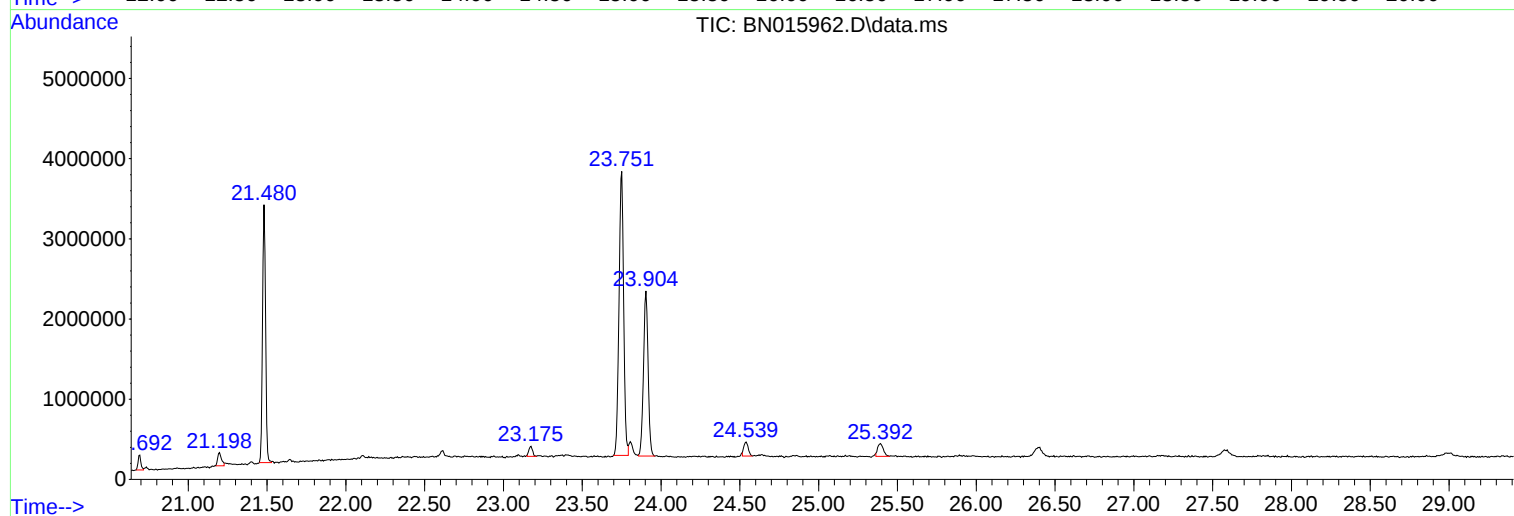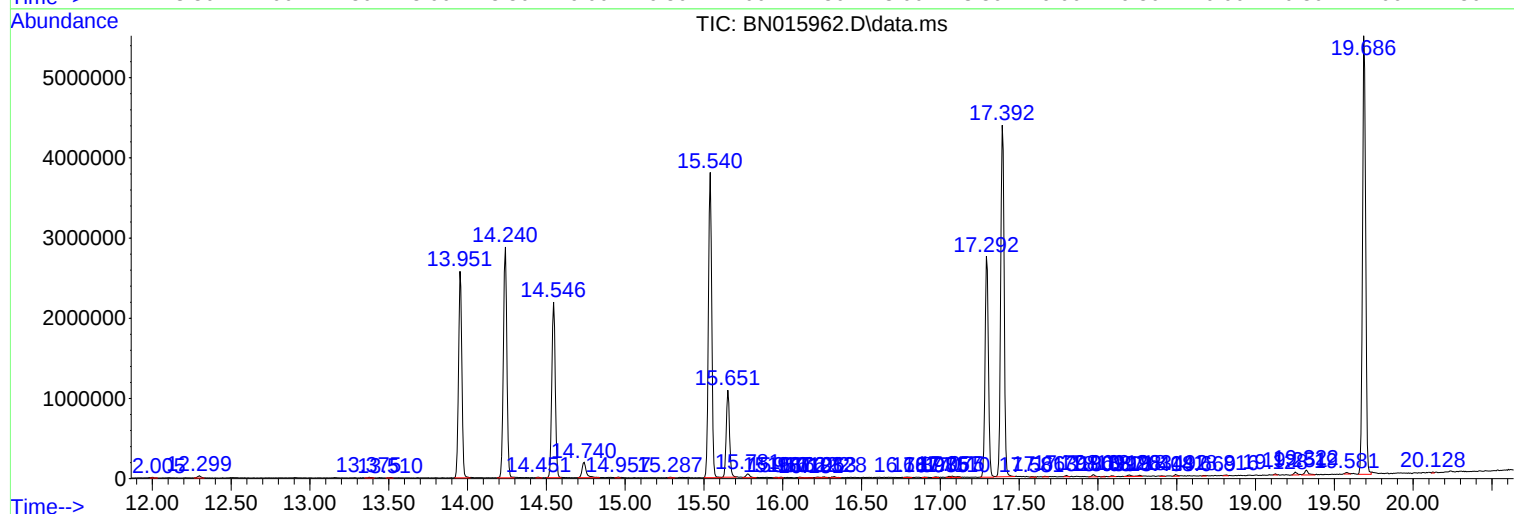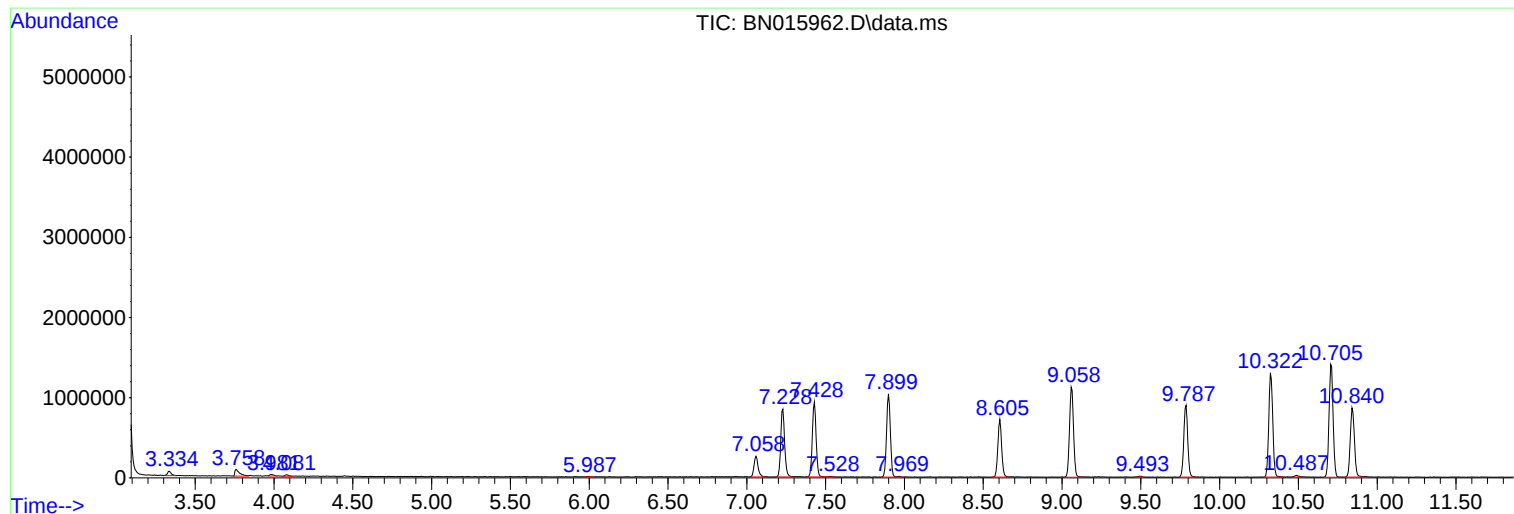

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015962.D
Acq On : 19 Aug 2021 07:31
Operator : CG/JU
Sample : M3399-20
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015962.D
Acq On : 19 Aug 2021 07:31
Operator : CG/JU
Sample : M3399-20
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
