

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015967.D
 Acq On : 19 Aug 2021 10:36
 Operator : CG/JU
 Sample : M3422-13
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015967.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	37	42	53	rVB	53696	91493	1.06%	0.118%
2	3.752	110	113	129	rBV	199231	375259	4.34%	0.483%
3	3.987	148	153	160	rVB4	20240	35524	0.41%	0.046%
4	4.075	165	168	172	rBV2	18679	27049	0.31%	0.035%
5	7.058	669	675	685	rVB	293715	504207	5.83%	0.649%
6	7.228	697	704	717	rBV	882824	1483121	17.15%	1.910%
7	7.428	731	738	747	rVV	985787	1633628	18.89%	2.104%
8	7.522	750	754	759	rVB6	6429	8821	0.10%	0.011%
9	7.899	811	818	826	rBV	990392	1674550	19.37%	2.156%
10	7.969	826	830	835	rVB5	7401	12049	0.14%	0.016%
11	8.604	931	938	951	rVB	784458	1338685	15.48%	1.724%
12	9.063	1008	1016	1027	rBV	1221022	2063778	23.87%	2.657%
13	9.499	1085	1090	1098	rVB4	19280	34630	0.40%	0.045%
14	9.787	1132	1139	1150	rVB	939417	1617617	18.71%	2.083%
15	10.116	1188	1195	1199	rVB7	7684	12128	0.14%	0.016%
16	10.328	1224	1231	1242	rBV	1359318	2348524	27.16%	3.024%
17	10.481	1251	1257	1265	rBV3	113832	207607	2.40%	0.267%
18	10.710	1286	1296	1303	rBV	1382329	2404535	27.81%	3.096%
19	10.846	1310	1319	1337	rVV	1226054	2248631	26.01%	2.895%
20	10.963	1337	1339	1345	rVB6	7662	10217	0.12%	0.013%
21	11.063	1353	1356	1358	rBV4	8335	9837	0.11%	0.013%
22	12.004	1506	1516	1521	rBV5	14642	27668	0.32%	0.036%
23	12.298	1555	1566	1571	rBV4	26421	67316	0.78%	0.087%
24	12.587	1613	1615	1620	rVB6	7597	9456	0.11%	0.012%
25	13.157	1709	1712	1717	rVB6	7167	9816	0.11%	0.013%
26	13.381	1743	1750	1755	rBV4	23062	36925	0.43%	0.048%
27	13.563	1777	1781	1785	rVB7	12266	19665	0.23%	0.025%
28	13.957	1841	1848	1859	rBV	2821830	4070831	47.08%	5.242%
29	14.239	1889	1896	1906	rVB	3011929	4604390	53.25%	5.929%
30	14.457	1929	1933	1935	rBV3	7508	9201	0.11%	0.012%
31	14.545	1938	1948	1956	rBV	2108572	3342974	38.66%	4.305%
32	14.610	1956	1959	1964	rVB2	27435	41613	0.48%	0.054%
33	14.739	1975	1981	1992	rBV	246602	423101	4.89%	0.545%
34	14.857	1997	2001	2008	rVV	55753	80113	0.93%	0.103%
35	14.945	2011	2016	2023	rVB	73925	122430	1.42%	0.158%
36	15.051	2031	2034	2037	rBV4	7895	9925	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015967.D
 Acq On : 19 Aug 2021 10:36
 Operator : CG/JU
 Sample : M3422-13
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

37	15.463	2100	2104	2110	rVB7	8660	15463	0.18%	0.020%
38	15.539	2110	2117	2130	rBV	4030665	6161072	71.26%	7.933%
39	15.651	2130	2136	2144	rVV	1164547	1754203	20.29%	2.259%
40	15.751	2144	2153	2155	rVV6	49826	127511	1.47%	0.164%
41	15.781	2155	2158	2166	rVV2	61144	97665	1.13%	0.126%
42	15.904	2176	2179	2183	rVB5	14370	16801	0.19%	0.022%
43	15.992	2190	2194	2197	rBV3	48250	72781	0.84%	0.094%
44	16.034	2197	2201	2209	rVB2	69821	116554	1.35%	0.150%
45	16.104	2209	2213	2214	rBV4	8860	11489	0.13%	0.015%
46	16.233	2228	2235	2236	rBV6	16050	27137	0.31%	0.035%
47	16.257	2236	2239	2243	rVV5	21387	34259	0.40%	0.044%
48	16.328	2247	2251	2255	rVB7	11668	17825	0.21%	0.023%
49	16.569	2282	2292	2296	rBV6	43860	96786	1.12%	0.125%
50	16.792	2328	2330	2334	rVB5	9428	10049	0.12%	0.013%
51	16.945	2352	2356	2359	rBV5	17479	27427	0.32%	0.035%
52	17.028	2367	2370	2373	rBV5	5839	9398	0.11%	0.012%
53	17.063	2373	2376	2379	rVV2	24843	42582	0.49%	0.055%
54	17.110	2382	2384	2388	rVB4	14059	16939	0.20%	0.022%
55	17.298	2409	2416	2426	rBV	2593672	3835475	44.36%	4.939%
56	17.398	2426	2433	2447	rBV	4577961	7189005	83.15%	9.257%
57	17.610	2466	2469	2473	rVB6	7493	9367	0.11%	0.012%
58	17.704	2473	2485	2490	rBV3	38581	78196	0.90%	0.101%
59	17.798	2497	2501	2509	rBV9	28352	61923	0.72%	0.080%
60	17.975	2525	2531	2533	rBV5	43919	60787	0.70%	0.078%
61	18.098	2546	2552	2557	rBV10	26782	40245	0.47%	0.052%
62	18.192	2563	2568	2578	rBV9	52376	108296	1.25%	0.139%
63	18.275	2578	2582	2585	rVB2	14219	22305	0.26%	0.029%
64	18.375	2593	2599	2605	rVB2	80905	122200	1.41%	0.157%
65	18.492	2614	2619	2623	rBV7	32953	56893	0.66%	0.073%
66	18.557	2627	2630	2633	rBV5	10687	17277	0.20%	0.022%
67	18.610	2636	2639	2644	rVB7	13385	21205	0.25%	0.027%
68	18.669	2644	2649	2650	rBV5	14347	22889	0.26%	0.029%
69	18.710	2653	2656	2660	rVB3	40415	49150	0.57%	0.063%
70	18.775	2662	2667	2669	rBV5	17729	22075	0.26%	0.028%
71	18.869	2681	2683	2684	rBV2	11291	11577	0.13%	0.015%
72	18.910	2686	2690	2695	rVB6	31009	53801	0.62%	0.069%
73	19.069	2711	2717	2718	rBV6	9699	15513	0.18%	0.020%
74	19.127	2724	2727	2733	rVB3	24824	40414	0.47%	0.052%
75	19.233	2741	2745	2746	rBV2	34223	43602	0.50%	0.056%
76	19.327	2756	2761	2763	rBV2	61387	96826	1.12%	0.125%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015967.D
 Acq On : 19 Aug 2021 10:36
 Operator : CG/JU
 Sample : M3422-13
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKC8

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

77	19.351	2763	2765	2770	rVB	63760	88314	1.02%	0.114%
78	19.422	2770	2777	2781	rBV8	26498	59171	0.68%	0.076%
79	19.574	2801	2803	2807	rBV3	21275	22941	0.27%	0.030%
80	19.627	2810	2812	2814	rVB3	14830	9597	0.11%	0.012%
81	19.692	2817	2823	2835	rVB	5998708	8646327	100.00%	11.133%
82	19.898	2855	2858	2863	rBV6	17343	22723	0.26%	0.029%
83	20.098	2889	2892	2897	rVB	42362	56658	0.66%	0.073%
84	20.257	2914	2919	2924	rVB3	53159	83027	0.96%	0.107%
85	20.633	2980	2983	2986	rVB4	27236	36019	0.42%	0.046%
86	20.692	2989	2993	2998	rBV	231356	307747	3.56%	0.396%
87	21.204	3075	3080	3087	rBV3	131074	282365	3.27%	0.364%
88	21.486	3122	3128	3137	rBV	3179109	4197968	48.55%	5.405%
89	21.816	3181	3184	3188	rBV2	54773	70614	0.82%	0.091%
90	23.174	3412	3415	3421	rVB4	101883	165706	1.92%	0.213%
91	23.751	3505	3513	3521	rBV2	3702998	7981841	92.31%	10.278%
92	23.910	3533	3540	3548	rVB	1879818	3978600	46.01%	5.123%


Sum of corrected areas: 77661894

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015967.D
Acq On : 19 Aug 2021 10:36
Operator : CG/JU
Sample : M3422-13
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

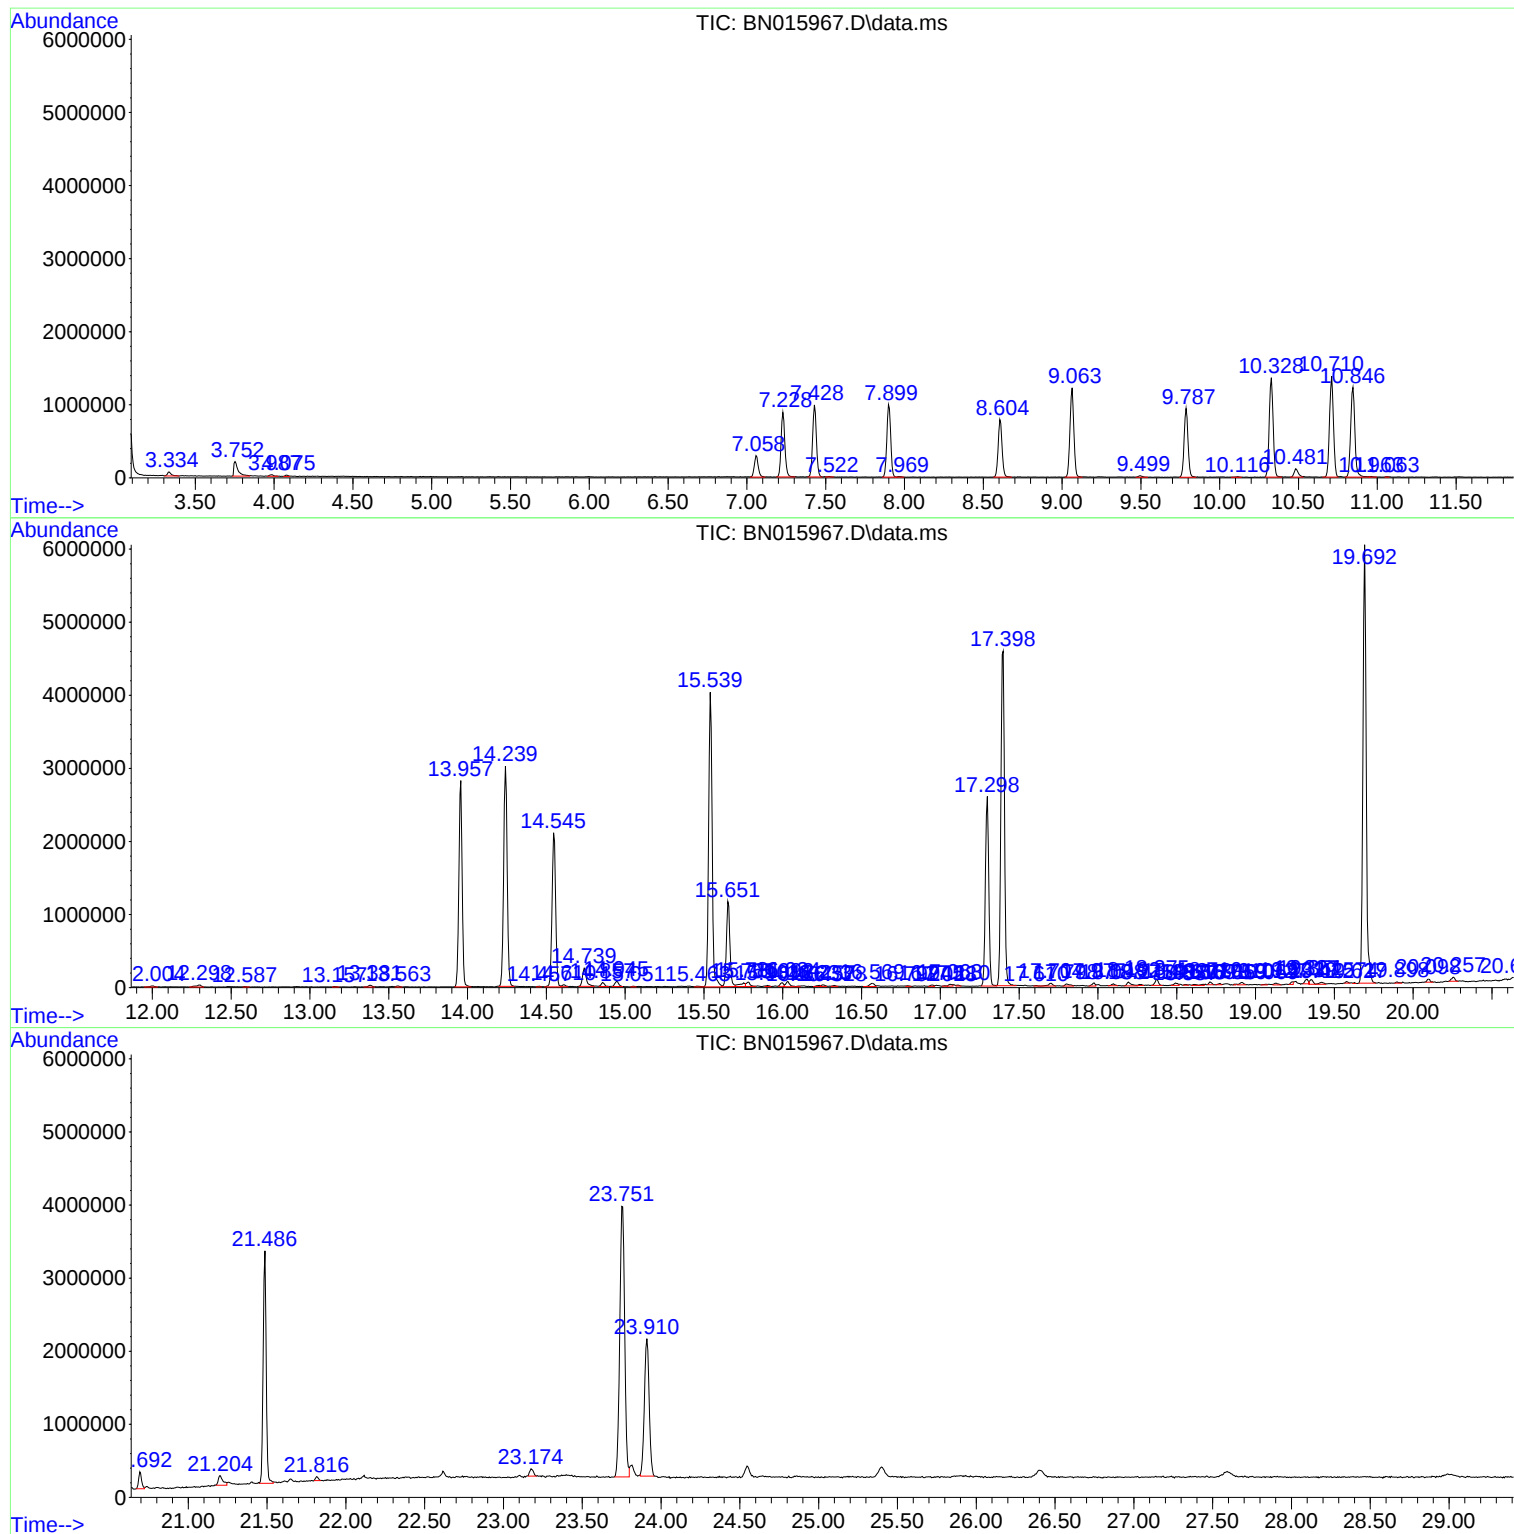

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015967.D
Acq On : 19 Aug 2021 10:36
Operator : CG/JU
Sample : M3422-13
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015967.D
Acq On : 19 Aug 2021 10:36
Operator : CG/JU
Sample : M3422-13
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
