

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015971.D
 Acq On : 19 Aug 2021 14:49
 Operator : CG/JU
 Sample : PB138520BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK520

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015971.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	36	40	50	rVB	83043	125519	1.63%	0.157%
2	3.734	107	110	129	rBV	1029639	1769265	22.91%	2.206%
3	3.946	144	146	150	rVB5	7161	9150	0.12%	0.011%
4	4.069	163	167	172	rVB4	15499	19264	0.25%	0.024%
5	5.069	335	337	342	rVB5	7962	10451	0.14%	0.013%
6	7.034	664	671	681	rVB	1345095	2244561	29.07%	2.799%
7	7.204	693	700	712	rBV	982609	1631661	21.13%	2.035%
8	7.310	716	718	722	rVB5	6190	9014	0.12%	0.011%
9	7.404	727	734	748	rBV	1347406	2288070	29.63%	2.853%
10	7.875	807	814	823	rVB	873106	1487660	19.27%	1.855%
11	8.581	927	934	944	rBV	1612637	2730404	35.36%	3.405%
12	9.034	1003	1011	1020	rBV	1295769	2183174	28.27%	2.722%
13	9.363	1064	1067	1068	rBV3	10628	8522	0.11%	0.011%
14	9.757	1127	1134	1143	rBV	1068587	1816580	23.53%	2.265%
15	10.293	1217	1225	1236	rBV	1582836	2715892	35.17%	3.387%
16	10.675	1280	1290	1299	rBV	1157491	2068110	26.78%	2.579%
17	10.810	1305	1313	1328	rBV	1628591	2933404	37.99%	3.658%
18	11.222	1380	1383	1390	rBV7	4900	8108	0.11%	0.010%
19	11.869	1490	1493	1495	rBV4	10230	13524	0.18%	0.017%
20	11.945	1501	1506	1507	rBV4	12027	16634	0.22%	0.021%
21	12.263	1553	1560	1565	rBV3	29135	49651	0.64%	0.062%
22	12.757	1635	1644	1653	rBV5	28466	79102	1.02%	0.099%
23	12.881	1658	1665	1671	rBV2	33464	70506	0.91%	0.088%
24	12.981	1678	1682	1685	rVB4	9234	11479	0.15%	0.014%
25	13.128	1703	1707	1711	rBV7	5465	10634	0.14%	0.013%
26	13.804	1818	1822	1825	rBV6	12053	20081	0.26%	0.025%
27	13.828	1825	1826	1830	rVB4	11685	12968	0.17%	0.016%
28	13.922	1835	1842	1853	rBV	2960780	4245075	54.98%	5.294%
29	14.110	1870	1874	1877	rVB6	5379	8975	0.12%	0.011%
30	14.204	1881	1890	1902	rVV	3180710	4806204	62.24%	5.993%
31	14.428	1920	1928	1932	rBV7	10379	17377	0.23%	0.022%
32	14.510	1935	1942	1954	rBV	1730271	2793049	36.17%	3.483%
33	14.704	1968	1975	1985	rBV	1470935	2192759	28.40%	2.734%
34	15.322	2073	2080	2088	rBV4	24753	57841	0.75%	0.072%
35	15.504	2104	2111	2119	rBV	4009445	5953085	77.09%	7.424%
36	15.616	2124	2130	2142	rBV	1316791	1900077	24.61%	2.369%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
 Data File : BN015971.D
 Acq On : 19 Aug 2021 14:49
 Operator : CG/JU
 Sample : PB138520BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK520

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

37	15.745	2146	2152	2156	rVV2	51162	83626	1.08%	0.104%
38	15.857	2167	2171	2172	rBV3	6189	9073	0.12%	0.011%
39	15.933	2182	2184	2191	rVB6	11537	15309	0.20%	0.019%
40	15.992	2191	2194	2201	rVB9	8044	12269	0.16%	0.015%
41	16.163	2218	2223	2231	rBV7	23146	52844	0.68%	0.066%
42	16.286	2241	2244	2249	rVB4	12296	17974	0.23%	0.022%
43	16.398	2260	2263	2267	rVB6	9325	12736	0.16%	0.016%
44	16.657	2303	2307	2313	rVB8	5628	12230	0.16%	0.015%
45	16.745	2319	2322	2323	rVV3	9061	7799	0.10%	0.010%
46	16.933	2350	2354	2359	rBV8	7495	9939	0.13%	0.012%
47	17.039	2368	2372	2375	rBV5	11018	15293	0.20%	0.019%
48	17.122	2382	2386	2388	rBV5	5918	10406	0.13%	0.013%
49	17.257	2401	2409	2416	rBV	2281670	3355231	43.45%	4.184%
50	17.357	2418	2426	2437	rBV	4516899	6562066	84.98%	8.183%
51	17.633	2468	2473	2474	rBV5	7705	9592	0.12%	0.012%
52	18.222	2572	2573	2578	rVB4	7343	9456	0.12%	0.012%
53	19.222	2735	2743	2746	rBV7	33363	59767	0.77%	0.075%
54	19.286	2750	2754	2761	rVB2	56019	84358	1.09%	0.105%
55	19.404	2770	2774	2776	rBV5	5906	9348	0.12%	0.012%
56	19.539	2793	2797	2800	rBV2	31797	38665	0.50%	0.048%
57	19.580	2803	2804	2808	rVB4	10527	8389	0.11%	0.010%
58	19.651	2810	2816	2828	rBV	5439191	7721311	99.99%	9.629%
59	20.127	2895	2897	2898	rBV2	8581	8517	0.11%	0.011%
60	20.657	2982	2987	2992	rBV	283736	358838	4.65%	0.447%
61	21.445	3116	3121	3128	rBV	2775022	3798615	49.19%	4.737%
62	23.692	3495	3503	3511	rBV	3676283	7721779	100.00%	9.629%
63	23.851	3522	3530	3539	rVB	1853347	3867672	50.09%	4.823%


Sum of corrected areas: 80190932

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015971.D
Acq On : 19 Aug 2021 14:49
Operator : CG/JU
Sample : PB138520BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK520

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

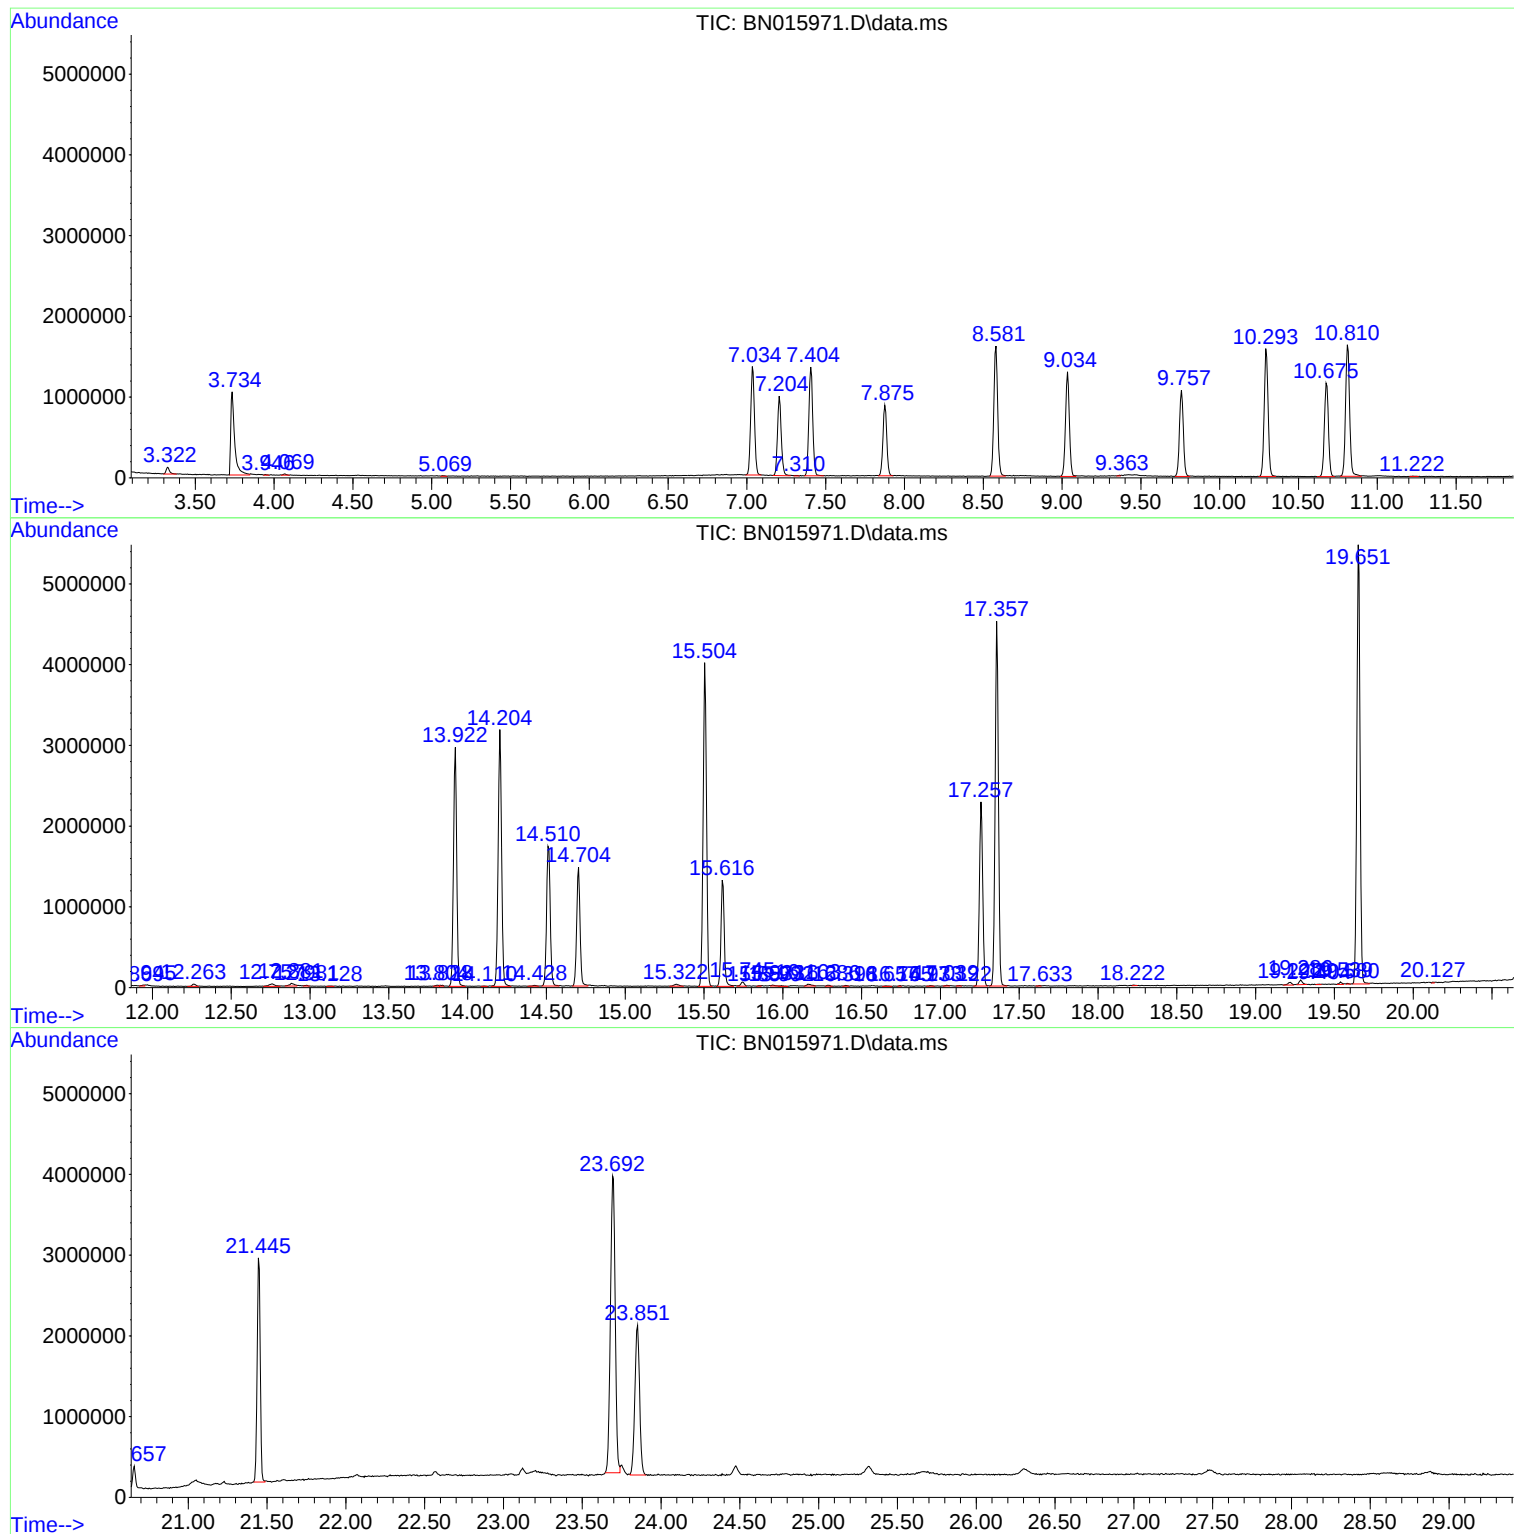

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015971.D
Acq On : 19 Aug 2021 14:49
Operator : CG/JU
Sample : PB138520BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK520

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015971.D
Acq On : 19 Aug 2021 14:49
Operator : CG/JU
Sample : PB138520BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK520

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
