
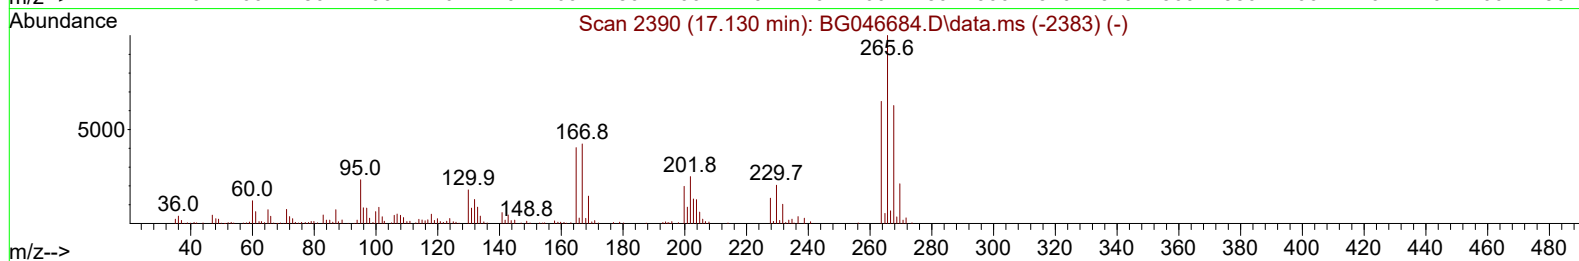
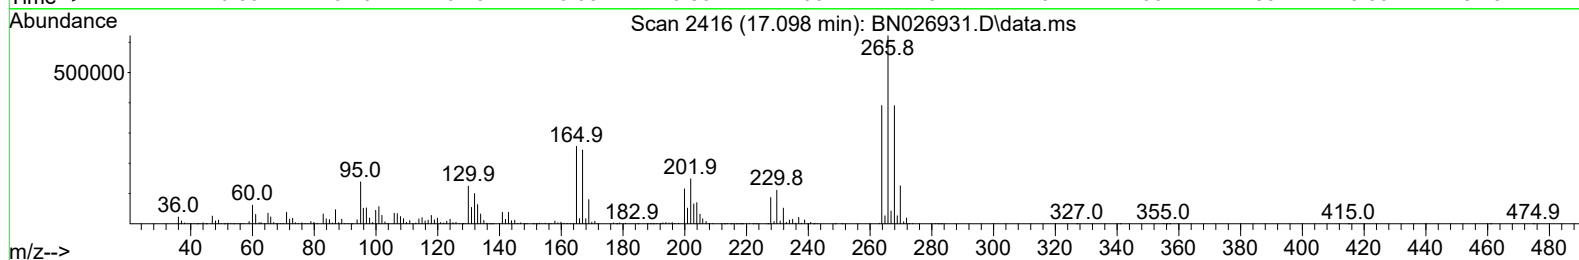


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081723\
Data File : BN026931.D
Acq On : 17 Aug 2023 07:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 04:48:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 18 04:48:11 2023
Response via : Initial Calibration

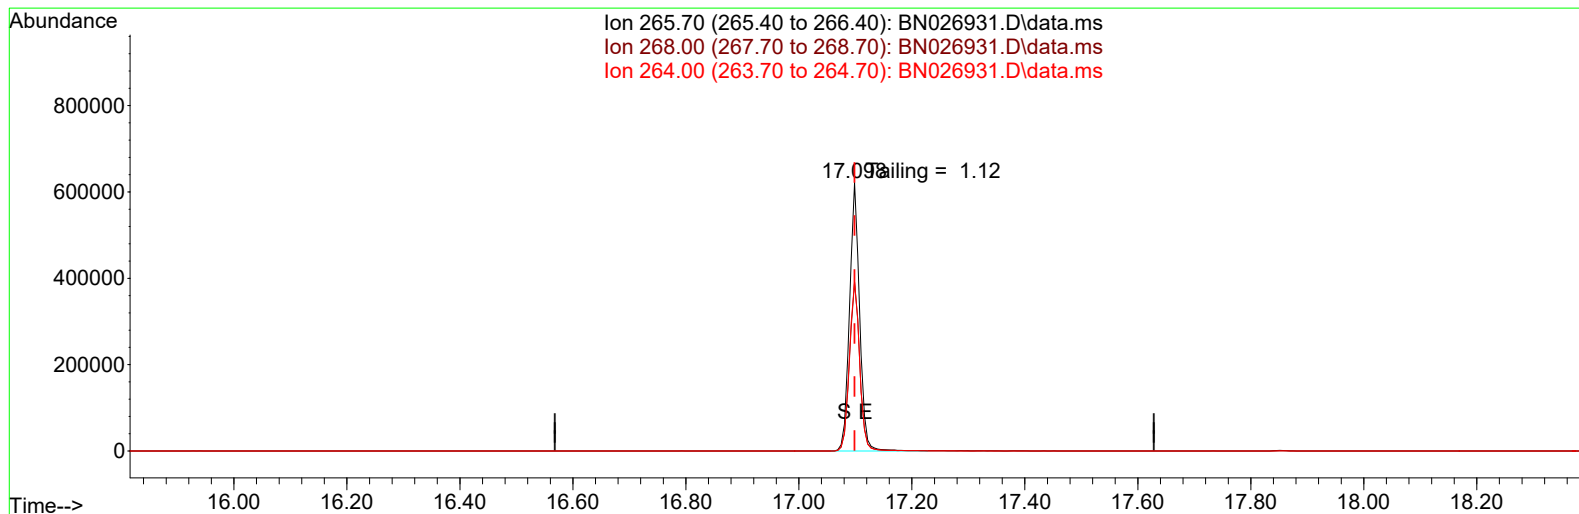

TIC: BN026931.D\data.ms

(70) Pentachlorophenol (C)




17.098min (0.000) 27355.81 ng

response 773068

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.86
264.00	61.60	62.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081723\
 Data File : BN026931.D
 Acq On : 17 Aug 2023 07:54
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 04:48:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 18 04:48:11 2023
 Response via : Initial Calibration

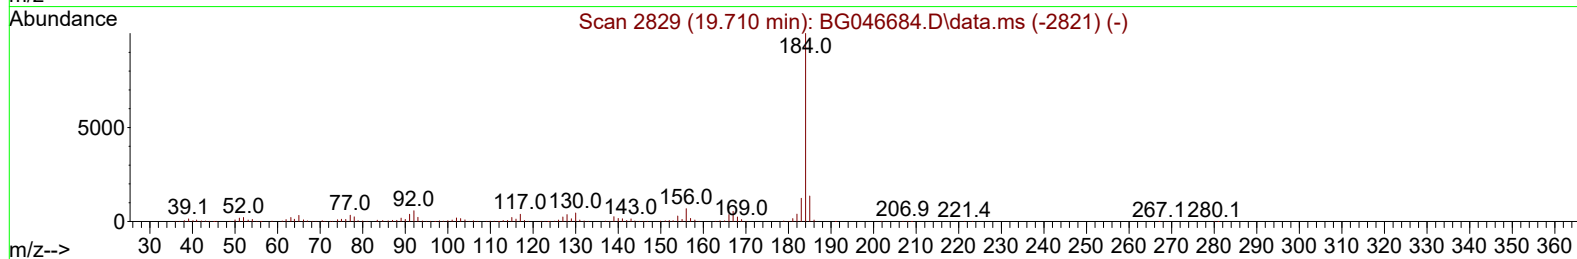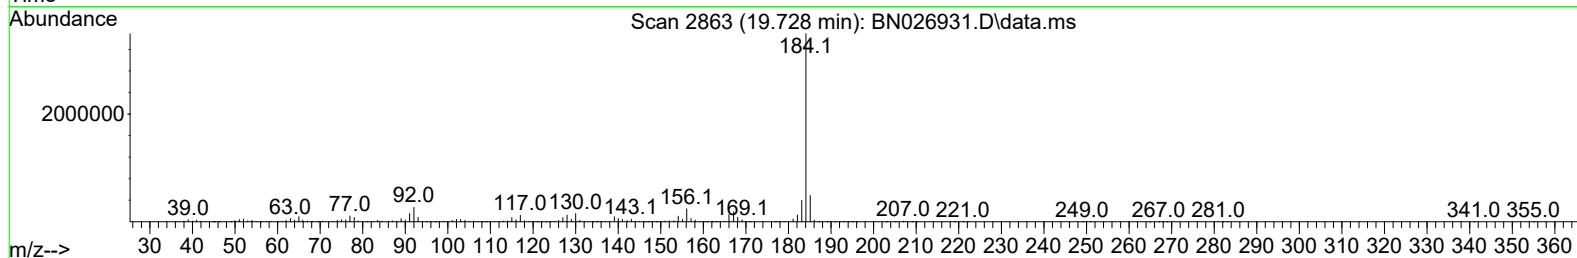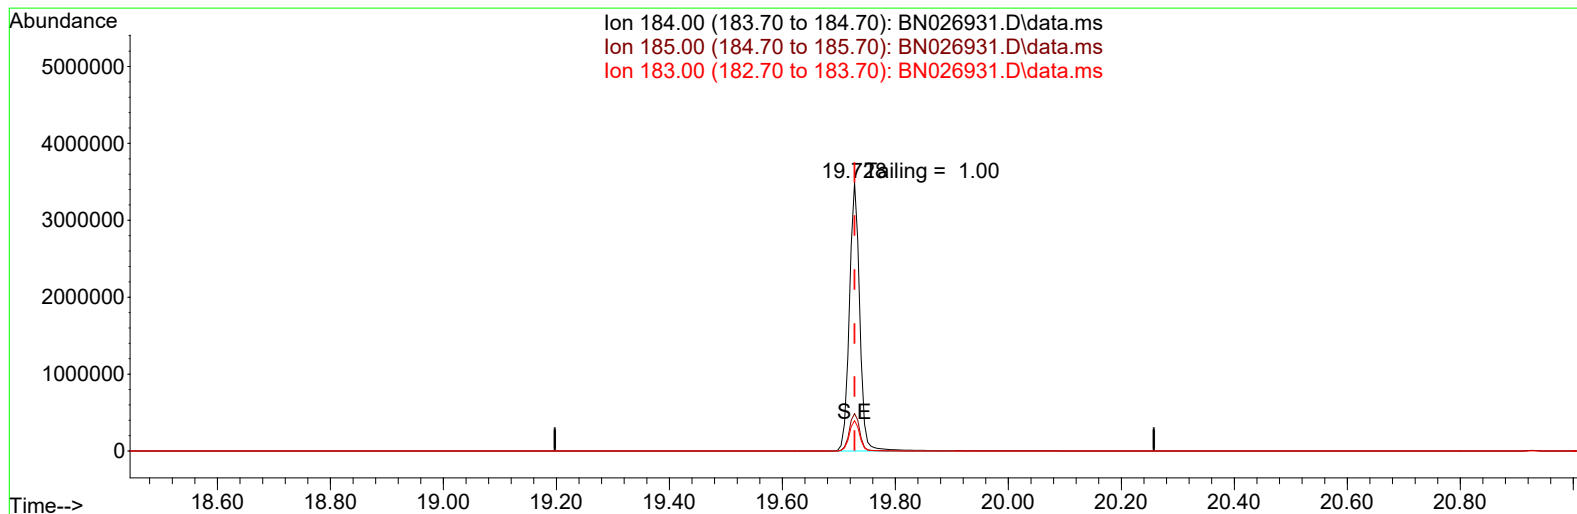

TIC: BN026931.D\data.ms

(77) Benzidine**19.728min (0.000) 2634059.81 ng****response 4465773**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.99
183.00	13.20	11.34
0.00	0.00	0.00