
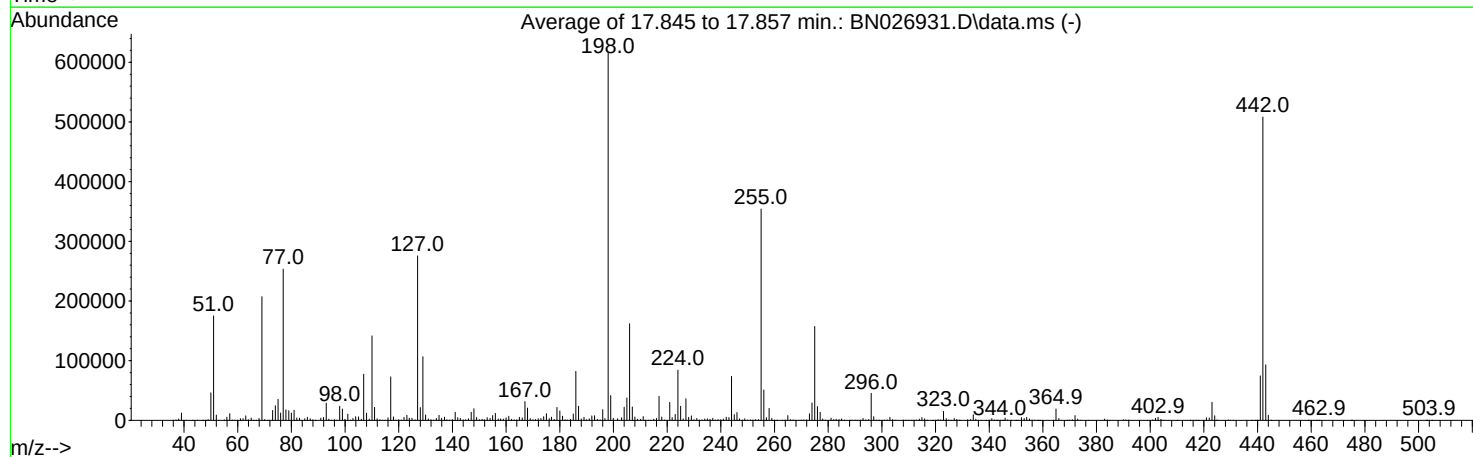


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081723\
Data File : BN026931.D
Acq On : 17 Aug 2023 07:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 16 15:56:02 2023

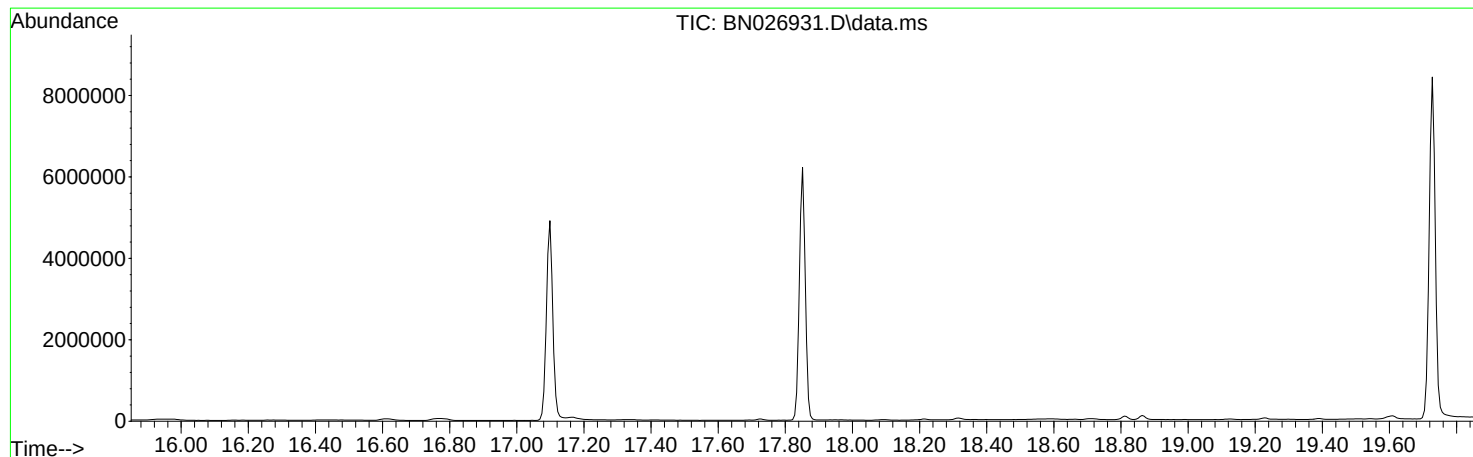




Spectrum Information: Average of 17.845 to 17.857 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.4	175199	PASS
68	69	0.00	2	1.6	3334	PASS
69	198	0.00	100	33.6	207388	PASS
70	69	0.00	2	0.6	1265	PASS
127	198	10	80	44.7	275499	PASS
197	198	0.00	2	0.5	3069	PASS
198	198	100	100	100.0	616363	PASS
199	198	5	9	6.7	41597	PASS
275	198	10	60	25.5	157461	PASS
365	198	1	100	3.1	19053	PASS
441	198	0.01	100	12.1	74501	PASS
442	442	50	100	100.0	508395	PASS
443	442	15	24	18.3	93008	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081723\
Data File : BN026931.D
Acq On : 17 Aug 2023 07:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 18 04:48:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 18 04:48:11 2023
Response via : Initial Calibration

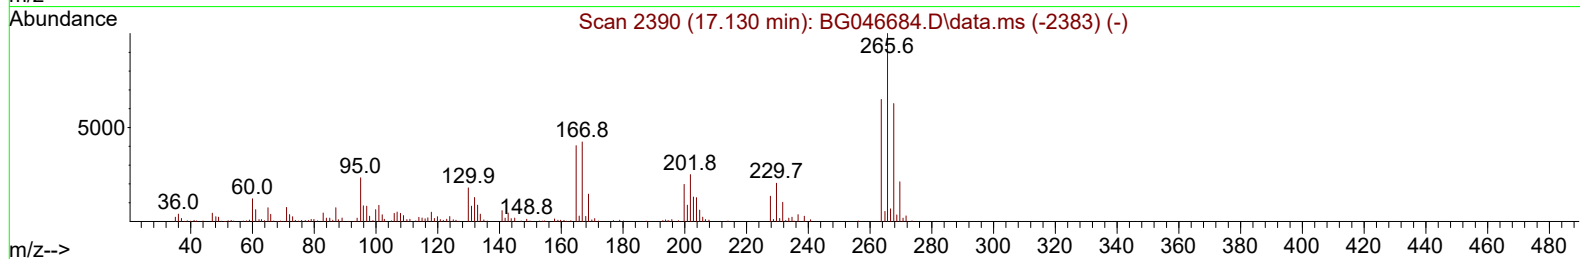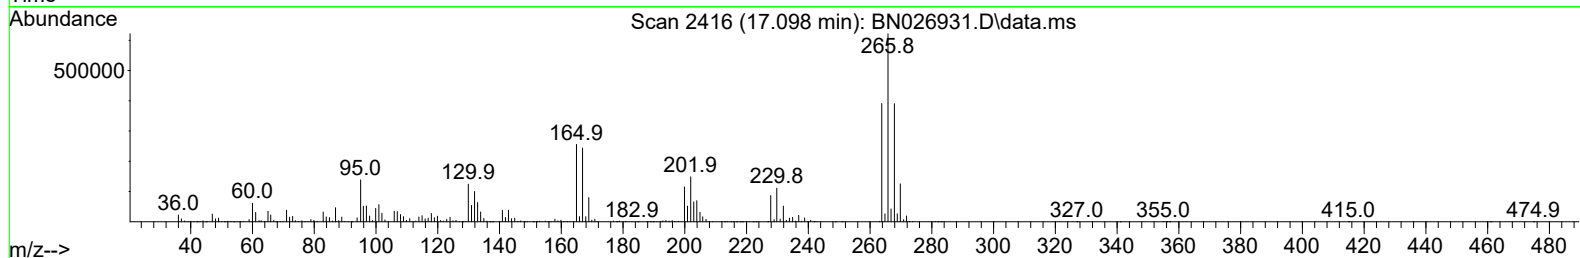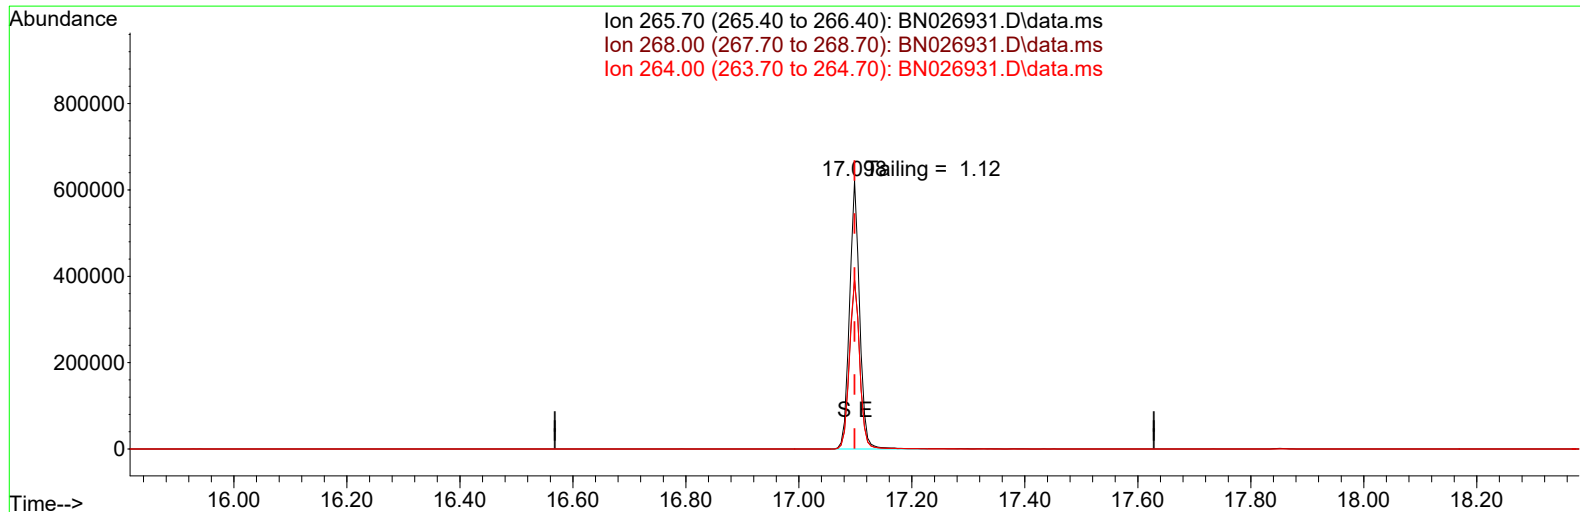

TIC: BN026931.D\data.ms

(70) Pentachlorophenol (C)

17.098min (0.000) 27355.81 ng




response 773068

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.86
264.00	61.60	62.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081723\
 Data File : BN026931.D
 Acq On : 17 Aug 2023 07:54
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Aug 18 04:48:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 18 04:48:11 2023
 Response via : Initial Calibration

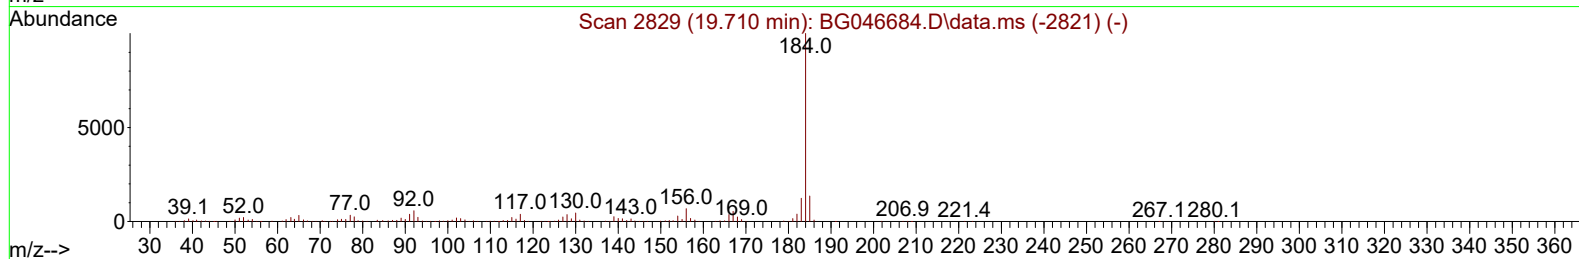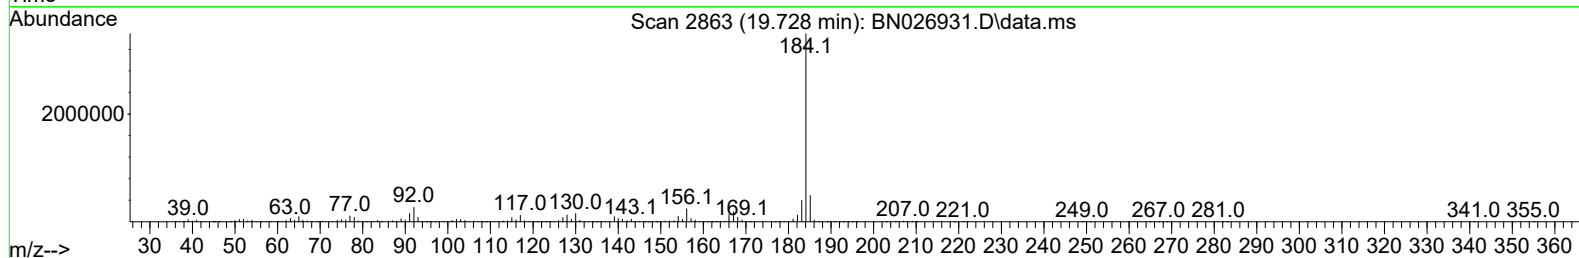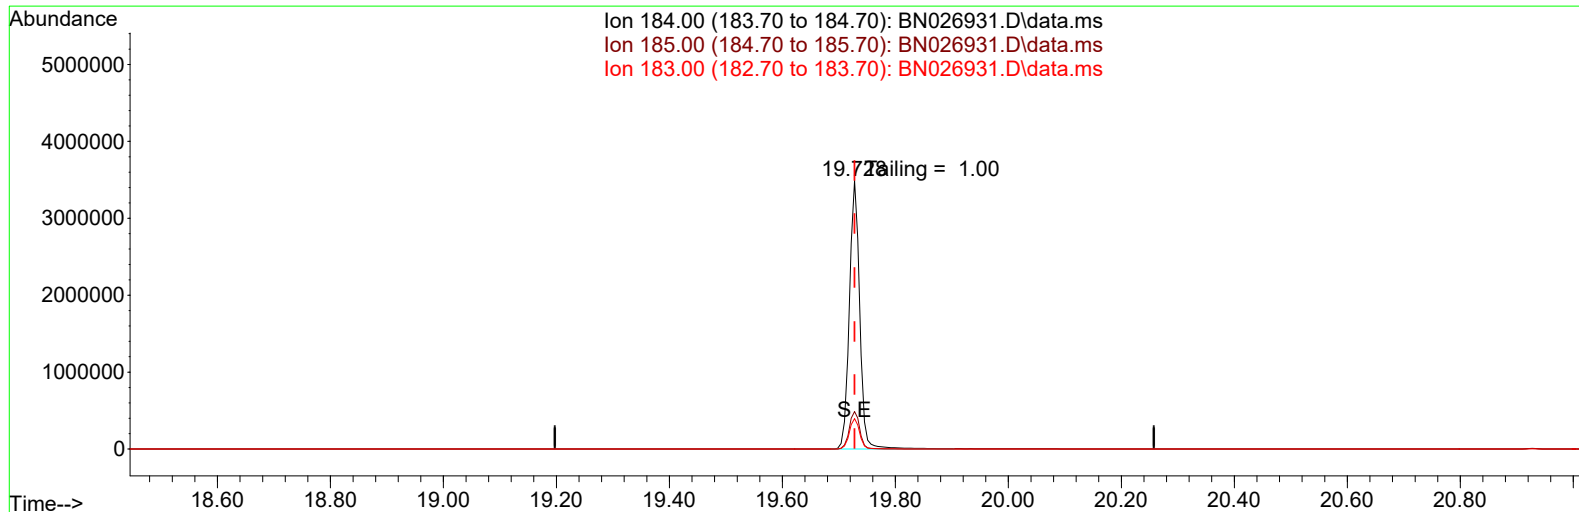

TIC: BN026931.D\data.ms

(77) Benzidine

19.728min (0.000) 2634059.81 ng

response 4465773

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.99
183.00	13.20	11.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/17/2023	BNA_N	<u>BN026931.D</u>
Compound Name	Response	Retention Time
DDT	2120507	20.928
DDD	20802	20.539
DDE	606	19.969
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21408	2141915	1.00

Instrument :
BNA_N
ClientSampleId :
DFTPP