

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081823\
 Data File : BN026959.D
 Acq On : 18 Aug 2023 14:55
 Operator : MA/JU
 Sample : PB154872BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK872

Quant Time: Aug 18 17:22:12 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 18 13:11:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.105	152	7186	0.400	ng/ul	0.00
4) Naphthalene-d8	10.927	136	22819	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.731	164	13598	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.476	188	29965	0.400	ng/ul	0.00
17) Chrysene-d12	21.656	240	22222	0.400	ng/ul	0.00
23) Perylene-d12	24.202	264	26158	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.439	96	54257	6.360	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.506	152	8525	0.254	ng/ul	0.00
18) Fluoranthene-d10	19.492	212	21989	0.313	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.859	202	3731	0.038	ng/ul#	1
26) Benzo(a)pyrene	24.035	252	8030	0.090	ng/ul#	42


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081823\
Data File : BN026959.D
Acq On : 18 Aug 2023 14:55
Operator : MA/JU
Sample : PB154872BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK872

Quant Time: Aug 18 17:22:12 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 18 13:11:26 2023
Response via : Initial Calibration

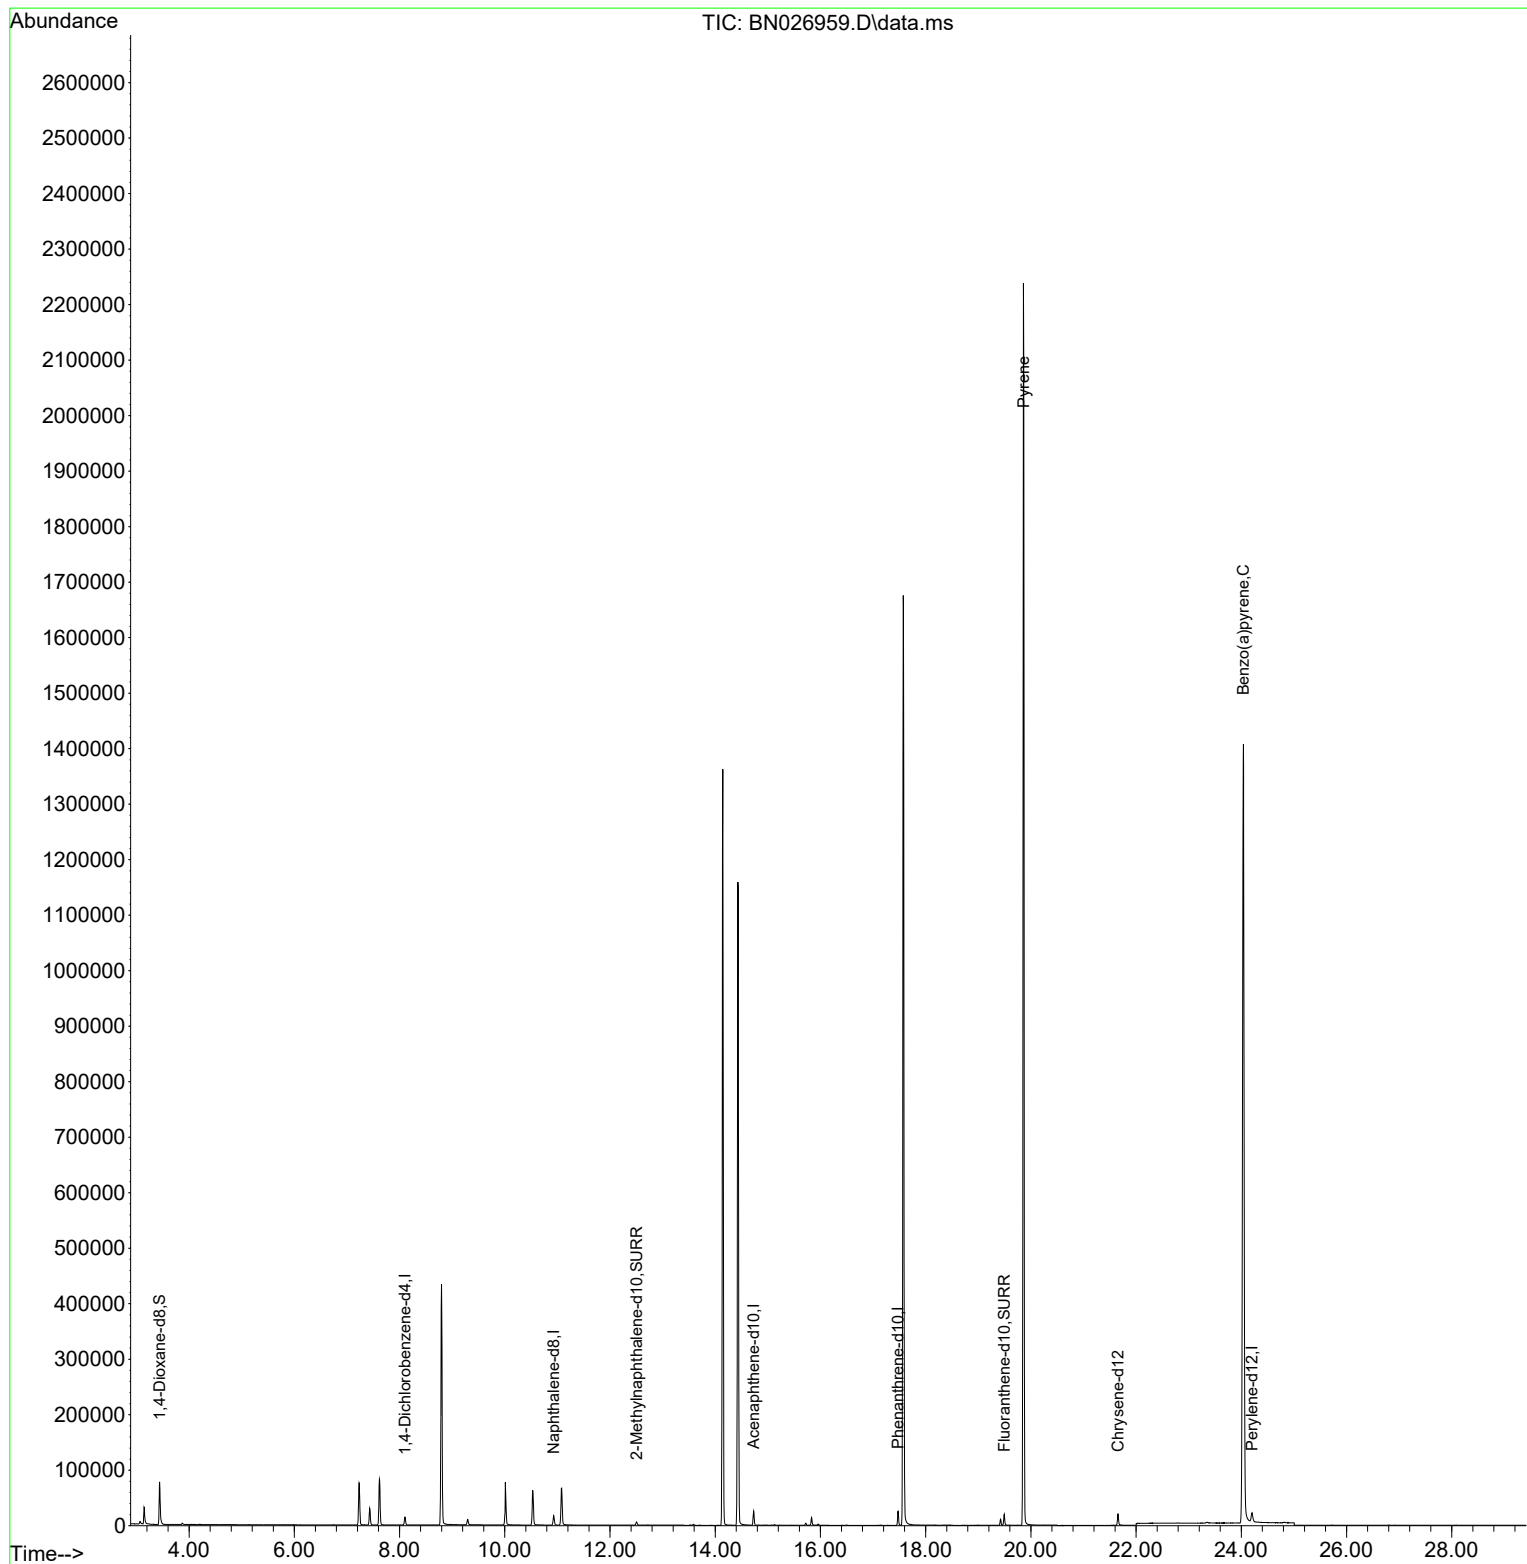

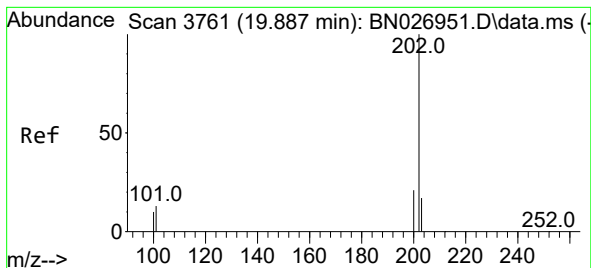

#20

Pyrene

Concen: 0.038 ng/ul

RT: 19.859 min Scan# 3761

Delta R.T. -0.028 min

Lab File: BN026959.D

Acq: 18 Aug 2023 14:55

Instrument :

BNA_N

ClientSampleId :

SBLK872





Tgt Ion:202 Resp: 3731

Ion Ratio Lower Upper

202 100

101 158.7 10.7 16.1#

100 1196.5 8.5 12.7#

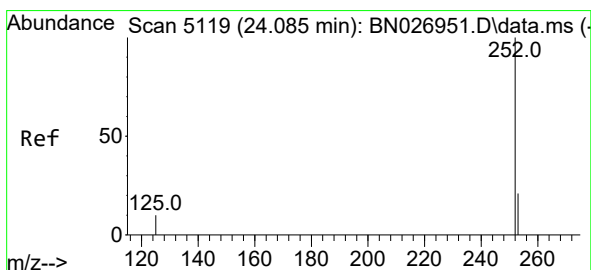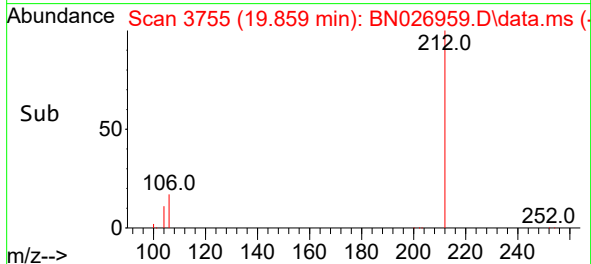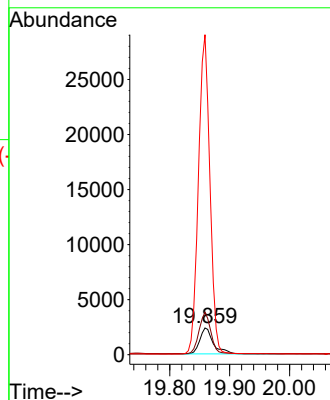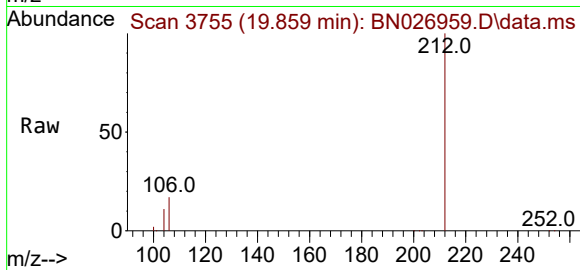

#26

Benzo(a)pyrene

Concen: 0.090 ng/ul

RT: 24.035 min Scan# 5102

Delta R.T. -0.050 min

Lab File: BN026959.D

Acq: 18 Aug 2023 14:55

Tgt Ion:252 Resp: 8030

Ion Ratio Lower Upper

252 100

253 40.8 19.0 28.6#

125 53.7 11.4 17.0#

