
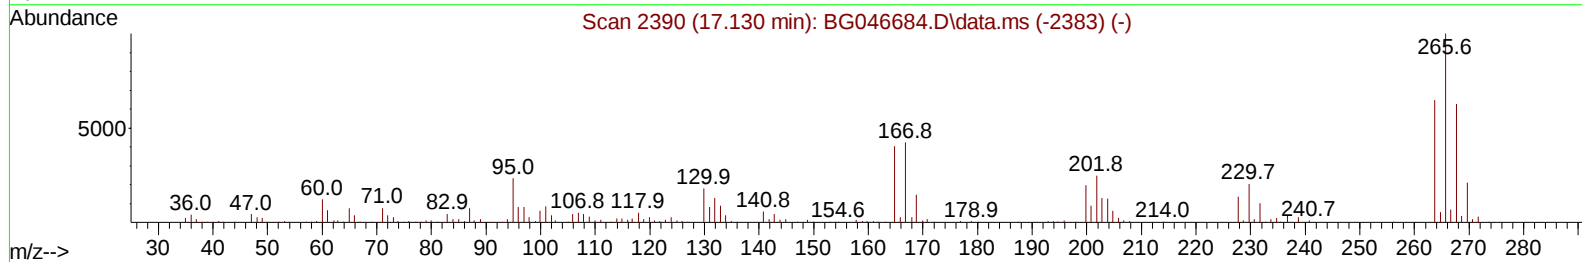
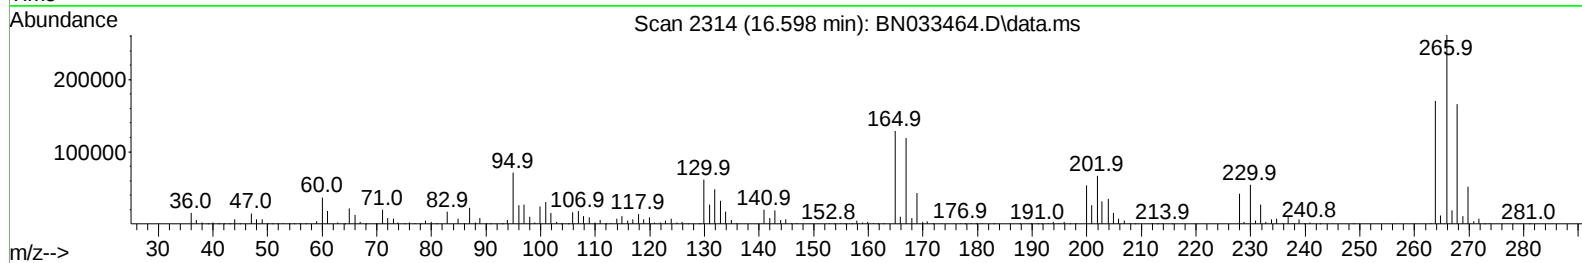


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081824\
Data File : BN033464.D
Acq On : 17 Aug 2024 12:05
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 38 Sample Multiplier: 1

Quant Time: Aug 18 00:33:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 18 00:33:21 2024
Response via : Initial Calibration

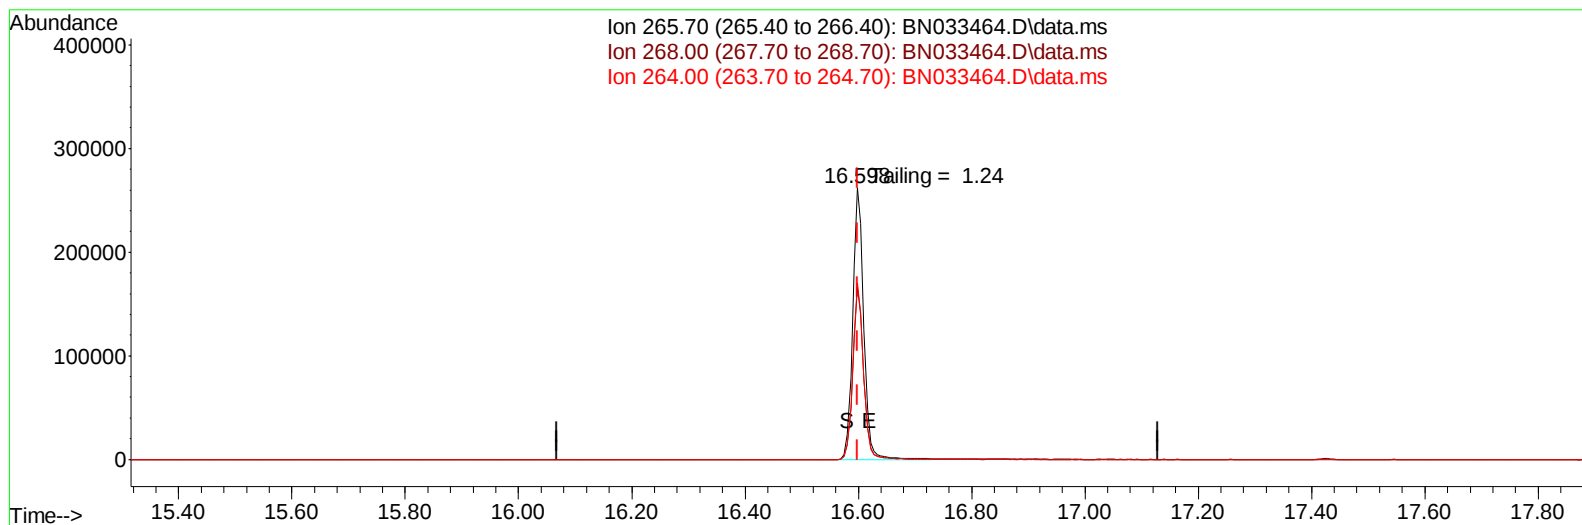




TIC: BN033464.D\data.ms

(70) Pentachlorophenol (C)**16.598min (0.000) 21414.02 ng****response 356438**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.53
264.00	61.60	64.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081824\
Data File : BN033464.D
Acq On : 17 Aug 2024 12:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 38 Sample Multiplier: 1

Quant Time: Aug 18 00:33:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 18 00:33:21 2024
Response via : Initial Calibration

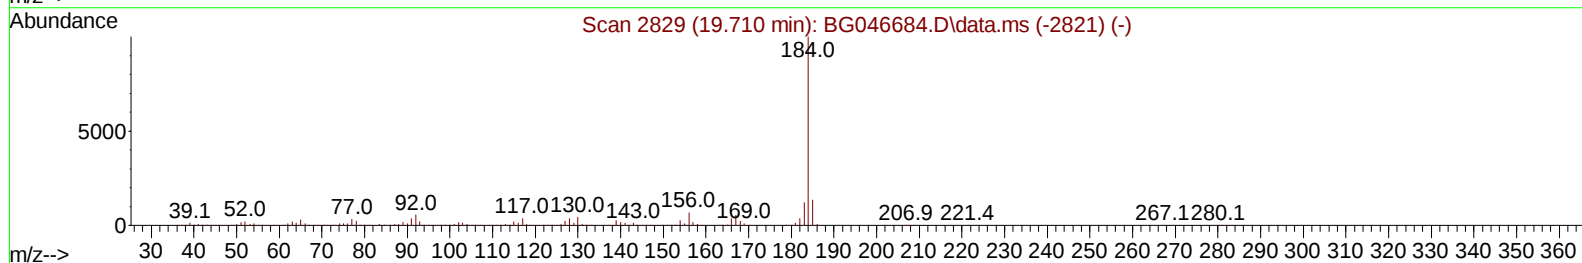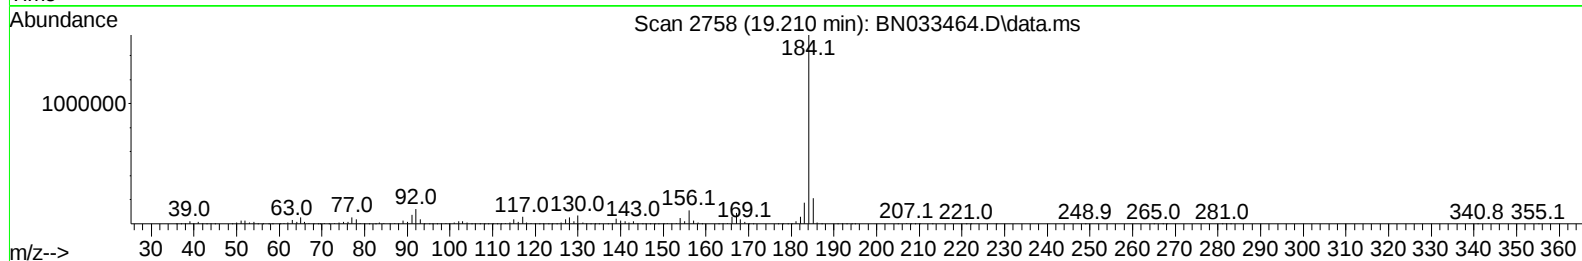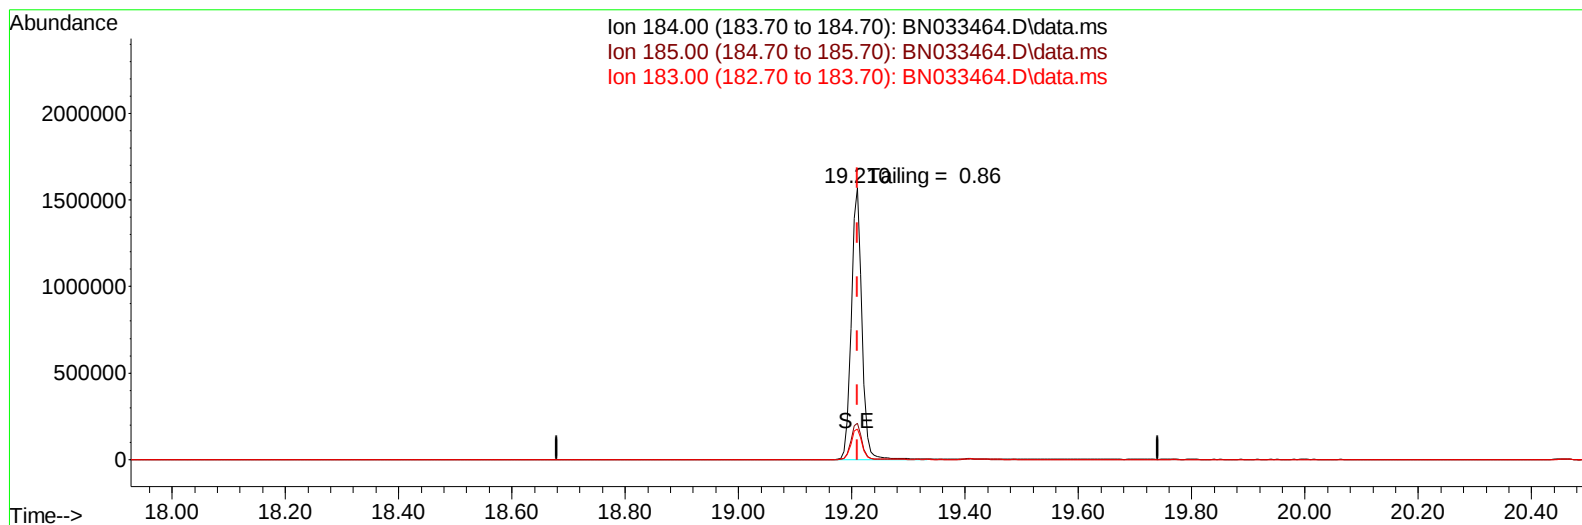

TIC: BN033464.D\data.ms

(77) Benzidine

19.210min (0.000) 0.00 ng

response 2051415

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.42
183.00	13.20	11.26
0.00	0.00	0.00