

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082018\
Data File : BN002432.D
Acq On : 20 Aug 2018 20:46
Operator : JU/SJ
Sample : J4514-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0324

Manual Integrations
APPROVED

Sohil
8/21/2018 4:47:22 PM

Quant Time: Aug 21 03:51:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 21 01:54:59 2018
Response via : Initial Calibration

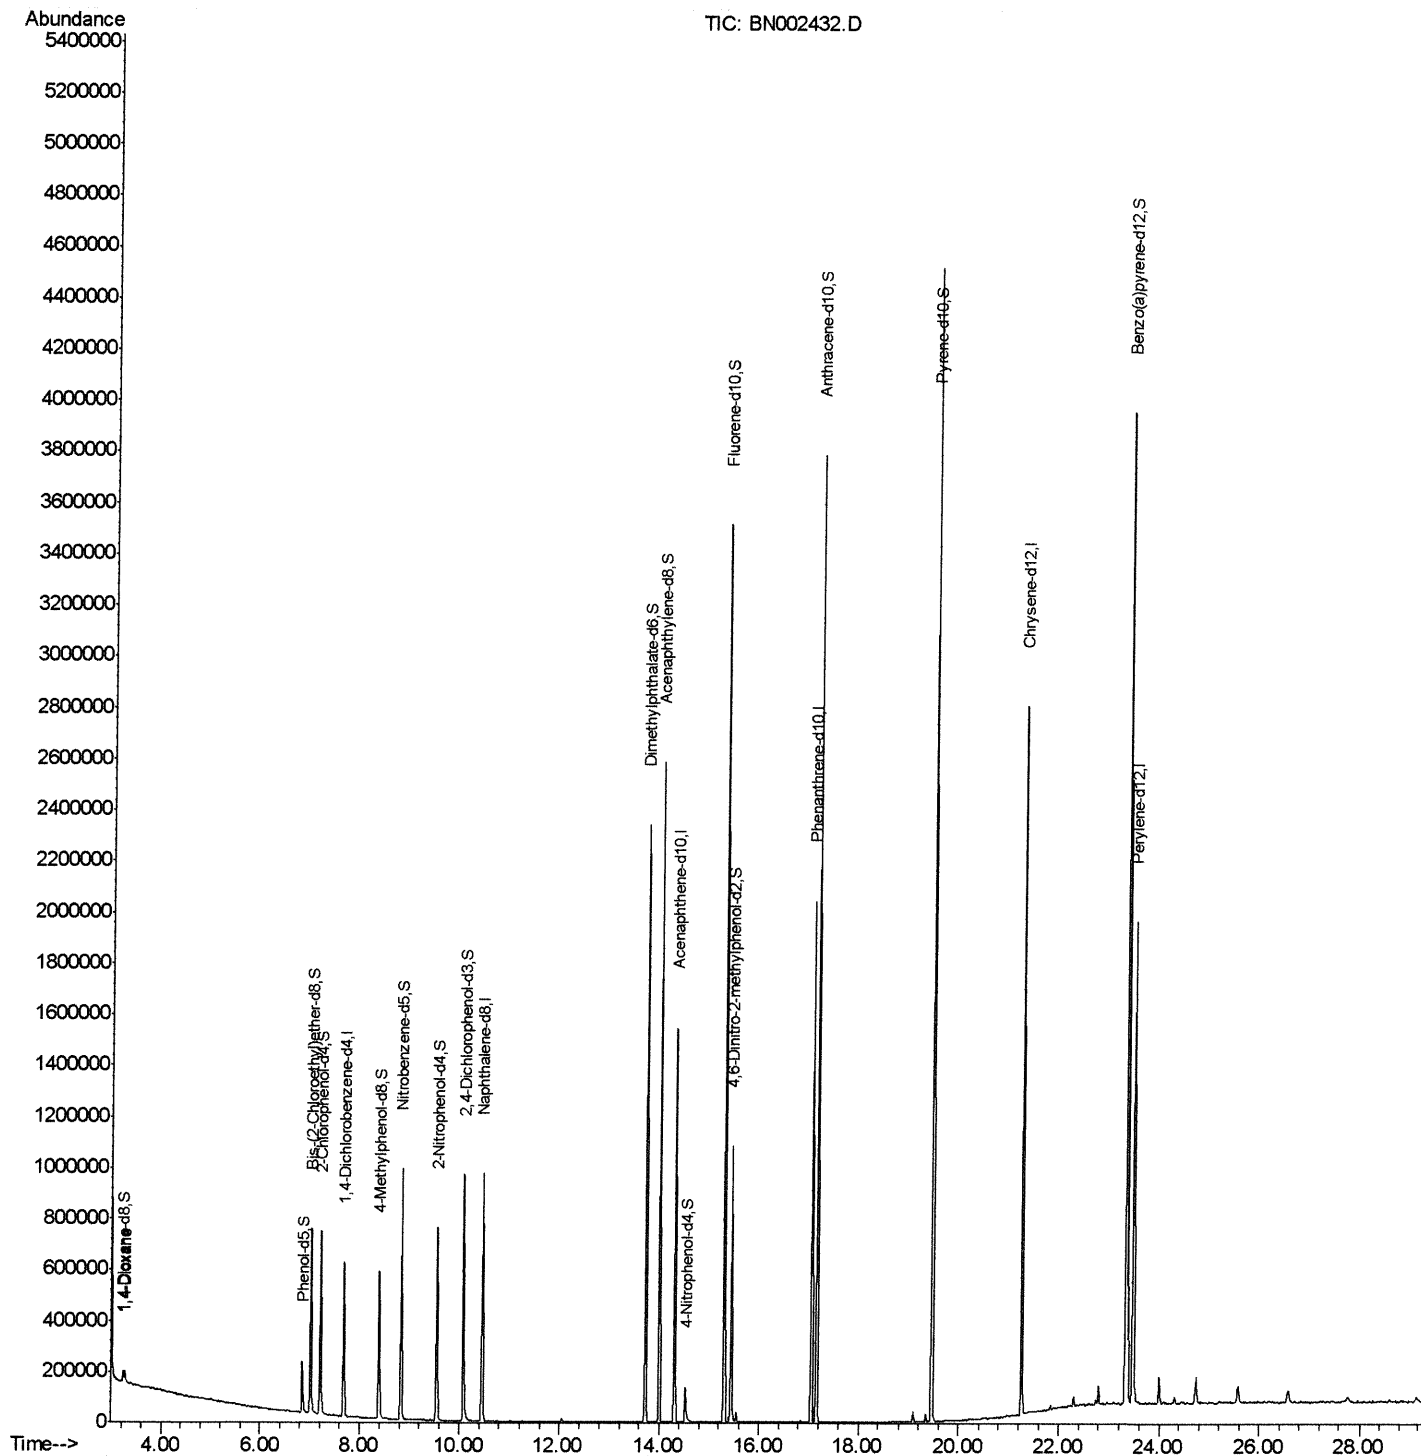

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082018\
 Data File : BN002432.D
 Acq On : 20 Aug 2018 20:46
 Operator : JU/SJ
 Sample : J4514-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 C0324

Manual Integrations
 APPROVED

Sohil
 8/21/2018 4:47:22 PM

Quant Time: Aug 21 01:56:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 21 01:54:59 2018
 Response via : Initial Calibration

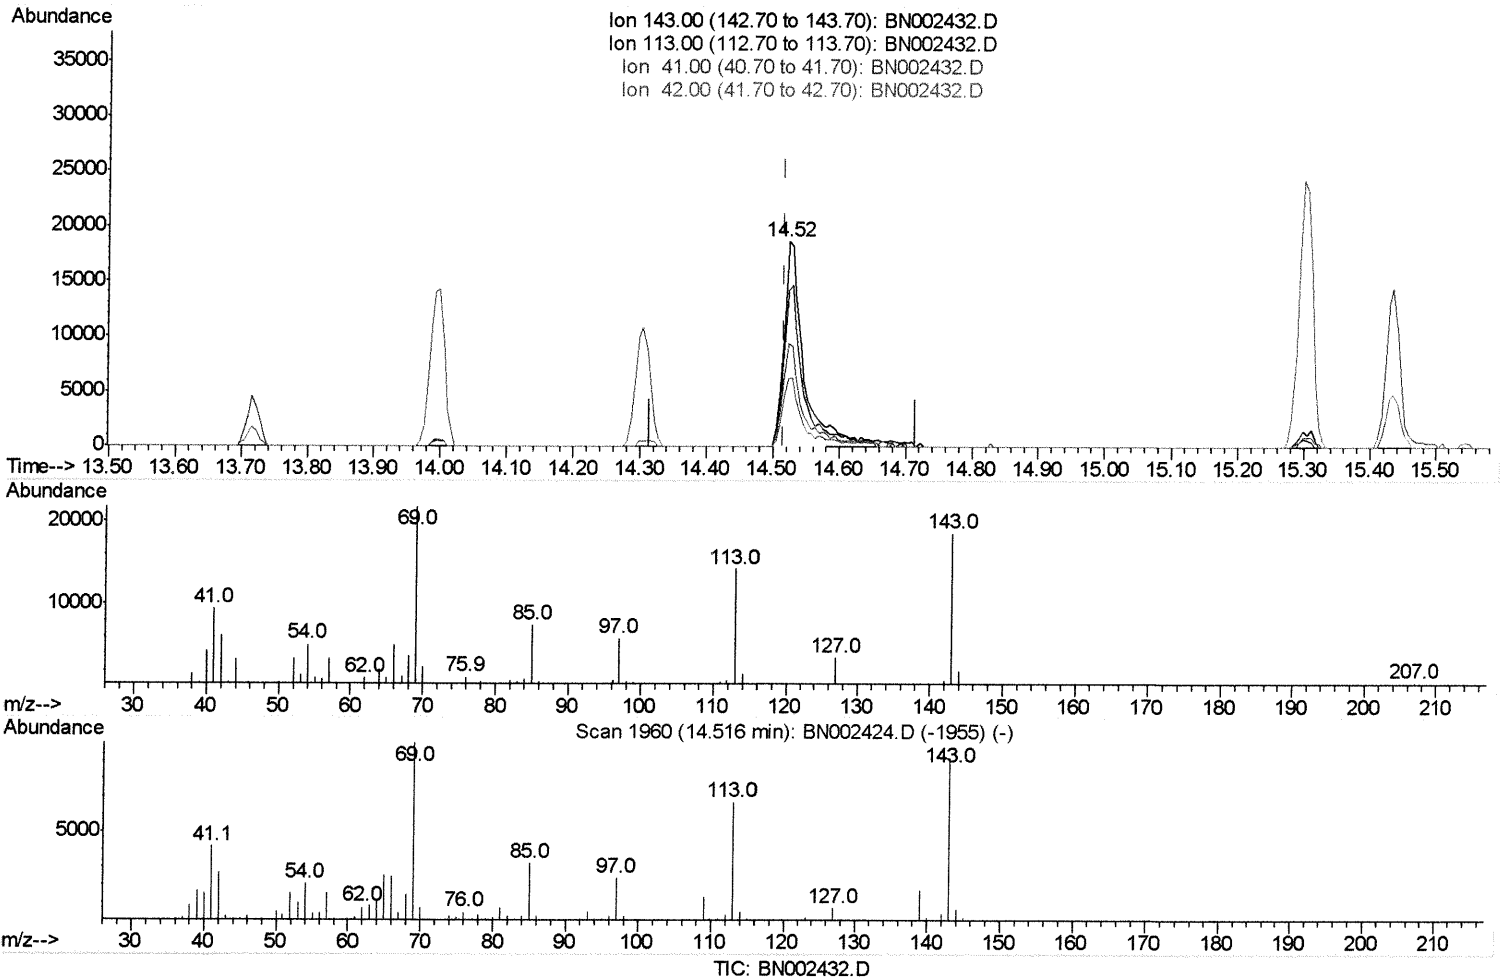

(51) 4-Nitrophenol-d4 (S)
 14.522min (+0.006) 4.56ng/ul
 response 35218

Ion	Exp%	Act%
143.00	100	100
113.00	75.10	76.44
41.00	28.80	50.40#
42.00	19.10	33.28#

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082018\
 Data File : BN002432.D
 Acq On : 20 Aug 2018 20:46
 Operator : JU/SJ
 Sample : J4514-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 C0324

Manual Integrations
 APPROVED

Sohil
 8/21/2018 4:47:22 PM

Quant Time: Aug 21 01:56:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 21 01:54:59 2018
 Response via : Initial Calibration

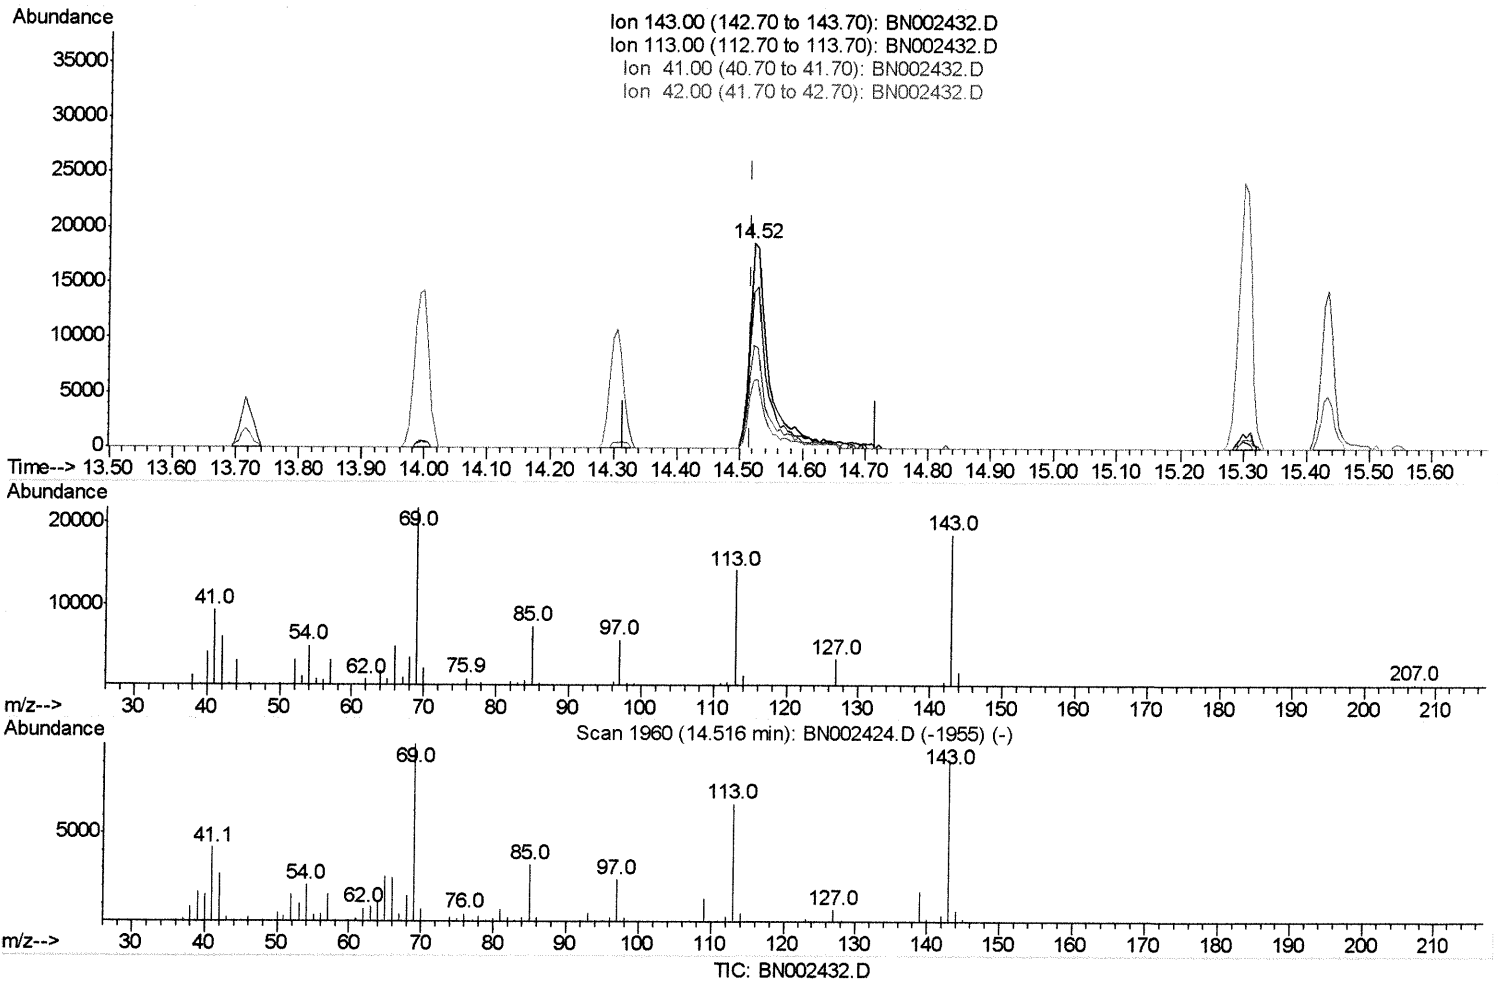

(51) 4-Nitrophenol-d4 (S)

14.522min (+0.006) 5.27ng/ul m

SJ 8/22/18

response 40666

Ion	Exp%	Act%
143.00	100	100
113.00	75.10	76.44
41.00	28.80	50.40#
42.00	19.10	33.28#

Quantitation Report (QT Reviewed)

Instrument :
BNA_N
ClientSampleId :
C0324

Manual Integrations
APPROVED

Sohil
8/21/2018 4:47:22 PM

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082018\
Data File : BN002432.D
Acq On : 20 Aug 2018 20:46
Operator : JU/SJ
Sample : J4514-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Aug 21 03:51:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 21 01:54:59 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	159631	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	772444	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	492436	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	1145656	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1263165	20.00	ng/ul	0.00
85) Perylene-d12	23.47	264	1304617	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	20370	6.02	ng/uL	0.00
5) Phenol-d5	6.85	99	116518	7.96	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	340536	37.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	322580	28.93	ng/ul	0.00
13) 4-Methylphenol-d8	8.38	113	215828	18.44	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	221301	35.99	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	235687	36.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	374341	31.51	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	1498088	36.70	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	1827756	36.50	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	40666m	5.27	ng/ul	0.00
57) Fluorene-d10	15.30	176	1328709	37.54	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	211160	28.95	ng/ul	0.00
70) Anthracene-d10	17.15	188	2080675	38.02	ng/ul	0.00
78) Pyrene-d10	19.45	212	2334883	38.63	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	2608805	38.24	ng/ul	0.00

5/8/22/18

Target Compounds				Ovalue
2) 1,4-Dioxane	3.27	88	23019	6.362 ng/uL 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed