

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082018\
Data File : BN002442.D
Acq On : 21 Aug 2018 02:38
Operator : JU/SJ
Sample : J4514-12
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0341

Manual Integrations
APPROVED

Sohil
8/21/2018 4:47:43 PM

Quant Time: Aug 21 06:52:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 21 04:38:31 2018
Response via : Initial Calibration

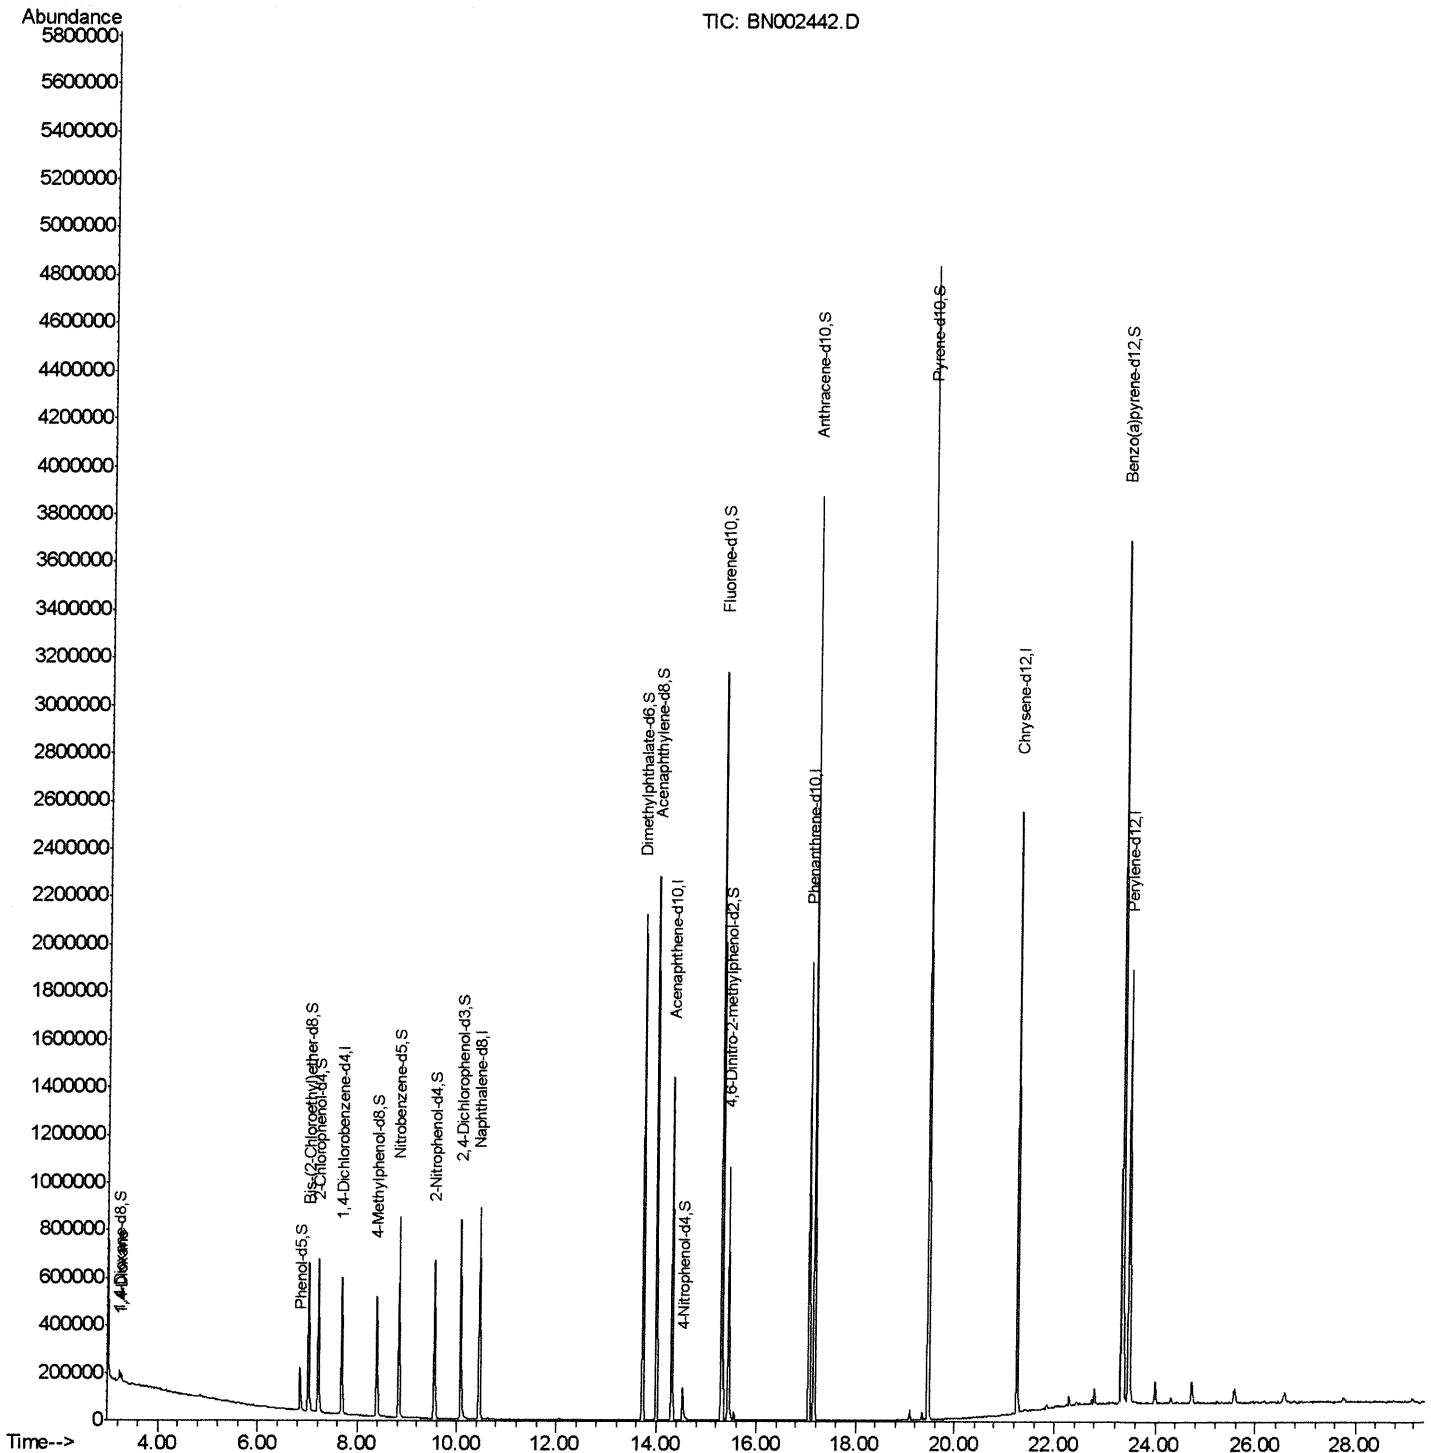

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082018\
 Data File : BN002442.D
 Acq On : 21 Aug 2018 02:38
 Operator : JU/SJ
 Sample : J4514-12
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 C0341

Manual Integrations
 APPROVED

Sohil
 8/21/2018 4:47:43 PM

Quant Time: Aug 21 06:47:27 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 21 04:38:31 2018
 Response via : Initial Calibration

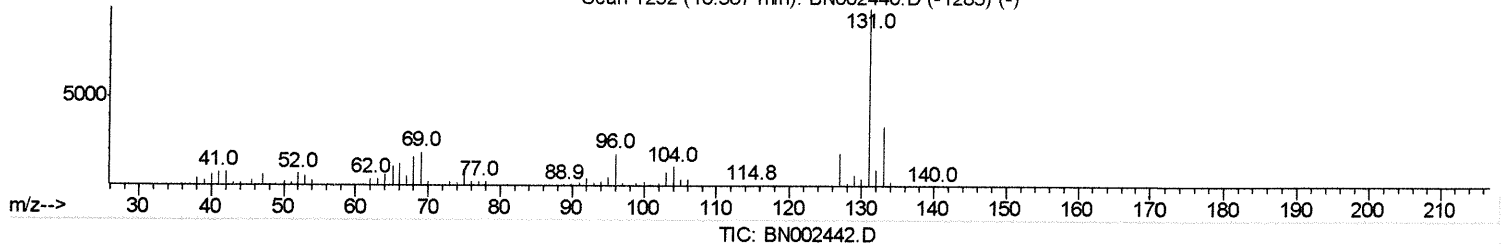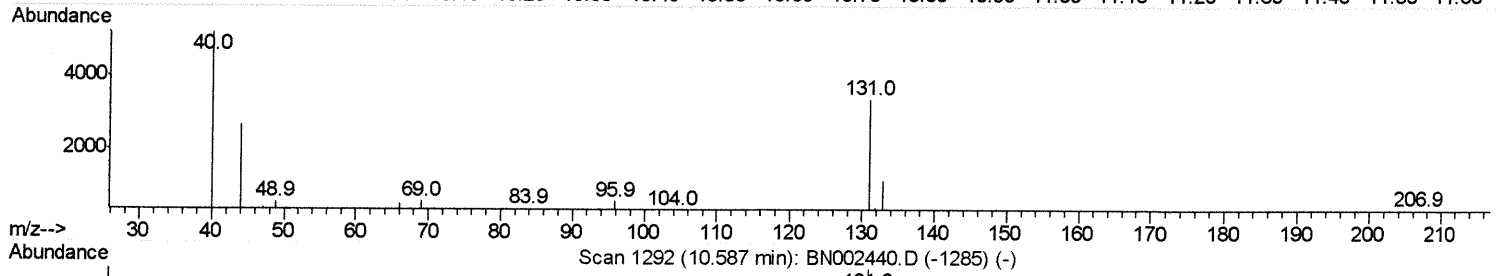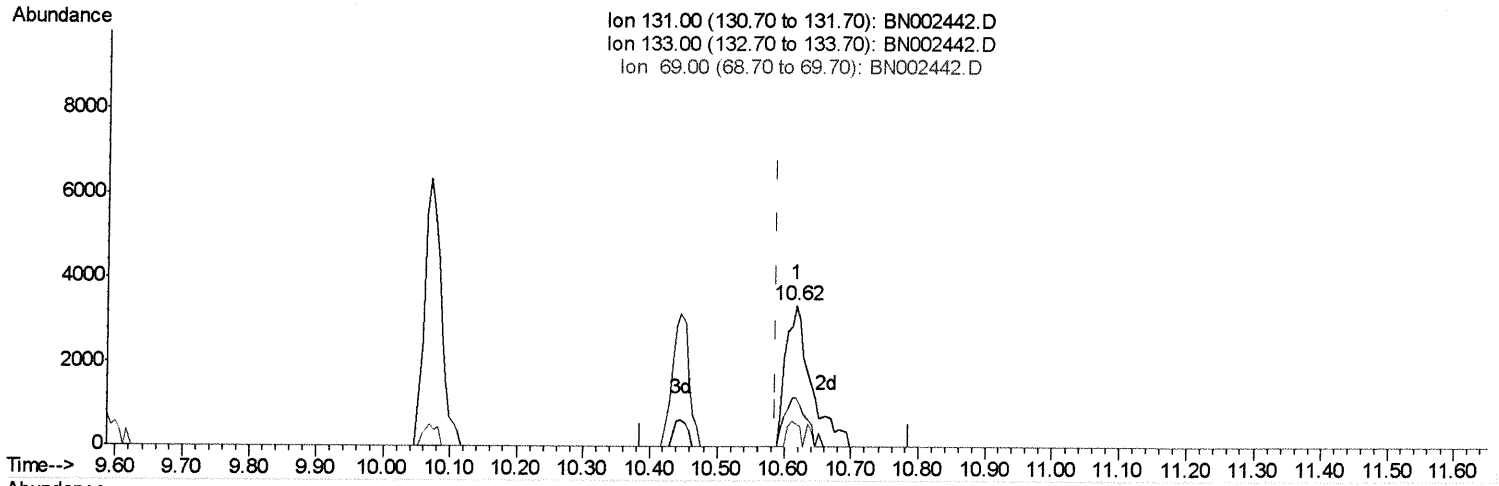

(29) 4-Chloroaniline-d4 (S)
 10.616min (+0.029) 0.64ng/ul
 response 7720

Ion	Exp%	Act%
131.00	100	100
133.00	32.10	34.16
69.00	16.20	16.53
0.00	0.00	0.00

Instrument :
BNA_N
ClientSampleId :
C0341

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082018\

Data File : BN002442.D

Acq On : 21 Aug 2018 02:38

Operator : JU/SJ

Sample : J4514-12

Misc :

ALS Vial : 30 Sample Multiplier: 1

Quant Time: Aug 21 06:47:27 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-BN081318MA.M



Quant Title : SVOA CALIBRATION

QLast Update : Tue Aug 21 04:38:31 2018

Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
8/21/2018 4:47:43 PM

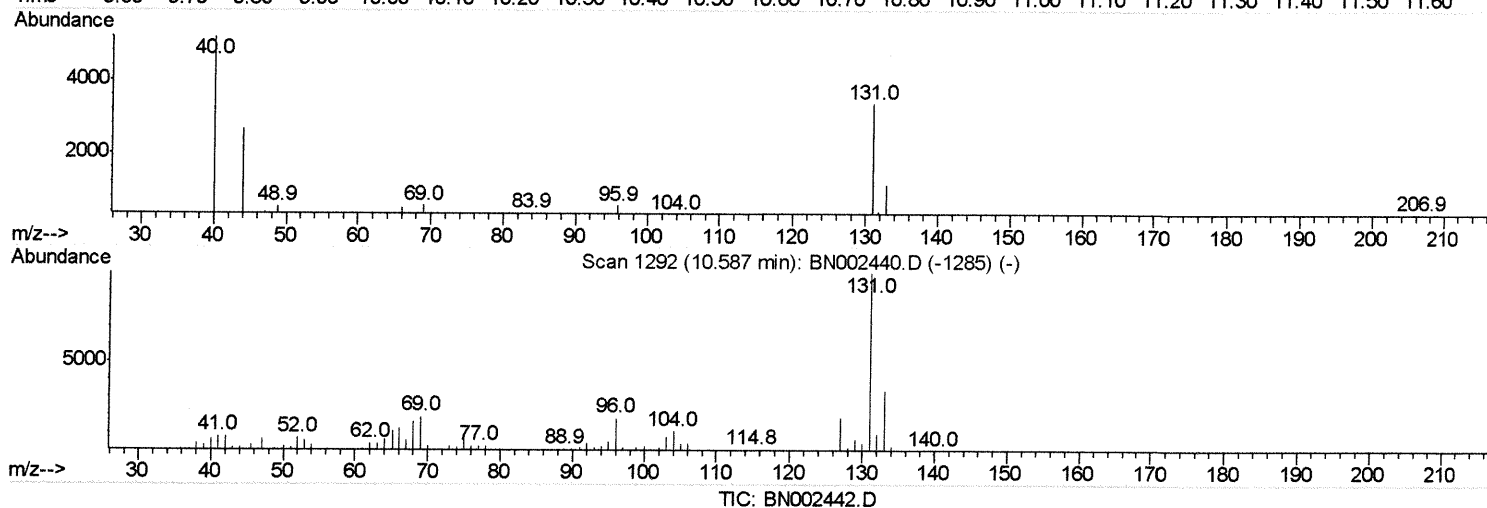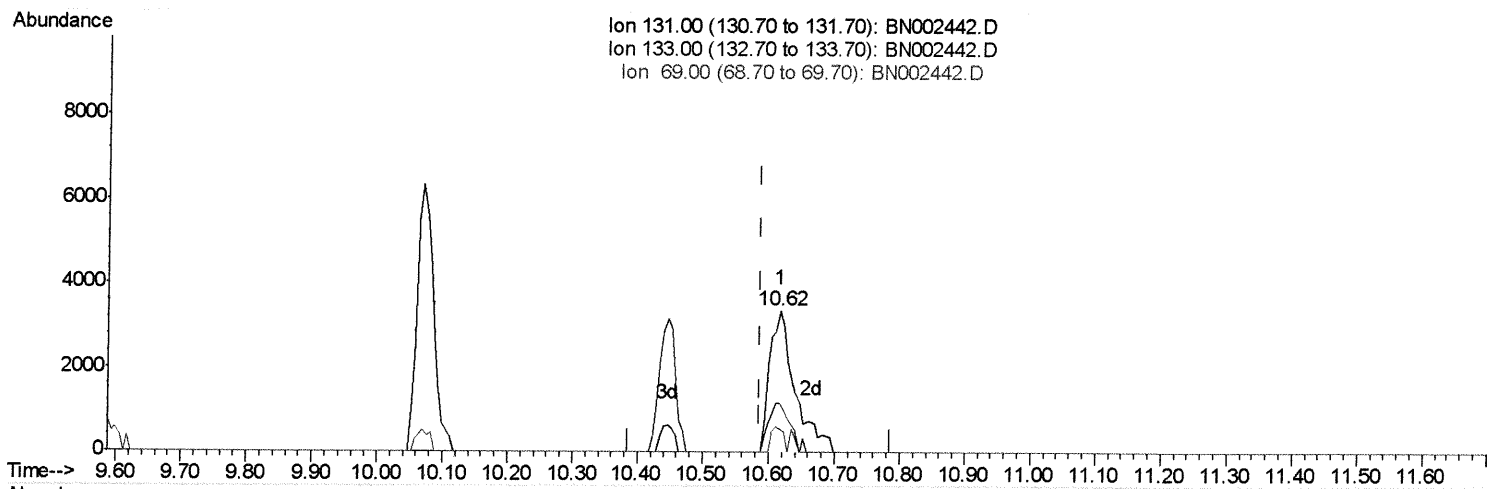

(29) 4-Chloroaniline-d4 (S)

10.616min (+0.029) 0.74ng/ul m

response 8986

Ion	Exp%	Act%
-----	------	------

131.00	100	100
--------	-----	-----

133.00	32.10	34.16
--------	-------	-------

69.00 16.20 16.53

0.00	0.00	0.00
------	------	------

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082018\
 Data File : BN002442.D
 Acq On : 21 Aug 2018 02:38
 Operator : JU/SJ
 Sample : J4514-12
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0341

Manual Integrations
 APPROVED

Sohil
 8/21/2018 4:47:43 PM

Quant Time: Aug 21 06:47:27 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 21 04:38:31 2018
 Response via : Initial Calibration

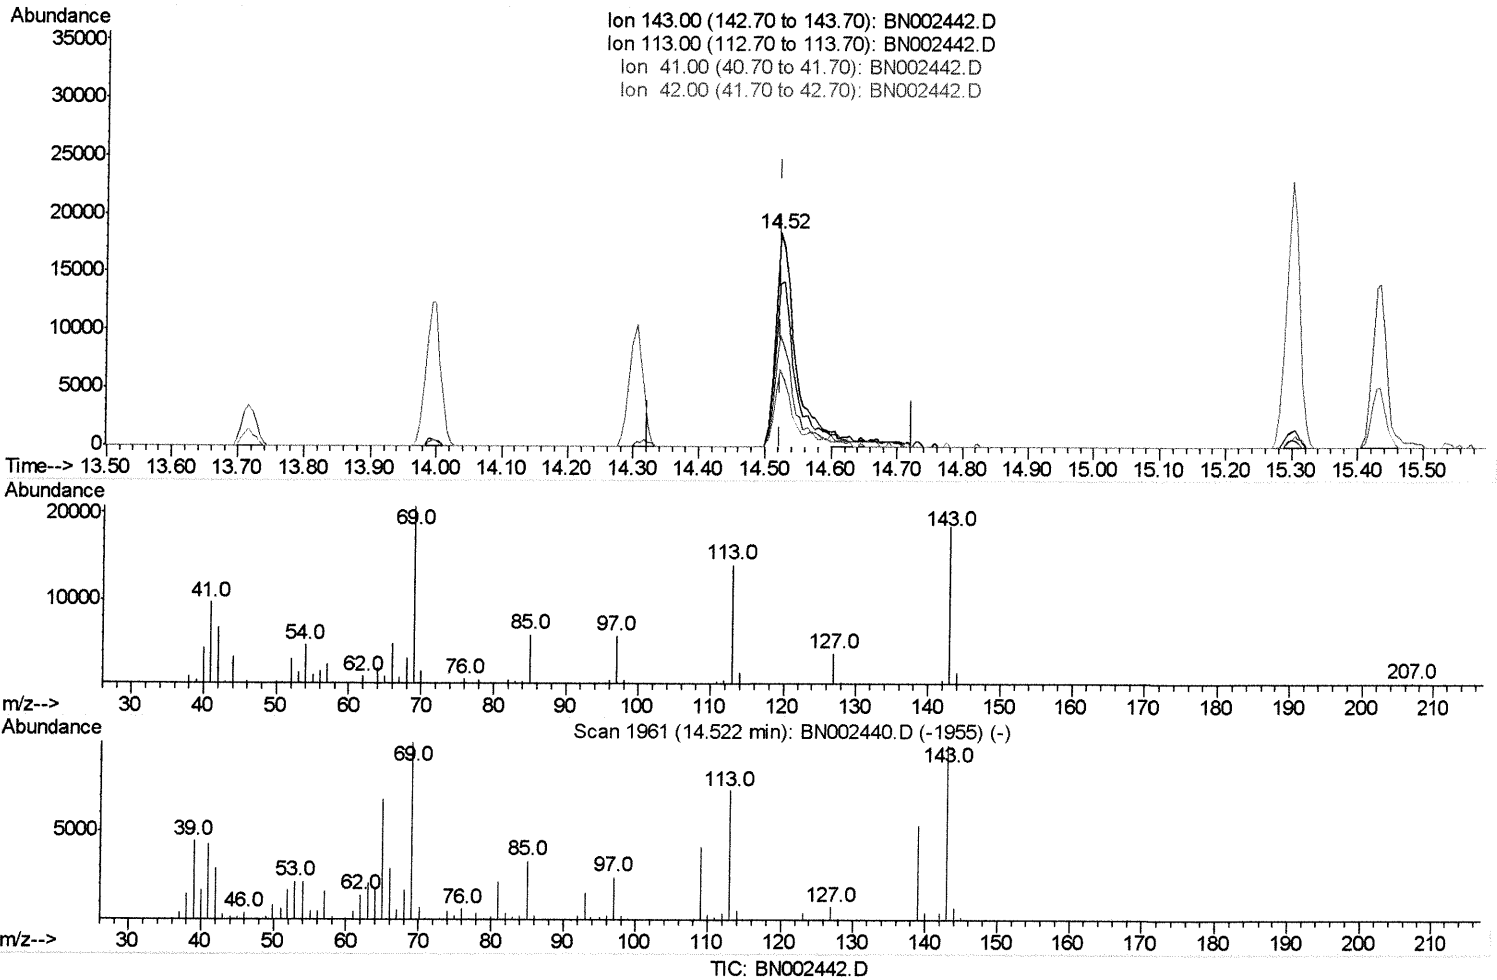

(51) 4-Nitrophenol-d4 (S)

14.522min (-0.000) 5.34ng/ul

response 38100

Ion	Exp%	Act%
143.00	100	100
113.00	75.10	76.21
41.00	28.80	52.40#
42.00	19.10	36.33#

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082018\
 Data File : BN002442.D
 Acq On : 21 Aug 2018 02:38
 Operator : JU/SJ
 Sample : J4514-12
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 C0341

Manual Integrations
 APPROVED

Sohil
 8/21/2018 4:47:43 PM

Quant Time: Aug 21 06:47:27 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 21 04:38:31 2018
 Response via : Initial Calibration

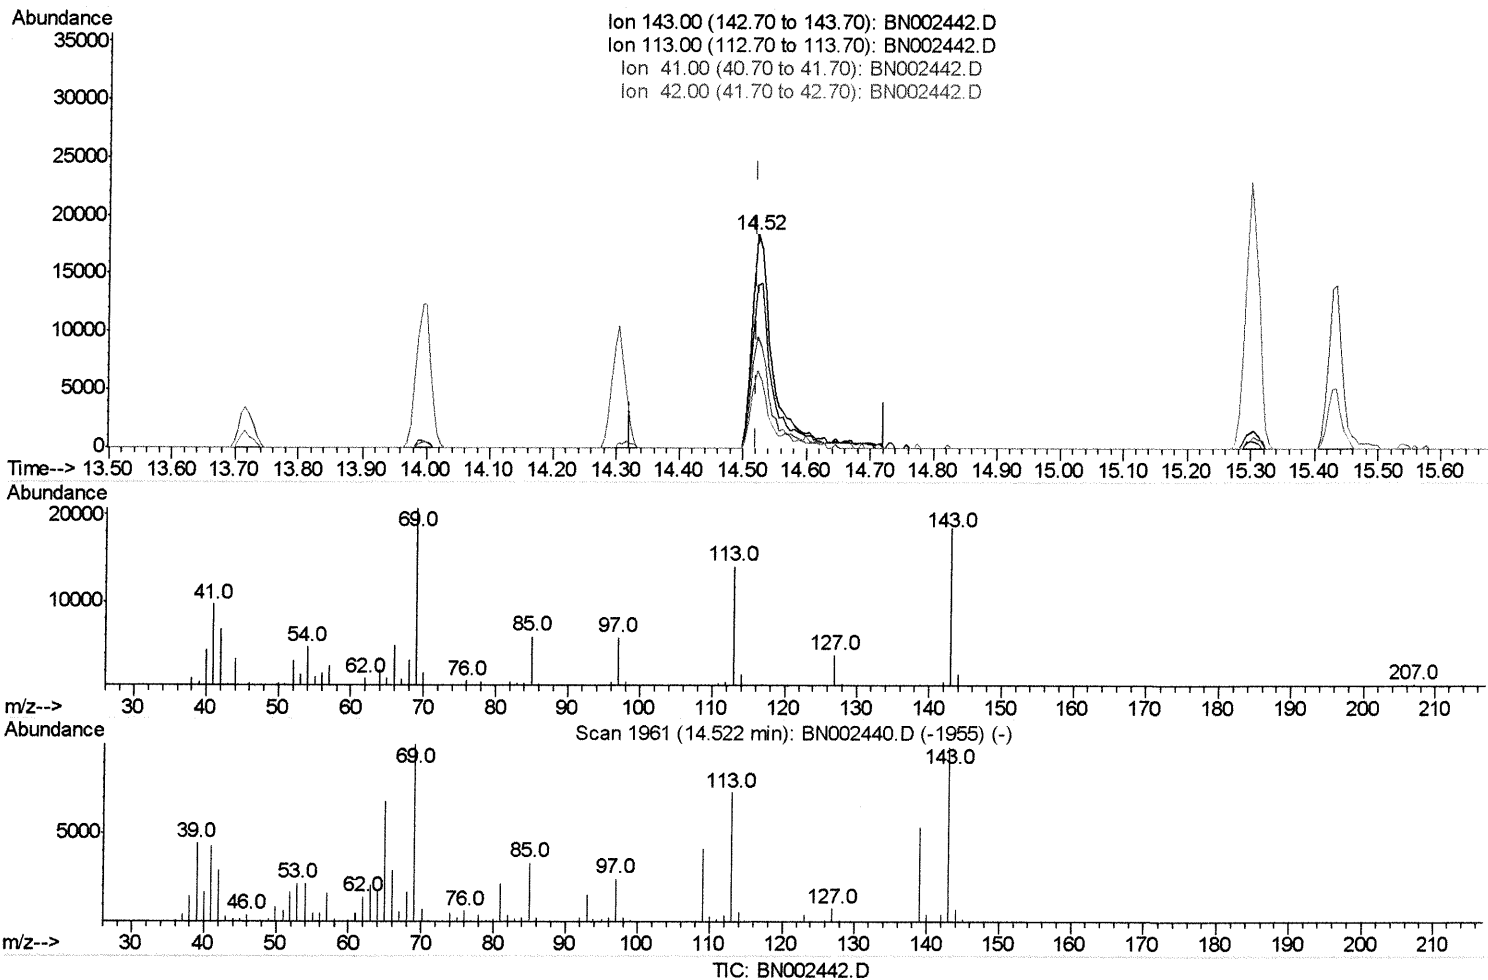

(51) 4-Nitrophenol-d4 (S)

14.522min (-0.000) 5.80ng/ul m

5/8/22/18

response 41402

Ion	Exp%	Act%
143.00	100	100
113.00	75.10	76.21
41.00	28.80	52.40#
42.00	19.10	36.33#

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082018\
 Data File : BN002442.D
 Acq On : 21 Aug 2018 02:38
 Operator : JU/SJ
 Sample : J4514-12
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0341

Manual Integrations
 APPROVED

Sohil
 8/21/2018 4:47:43 PM

Quant Time: Aug 21 06:52:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 21 04:38:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	152927	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	728099	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	455343	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	1089350	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1209491	20.00	ng/ul	0.00
85) Perylene-d12	23.47	264	1247911	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.24	96	20532	6.34	ng/uL	0.00
5) Phenol-d5	6.85	99	104568	7.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	298382	33.88	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	286838	26.86	ng/ul	0.00
13) 4-Methylphenol-d8	8.38	113	189116	16.87	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	191627	33.06	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	205498	33.72	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	322280	28.78	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	8986m	0.74	ng/ul	0.03
43) Dimethylphthalate-d6	13.72	166	1406048	37.25	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	1629091	35.18	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	41402m	5.80	ng/ul	0.00
57) Fluorene-d10	15.30	176	1211570	37.02	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	209326	30.18	ng/ul	0.00
70) Anthracene-d10	17.15	188	2057480	39.54	ng/ul	0.00
78) Pyrene-d10	19.45	212	2290843	39.58	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	2594602	39.76	ng/ul	0.00

SS 8/22/18
 SS 8/22/18

Target Compounds

Ovalue

2) 1,4-Dioxane	3.27	88	14869	4.290	ng/uL	94
----------------	------	----	-------	-------	-------	----

(#) = qualifier out of range (m) = manual integration (+) = signals summed