

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082018\
 Data File : BN002422.D
 Acq On : 20 Aug 2018 14:53
 Operator : JU/SJ
 Sample : J4491-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C01A4

Manual Integrations
 APPROVED

Sohil
 8/21/2018 4:46:55 PM

Quant Time: Aug 21 01:46:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 18 04:58:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	143079	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	693741	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	443450	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	1031185	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1147071	20.00	ng/ul	0.00
85) Perylene-d12	23.47	264	1210759	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.24	96	17596	5.81	ng/uL	0.00
5) Phenol-d5	6.85	99	106550	8.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	315408	38.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	304113	30.43	ng/ul	0.00
13) 4-Methylphenol-d8	8.38	113	210268	20.05	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	212268	38.44	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	223300	38.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	361250	33.85	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	11958m	1.04	ng/ul	0.02
43) Dimethylphthalate-d6	13.72	166	1450515	39.46	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	1798695	39.89	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	40459m	5.82	ng/ul	0.00
57) Fluorene-d10	15.30	176	1245879	39.09	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	213215	32.48	ng/ul	0.00
70) Anthracene-d10	17.15	188	2034773	41.30	ng/ul	0.00
78) Pyrene-d10	19.45	212	2279765	41.54	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	2494945	39.41	ng/ul	0.00

Target Compounds				Qvalue
2) 1,4-Dioxane	3.27	88	7368	2.272 ng/uL# 82

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082018\
Data File : BN002422.D
Acq On : 20 Aug 2018 14:53
Operator : JU/SJ
Sample : J4491-08
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C01A4

Quant Time: Aug 21 01:46:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 18 04:58:06 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
8/21/2018 4:46:55 PM

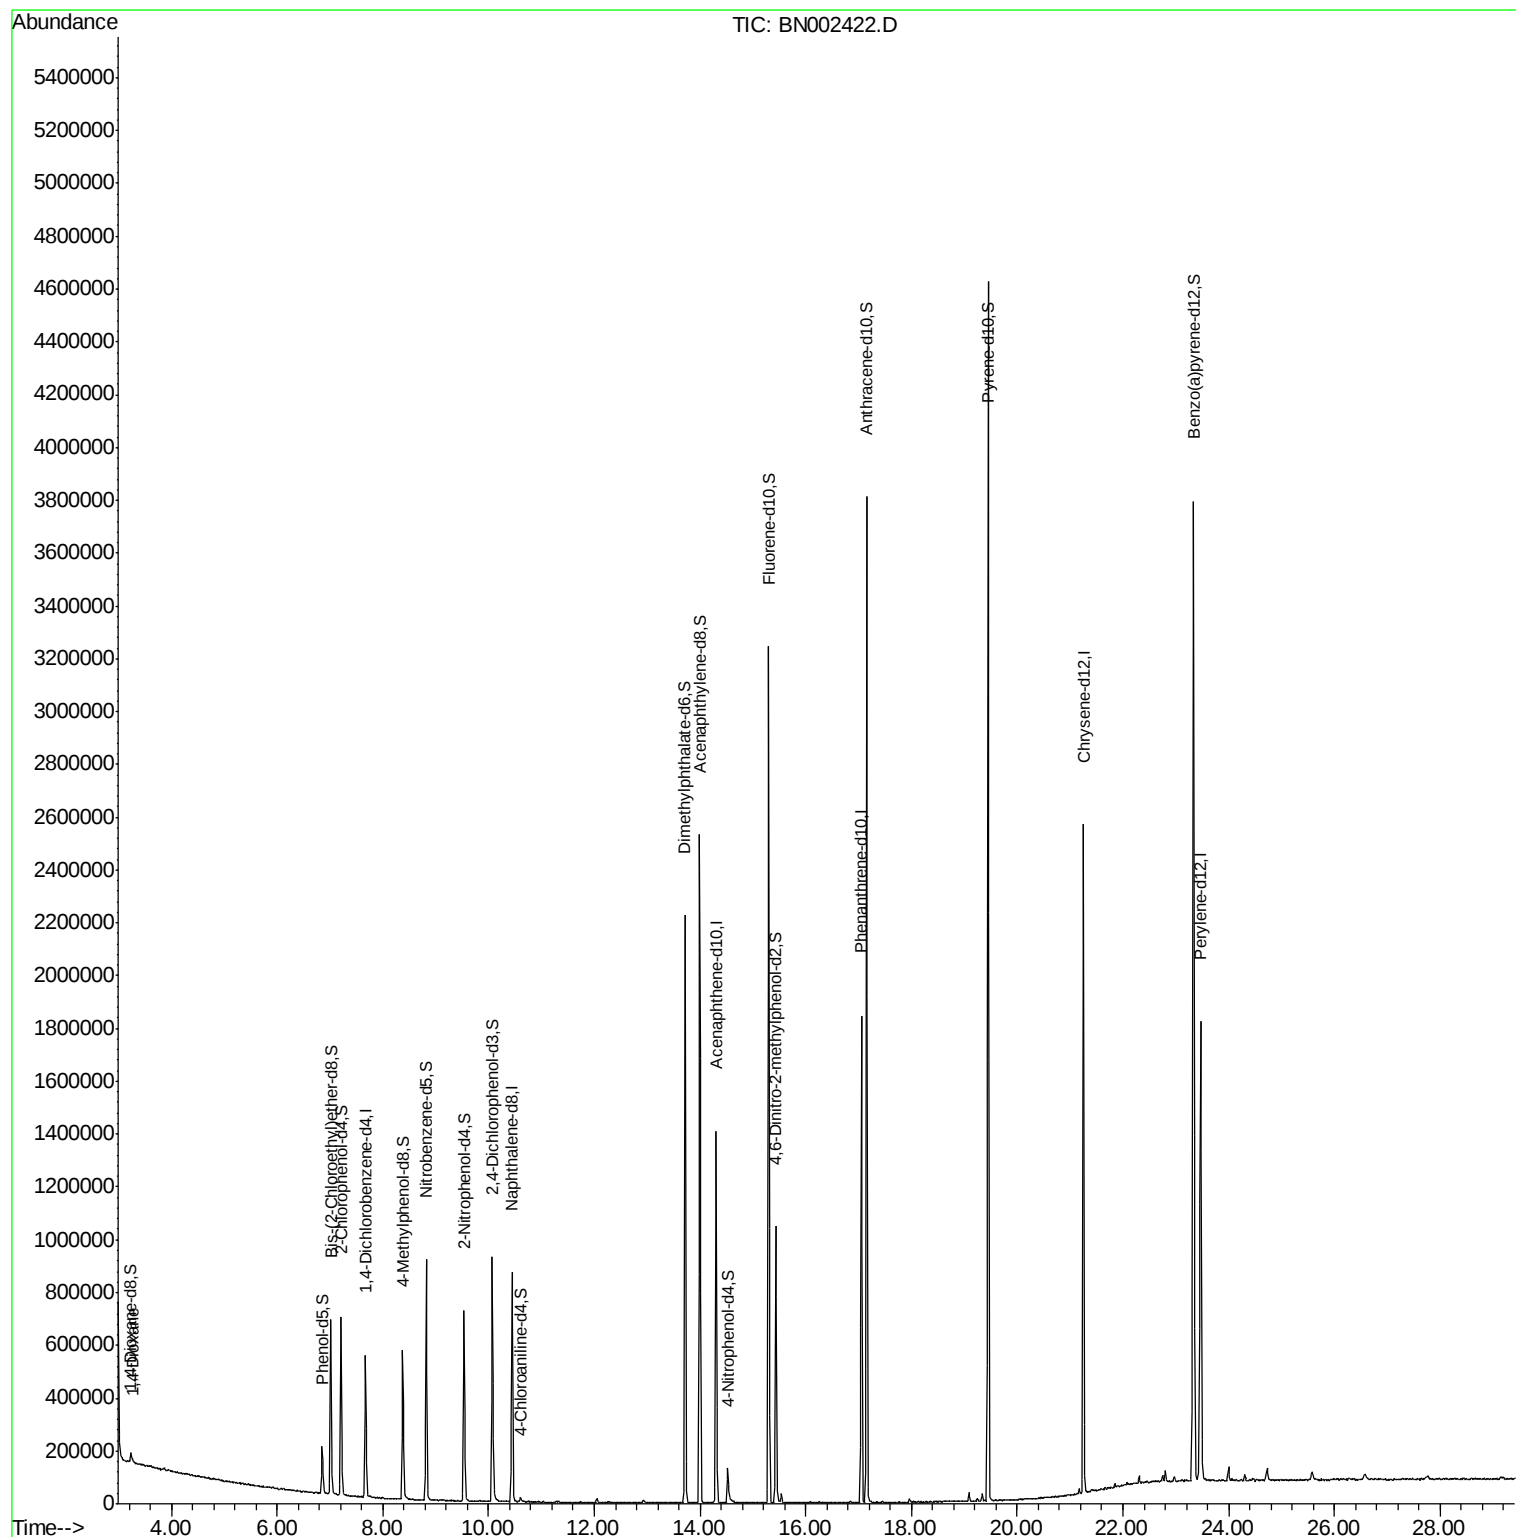

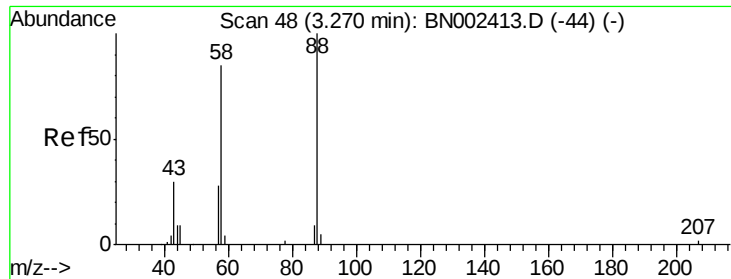

#2
 1,4-Dioxane
 Concen: 2.272 ng/uL
 RT: 3.27 min Scan# 48
 Delta R.T. -0.00 min
 Lab File: BN002422.D
 Acq: 20 Aug 2018 14:53

Instrument :
 BNA_N
 ClientSampleId :
 C01A4

Tgt Ion	Ratio	Lower	Upper
88	100		
43	48.8	32.0	48.0#
58	71.7	72.0	108.0#

Manual Integrations
 APPROVED

Sohil
 8/21/2018 4:46:55 PM

