
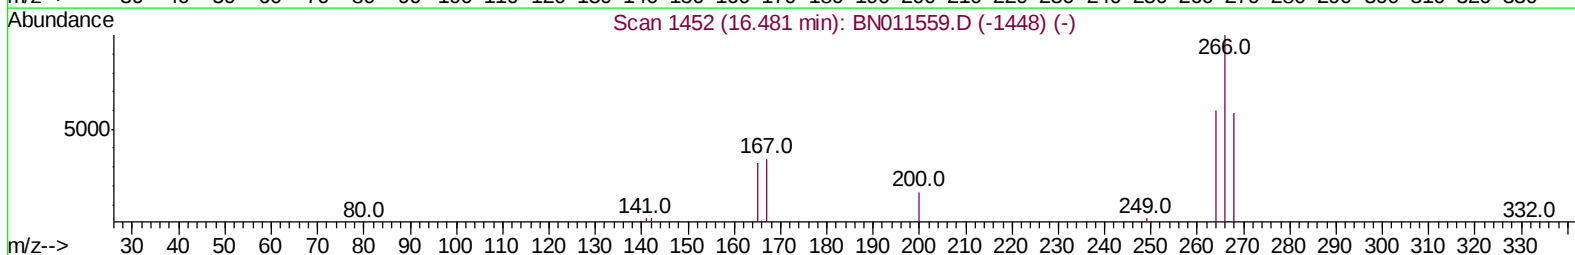
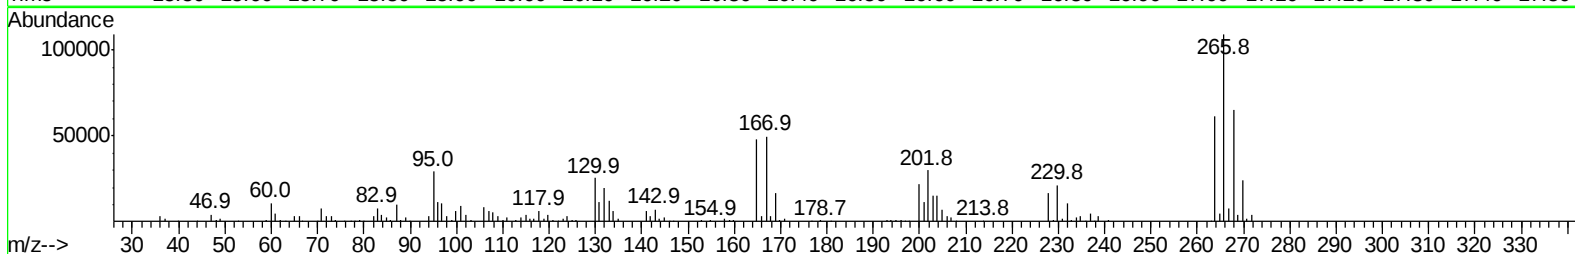


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082120\
 Data File : BN011585.D
 Acq On : 22 Aug 2020 13:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Quant Time: Aug 24 02:03:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN082120.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 22 04:52:07 2020
 Response via : Initial Calibration

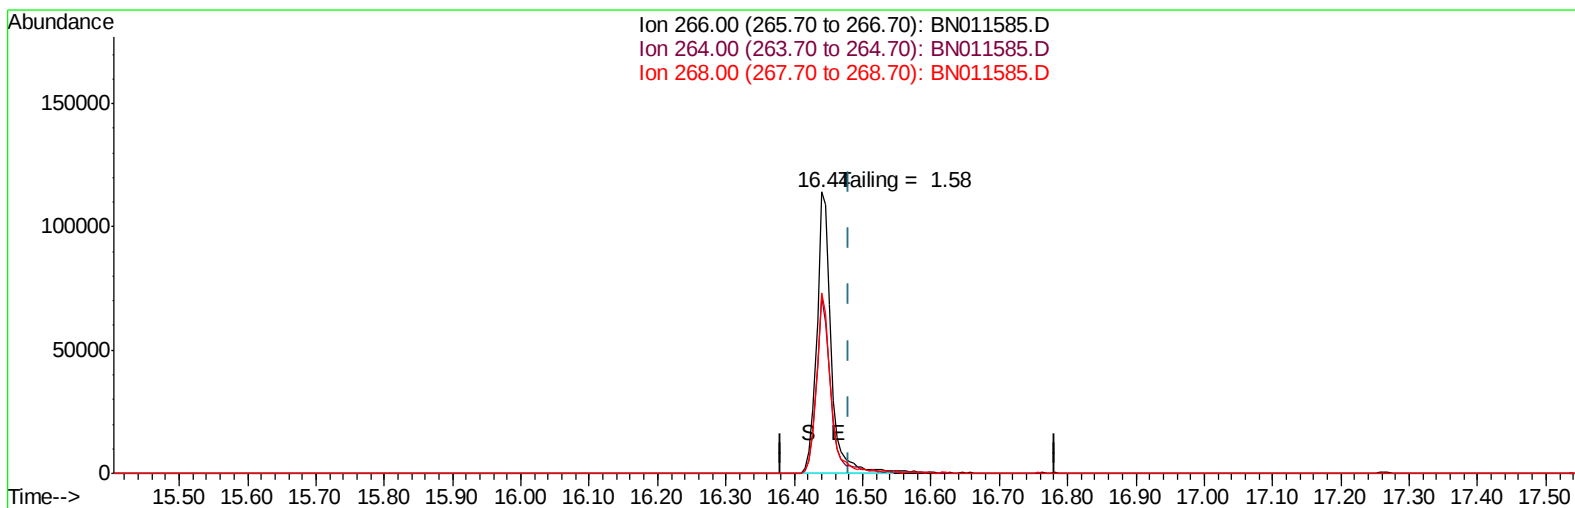

TIC: BN011585.D

(24) Pentachlorophenol

16.439min (-0.042) 0.00ng

response 166938

Ion	Exp%	Act%
266.00	100	100
264.00	60.90	63.10
268.00	63.80	64.41
0.00	0.00	0.00