


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082120\
 Data File : BN011556.D
 Acq On : 21 Aug 2020 15:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082120.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 22 04:52:07 2020

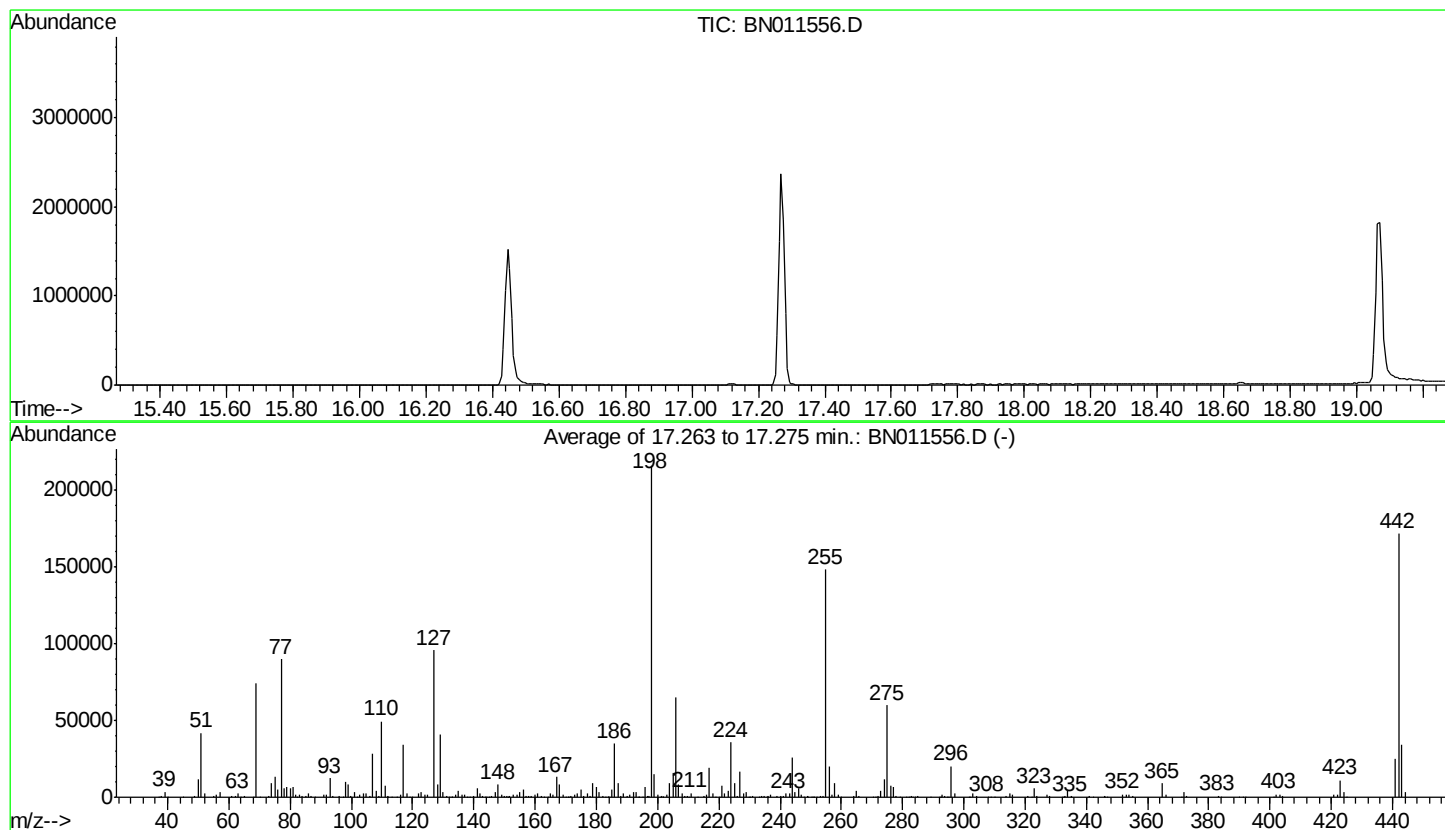

AutoFind: Scans 2427, 2428, 2429; Background Corrected with Scan 2421

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.3	41778	PASS
68	69	0.00	2	0.5	368	PASS
69	198	0.00	100	34.4	74290	PASS
70	69	0.00	2	0.6	442	PASS
127	198	10	80	44.4	95986	PASS
197	198	0.00	2	0.4	801	PASS
198	198	100	100	100.0	216213	PASS
199	198	5	9	6.8	14775	PASS
275	198	10	60	27.6	59746	PASS
365	198	1	100	4.2	9017	PASS
441	198	0.01	100	11.7	25262	PASS
442	198	50	100	79.4	171578	PASS
443	442	15	24	19.7	33832	PASS