


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082120\
 Data File : BN011585.D
 Acq On : 22 Aug 2020 13:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082120.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 22 04:52:07 2020

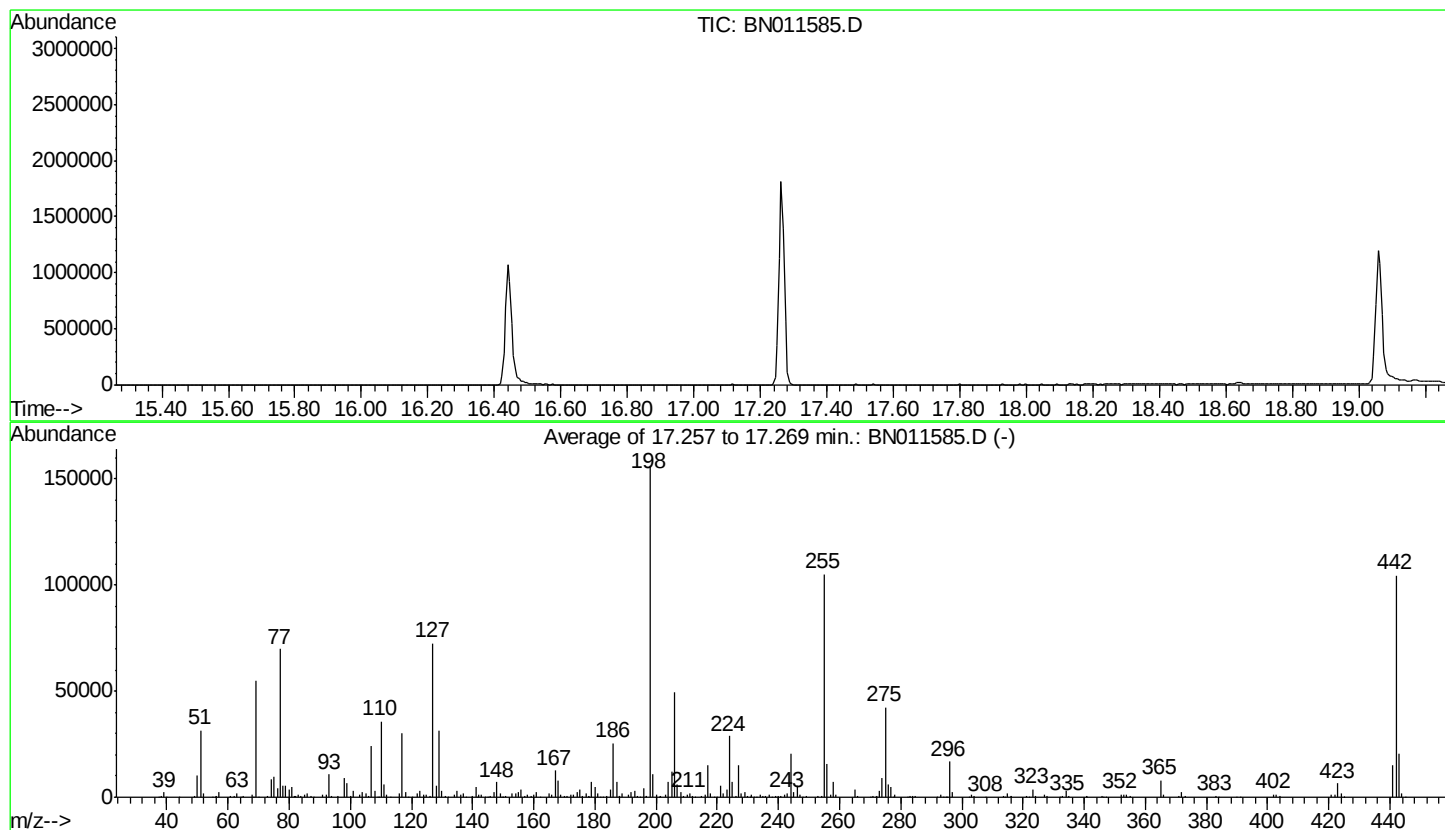

AutoFind: Scans 2426, 2427, 2428; Background Corrected with Scan 2420

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.2	31533	PASS
68	69	0.00	2	1.9	1032	PASS
69	198	0.00	100	35.3	55106	PASS
70	69	0.00	2	0.5	286	PASS
127	198	10	80	46.4	72517	PASS
197	198	0.00	2	0.3	394	PASS
198	198	100	100	100.0	156181	PASS
199	198	5	9	7.2	11169	PASS
275	198	10	60	27.0	42226	PASS
365	198	1	100	5.2	8087	PASS
441	198	0.01	100	9.6	15069	PASS
442	198	50	100	66.9	104509	PASS
443	442	15	24	19.5	20416	PASS