

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
 Data File : BN026987.D
 Acq On : 21 Aug 2023 11:33
 Operator : MA/JU
 Sample : PB154935BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK935

Quant Time: Aug 22 01:37:53 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 18 13:11:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.101	152	7157	0.400	ng/ul	0.00
4) Naphthalene-d8	10.927	136	24354	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.726	164	13978	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.473	188	30422	0.400	ng/ul	0.00
17) Chrysene-d12	21.650	240	21227	0.400	ng/ul	0.00
23) Perylene-d12	24.190	264	22138	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.435	96	49940	5.878	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.500	152	11469	0.320	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	27271	0.407	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.721	166	4337	0.071	ng/ul#	13
20) Pyrene	19.859	202	4927	0.052	ng/ul#	1
26) Benzo(a)pyrene	24.024	252	7934	0.105	ng/ul#	35


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
Data File : BN026987.D
Acq On : 21 Aug 2023 11:33
Operator : MA/JU
Sample : PB154935BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK935

Quant Time: Aug 22 01:37:53 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 18 13:11:26 2023
Response via : Initial Calibration




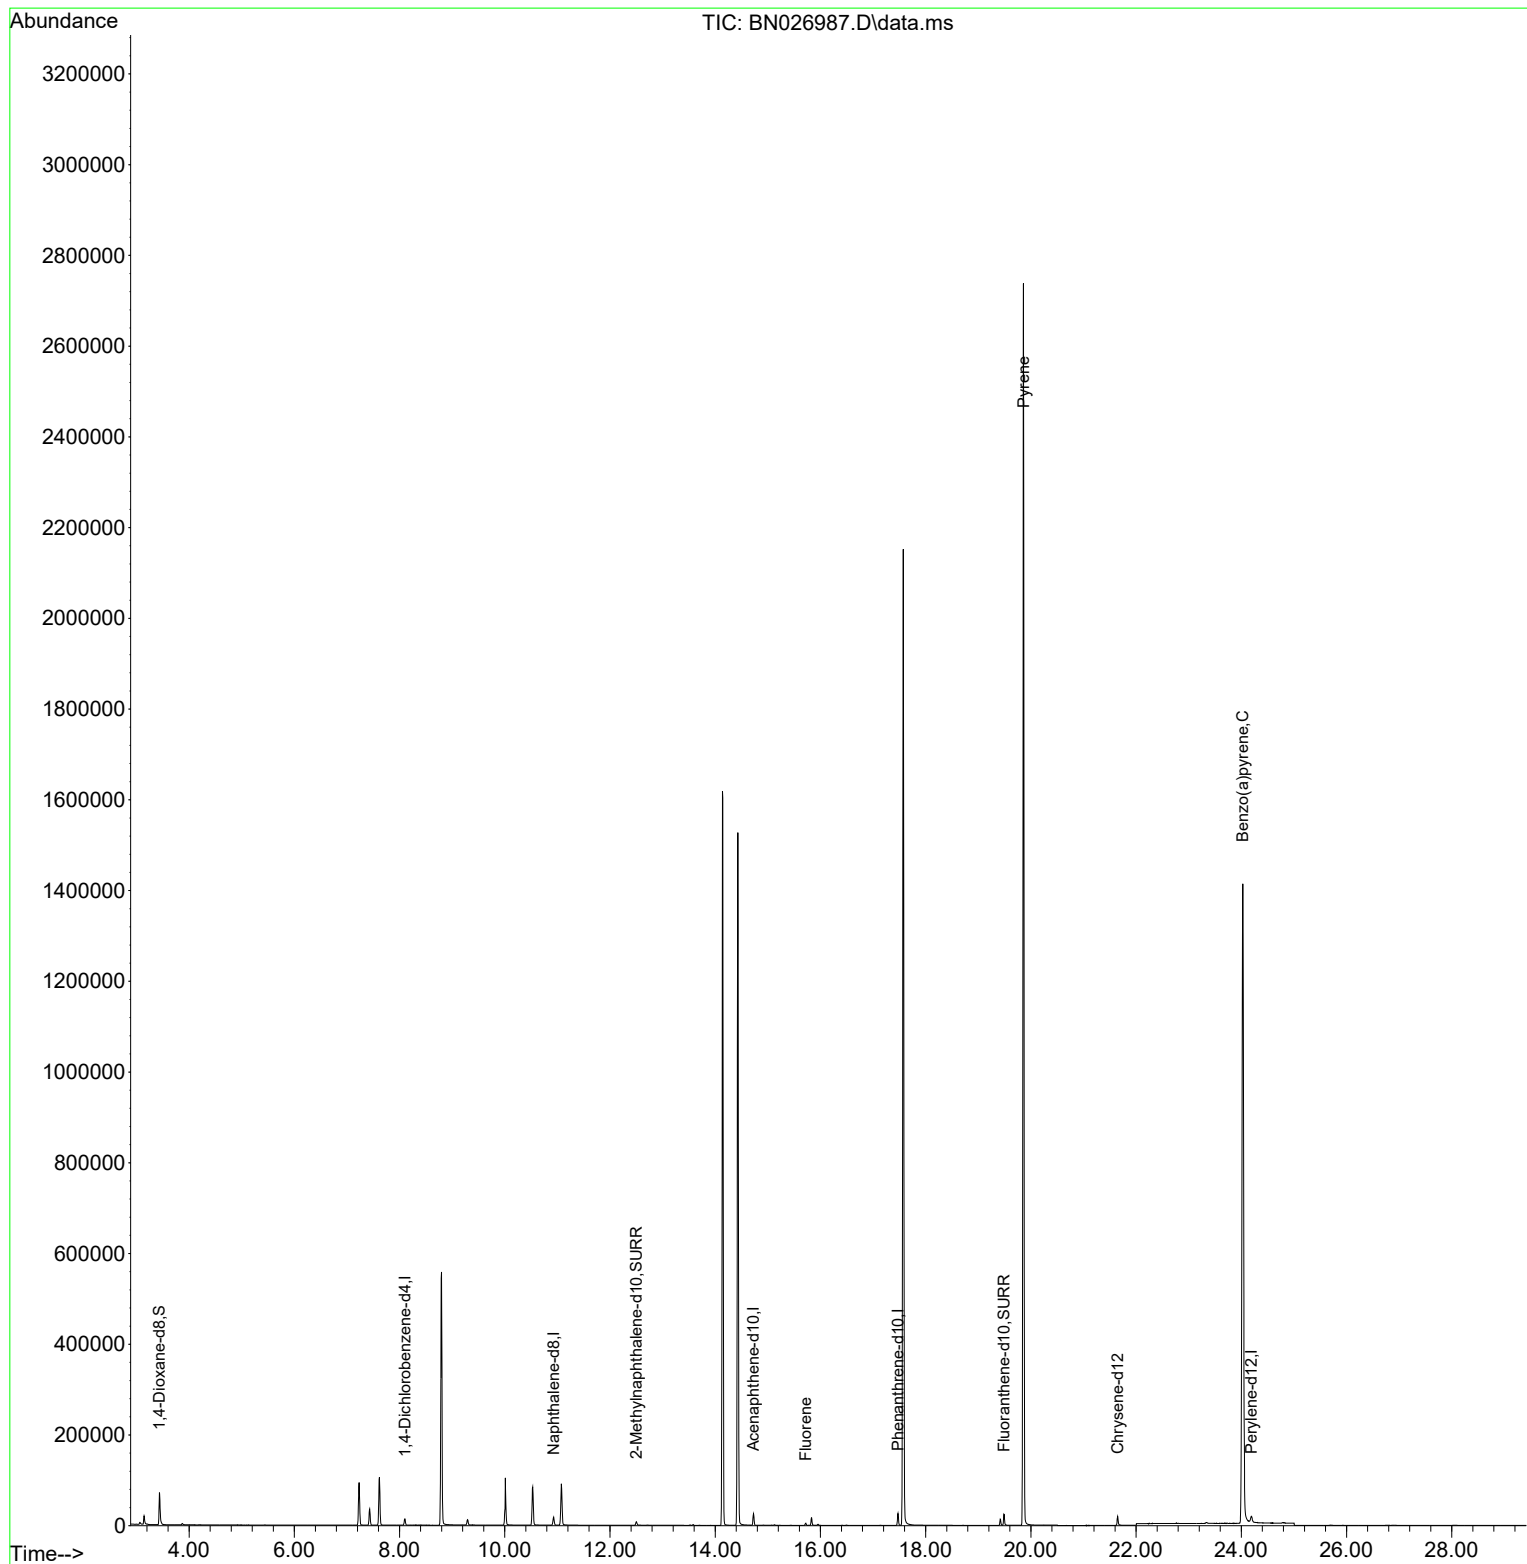


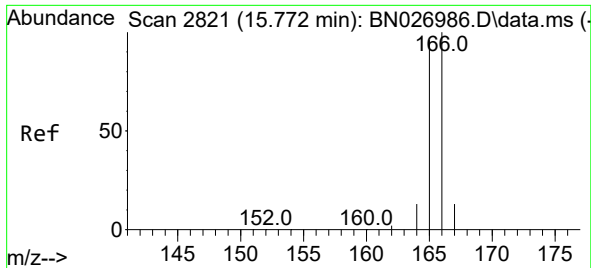

#12
Fluorene
Concen: 0.071 ng/ul
RT: 15.721 min Scan# 21
Delta R.T. -0.051 min
Lab File: BN026987.D
Acq: 21 Aug 2023 11:33




Instrument :
BNA_N
ClientSampleId :
SBLK935


Tgt Ion:166 Resp: 4337
Ion Ratio Lower Upper
166 100
165 7.7 79.1 118.7#
167 37.1 11.4 17.0#

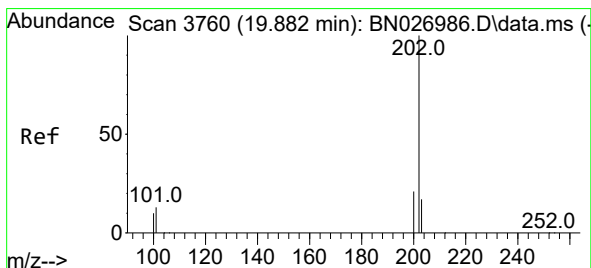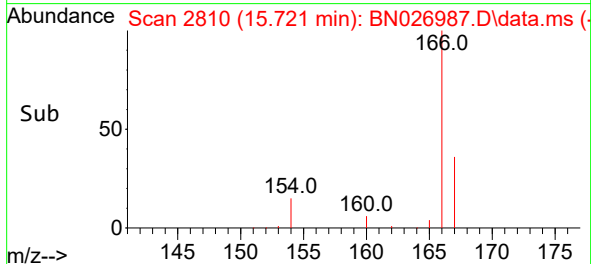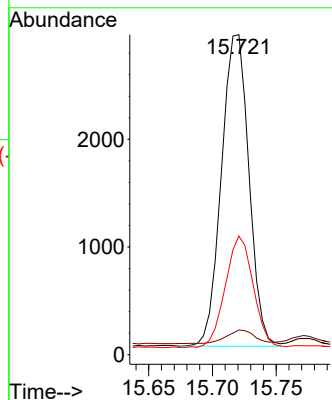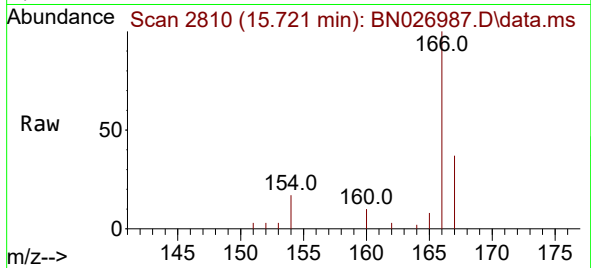

#20
Pyrene
Concen: 0.052 ng/ul
RT: 19.859 min Scan# 3755
Delta R.T. -0.028 min
Lab File: BN026987.D
Acq: 21 Aug 2023 11:33


Tgt Ion:202 Resp: 4927
Ion Ratio Lower Upper
202 100
101 149.1 10.7 16.1#
100 1083.5 8.5 12.7#

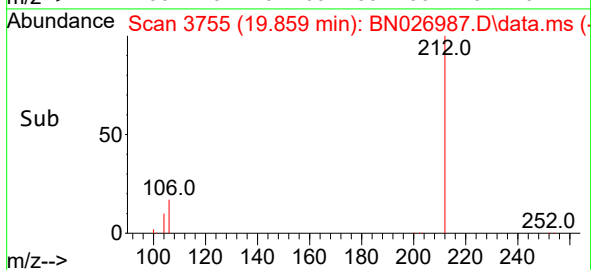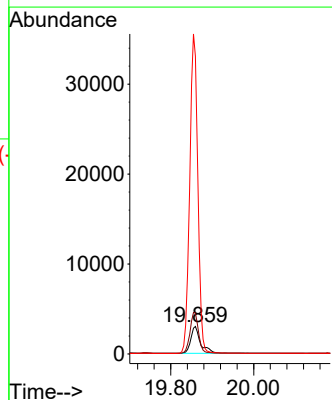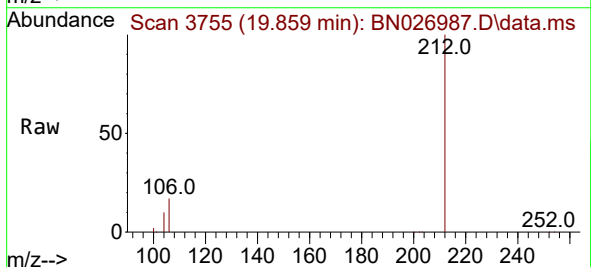

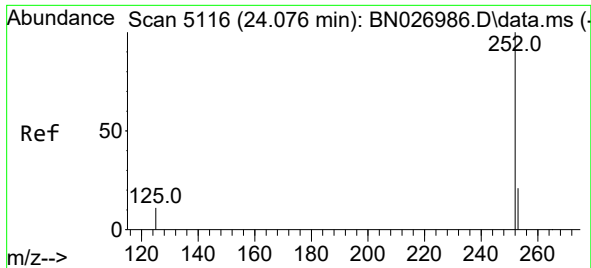

#26
Benzo(a)pyrene
Concen: 0.105 ng/ul
RT: 24.024 min Scan# 5098
Delta R.T. -0.061 min
Lab File: BN026987.D
Acq: 21 Aug 2023 11:33

Instrument :
BNA_N
ClientSampleId :
SBLK935

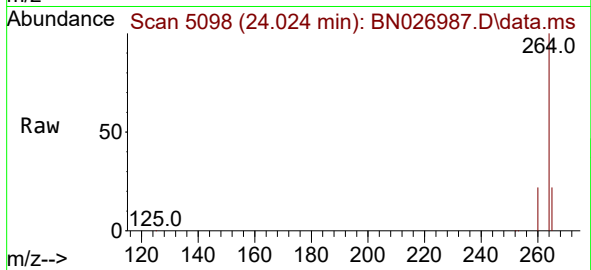

Tgt Ion:252 Resp: 7934
Ion Ratio Lower Upper
252 100
253 41.5 19.0 28.6#
125 60.9 11.4 17.0#

