

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
 Data File : BN026999.D
 Acq On : 21 Aug 2023 19:39
 Operator : MA/JU
 Sample : PB154792BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK792

Quant Time: Aug 22 01:39:53 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 18 13:11:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.101	152	8058	0.400	ng/ul	0.00
4) Naphthalene-d8	10.927	136	26930	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.731	164	15387	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.472	188	34282	0.400	ng/ul	0.00
17) Chrysene-d12	21.647	240	24638	0.400	ng/ul	0.00
23) Perylene-d12	24.193	264	26199	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.439	96	44619	4.664	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.500	152	10379	0.262	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	24239	0.312	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.859	202	4366	0.040	ng/ul#	1
26) Benzo(a)pyrene	24.024	252	7218	0.081	ng/ul#	43


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
Data File : BN026999.D
Acq On : 21 Aug 2023 19:39
Operator : MA/JU
Sample : PB154792BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK792

Quant Time: Aug 22 01:39:53 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 18 13:11:26 2023
Response via : Initial Calibration

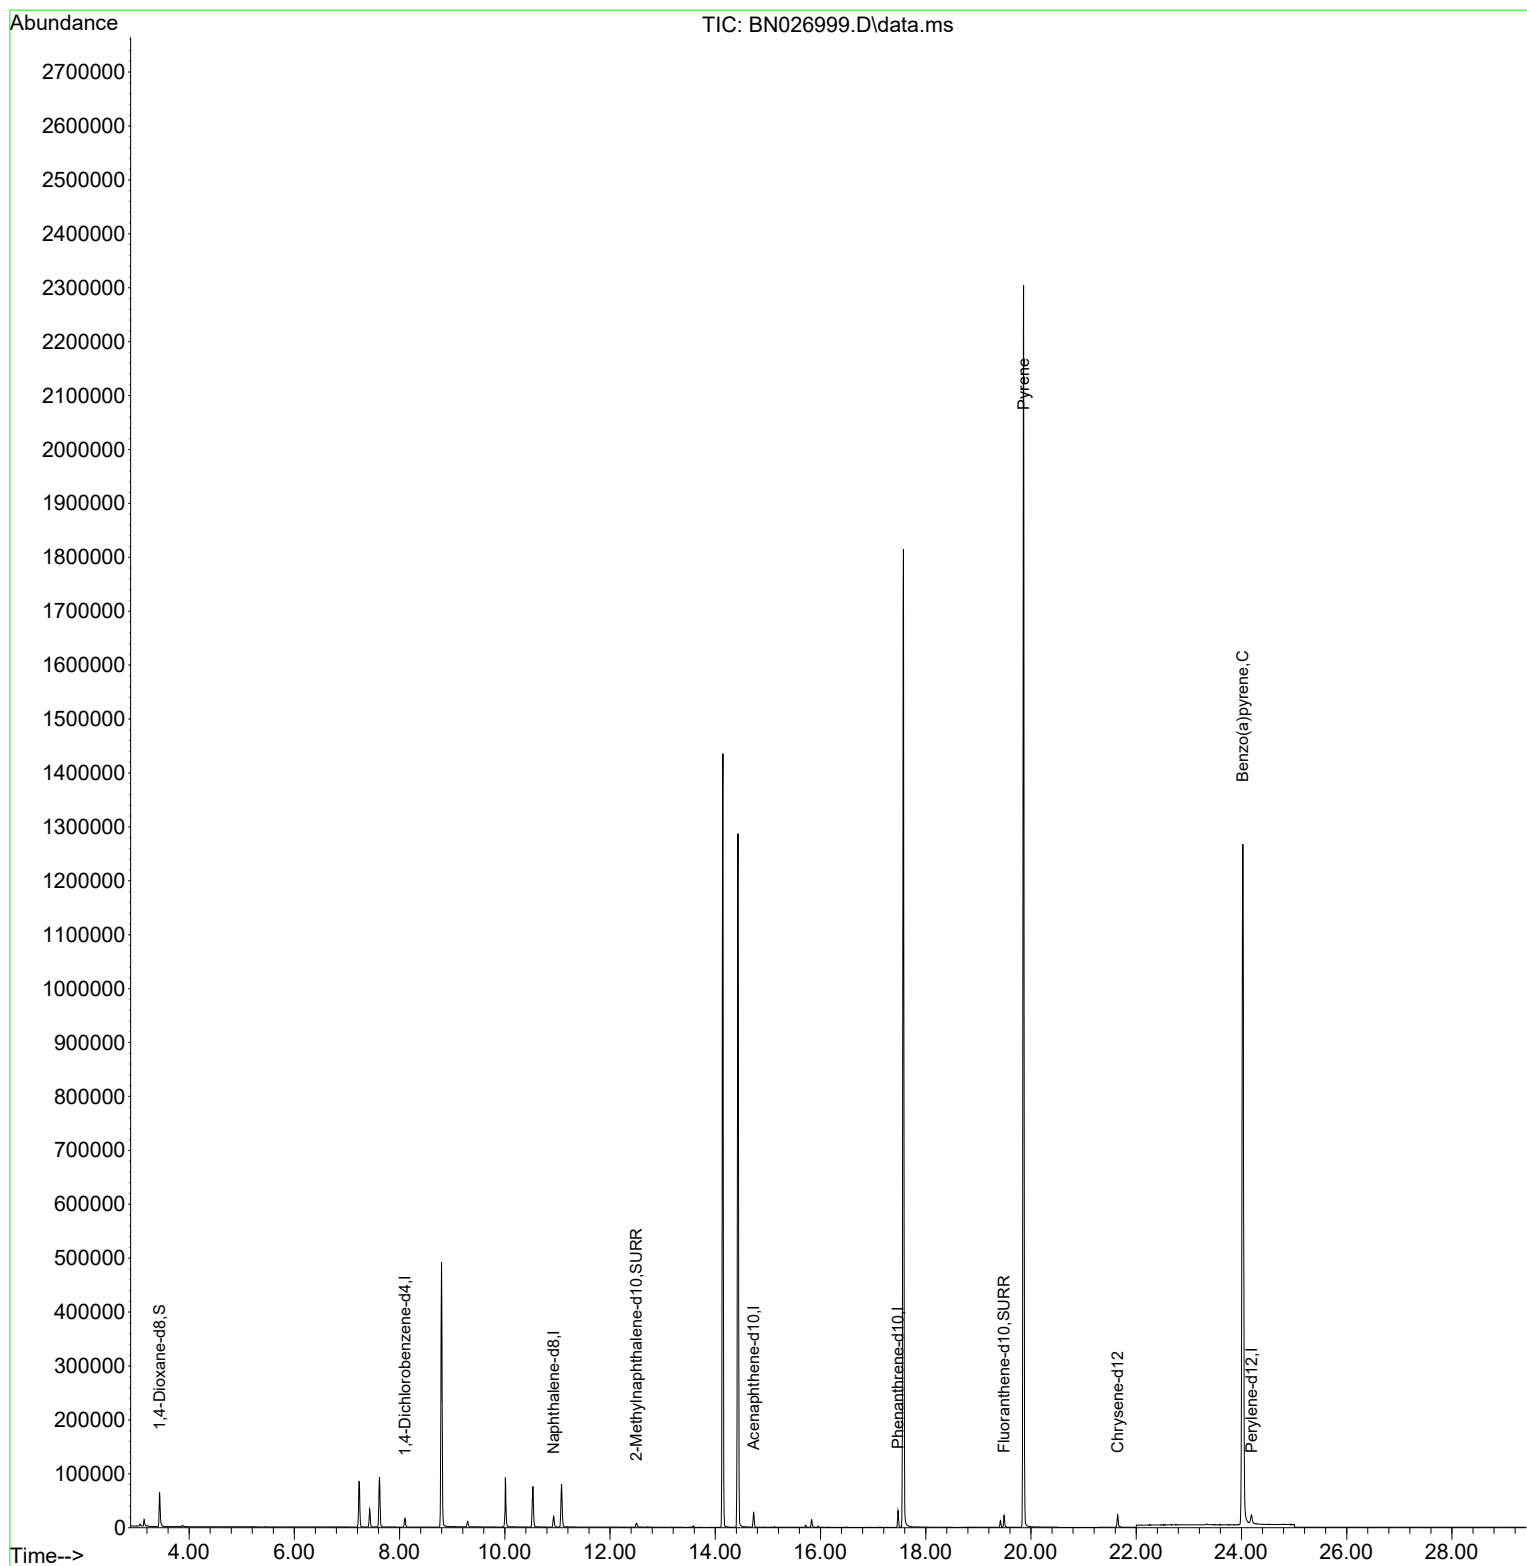

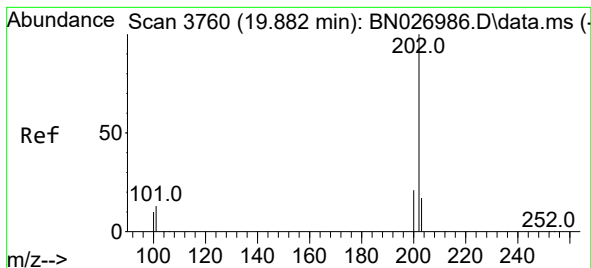

#20

Pyrene

Concen: 0.040 ng/ul

RT: 19.859 min Scan# 31

Delta R.T. -0.028 min

Lab File: BN026999.D

Acq: 21 Aug 2023 19:39

Instrument :

BNA_N

ClientSampleId :

SBLK792





Tgt Ion:202 Resp: 4366

Ion Ratio Lower Upper

202 100

101 148.9 10.7 16.1#

100 1062.5 8.5 12.7#

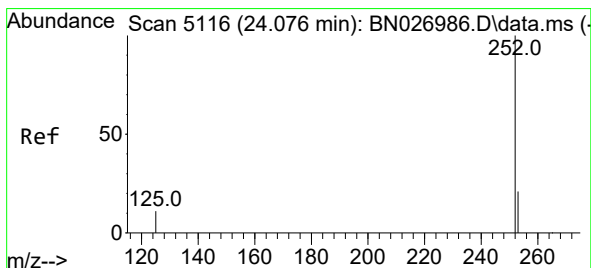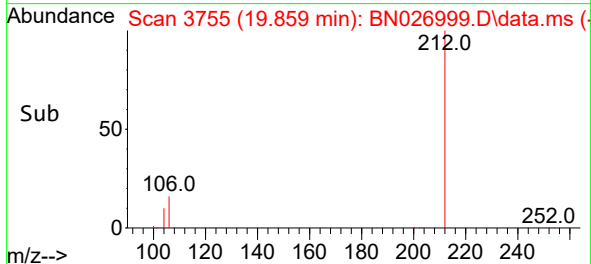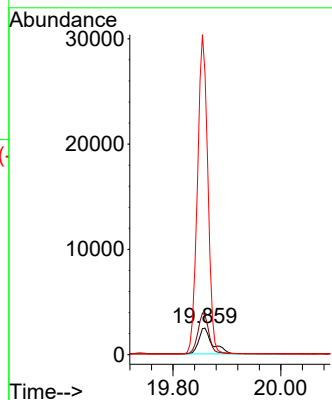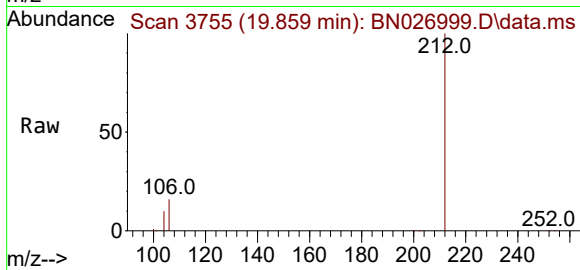

#26

Benzo(a)pyrene

Concen: 0.081 ng/ul

RT: 24.024 min Scan# 5098

Delta R.T. -0.061 min

Lab File: BN026999.D

Acq: 21 Aug 2023 19:39

Tgt Ion:252 Resp: 7218

Ion Ratio Lower Upper

252 100

253 42.7 19.0 28.6#

125 50.0 11.4 17.0#

